

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010284.D
 Acq On : 27 May 2017 20:20
 Operator : SJ/MA
 Sample : I3162-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSL0

Quant Time: May 29 05:34:03 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 27 15:01:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	360830	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	1293026	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	766218	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.31	188	1801169	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	2531061	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	2709263	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	45579	5.18	ng/uL	0.00
5) Phenol-d5	7.12	99	726180	26.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.27	67	412665	26.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.47	132	591839	27.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	566334	25.67	ng/ul	0.00
19) Nitrobenzene-d5	9.12	128	266871	28.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.83	143	308909	28.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	590453	26.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	476987	21.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.98	166	1986148	31.20	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	2250375	30.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	249647	26.21	ng/ul	0.00
57) Fluorene-d10	15.55	176	1675284	29.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	320619	25.13	ng/ul	0.00
70) Anthracene-d10	17.40	188	2714460	30.97	ng/ul	0.00
76) Pyrene-d10	19.69	212	3477863	33.23	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.67	264	4019458	31.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.02	163	489604	7.82	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010284.D
Acq On : 27 May 2017 20:20
Operator : SJ/MA
Sample : I3162-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSL0

Quant Time: May 29 05:34:03 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 27 15:01:38 2017
Response via : Initial Calibration

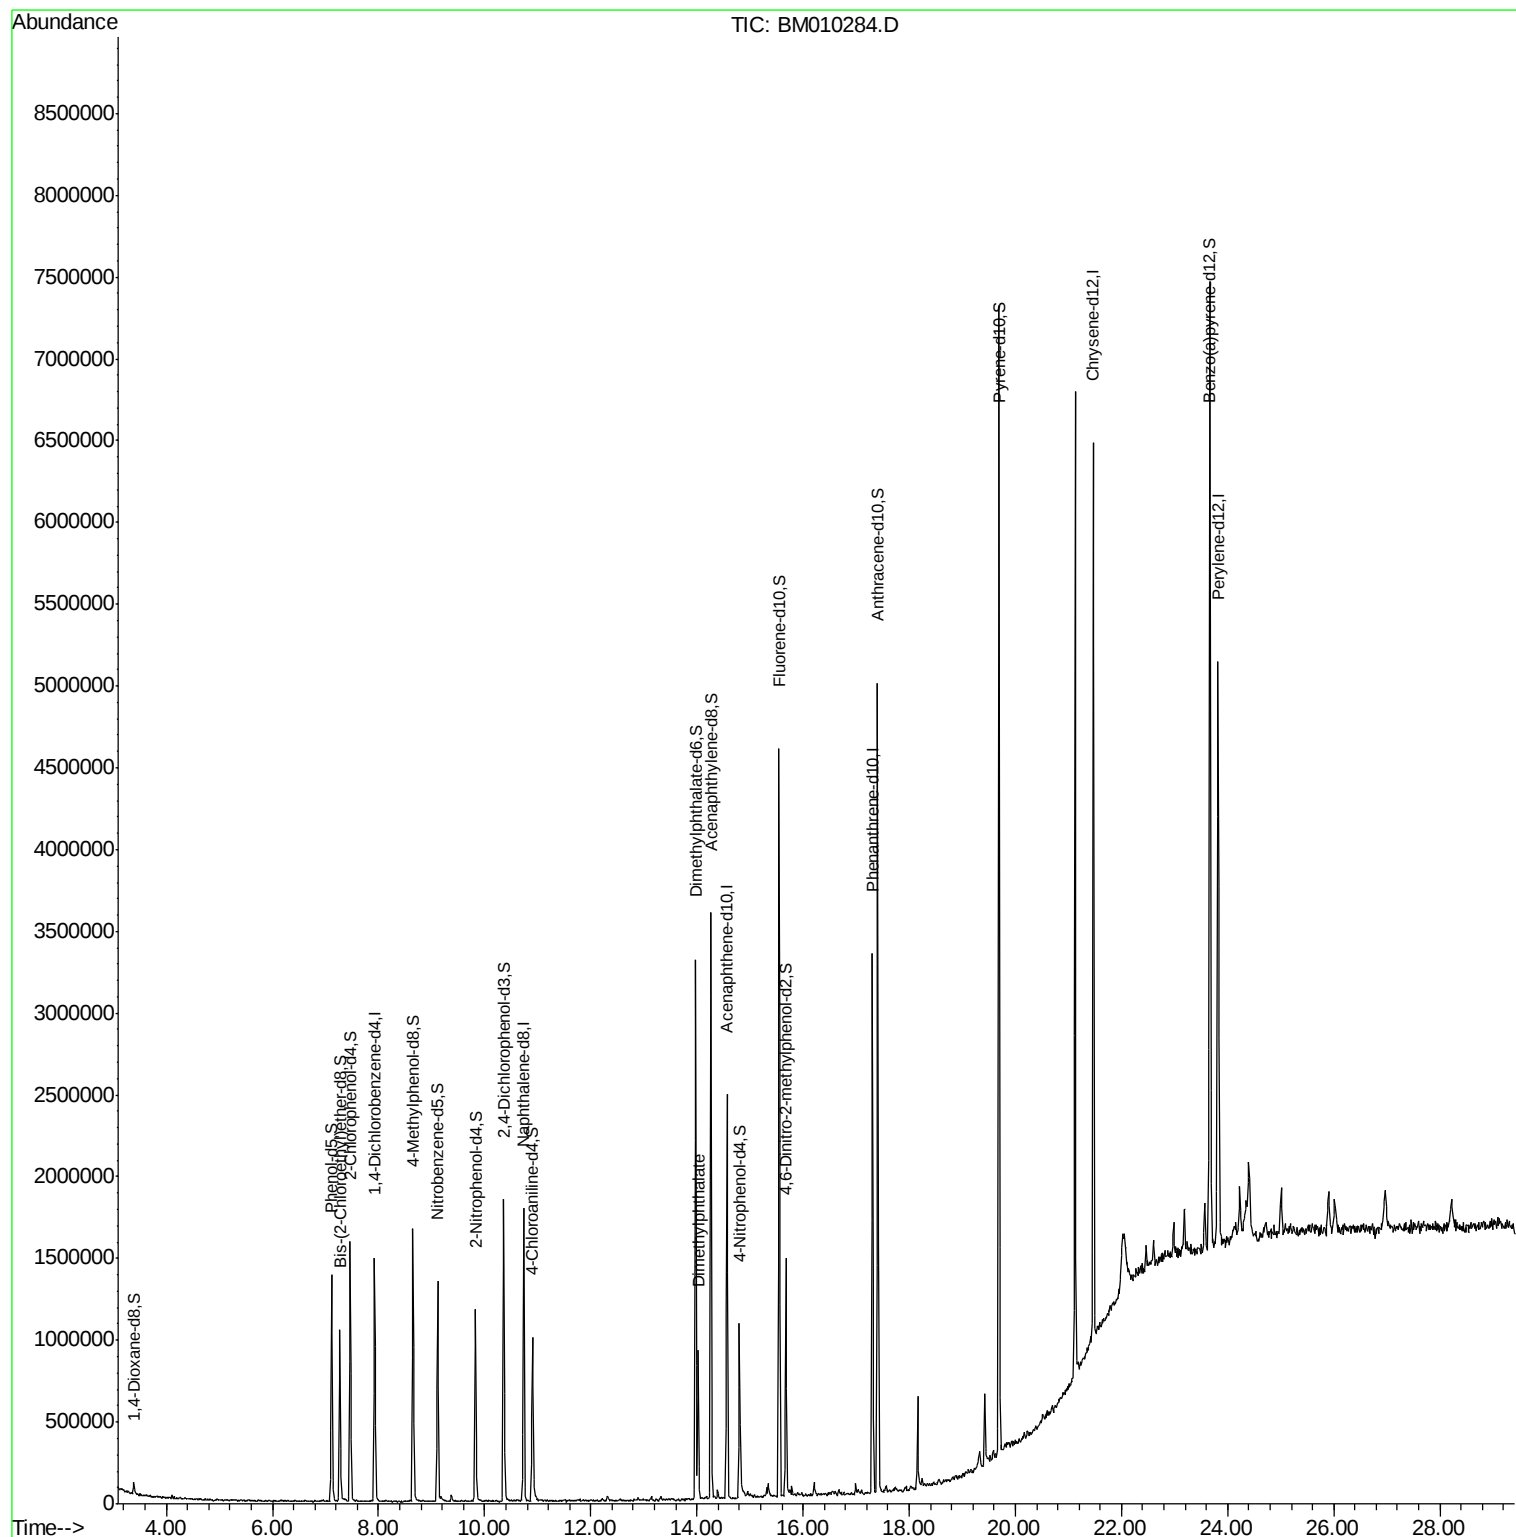

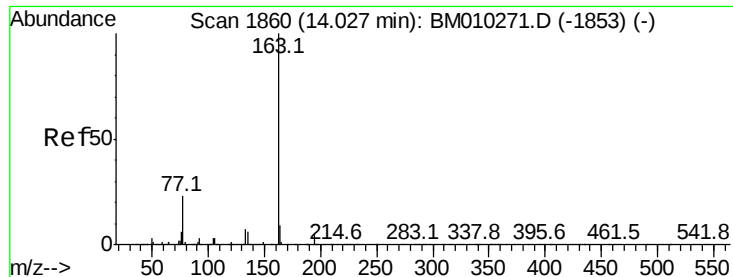

#44

Dimethylphthalate

Concen: 7.82 ng/ul

RT: 14.02 min Scan# 1859

Delta R.T. -0.01 min

Lab File: BM010284.D

Acq: 27 May 2017 20:20

Instrument :

BNA_M

ClientSampleId :

JHSL0


Tot Ion:163 Resp: 489604

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 11.3 8.2 12.4

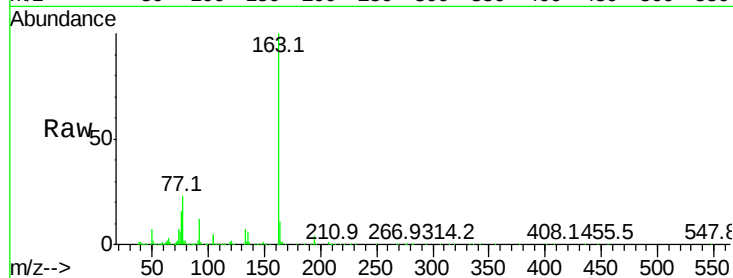

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

