

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010291.D
 Acq On : 28 May 2017 00:32
 Operator : SJ/MA
 Sample : I3162-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSE9

Quant Time: May 29 06:53:18 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 29 06:51:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	413702	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	1470250	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	894684	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.31	188	2150147	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	3093144	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	3196179	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	30411	3.02	ng/uL	0.00
5) Phenol-d5	7.12	99	645285	20.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.27	67	369999	21.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.47	132	545776	21.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	540677	21.38	ng/ul	0.00
19) Nitrobenzene-d5	9.12	128	258090	23.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.83	143	295671	23.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	584006	22.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	354031	14.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1953218	26.28	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	2236806	25.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	269678	24.25	ng/ul	0.00
57) Fluorene-d10	15.55	176	1658341	25.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	339189	22.27	ng/ul	0.00
70) Anthracene-d10	17.40	188	2672134	25.54	ng/ul	0.00
76) Pyrene-d10	19.69	212	3503676	27.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.67	264	3974638	26.71	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.02	163	660581	9.04	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010291.D
Acq On : 28 May 2017 00:32
Operator : SJ/MA
Sample : I3162-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSE9

Quant Time: May 29 06:53:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 29 06:51:20 2017
Response via : Initial Calibration

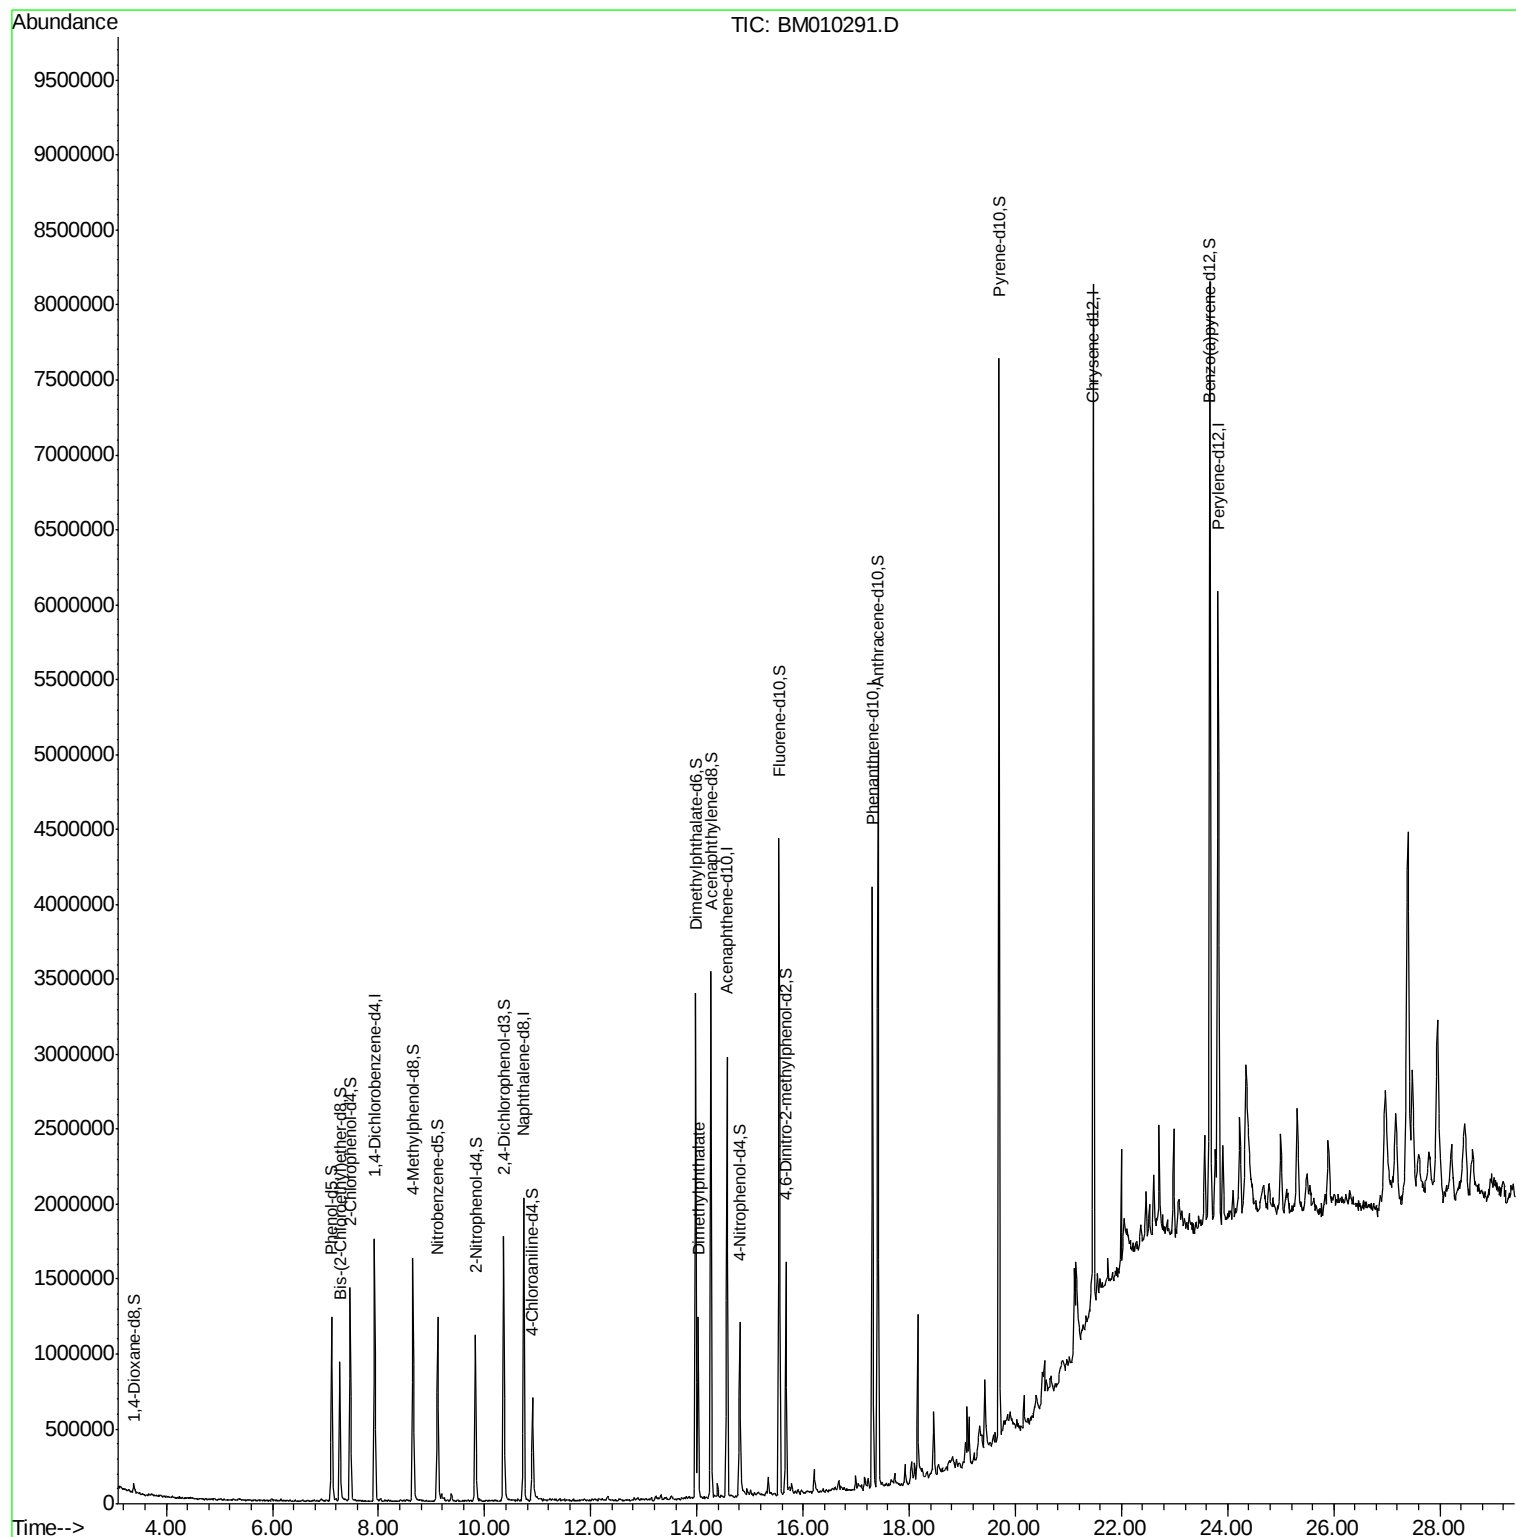

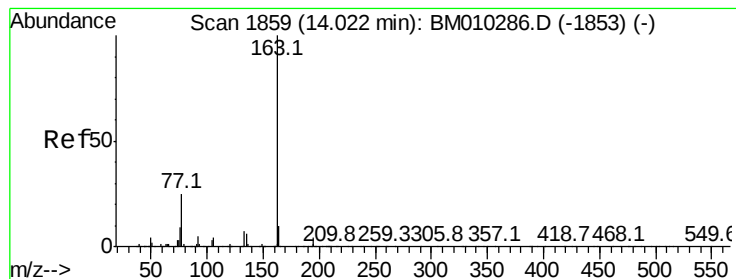

#44

Dimethylphthalate

Concen: 9.04 ng/ul

RT: 14.02 min Scan# 1859

Delta R.T. -0.00 min

Lab File: BM010291.D

Acq: 28 May 2017 00:32

Instrument :

BNA_M

ClientSampleId :

JHSE9

Tot Ion:163 Resp: 660581

Ion Ratio Lower Upper

163 100

194 3.7 3.5 5.3

164 10.3 8.2 12.4

