

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010298.D
 Acq On : 28 May 2017 04:44
 Operator : SJ/MA
 Sample : I3162-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSF3

Manual Integrations
 APPROVED

mohammad
 5/30/2017 4:41:35 PM

Quant Time: May 29 07:26:30 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 29 06:51:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	382454	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	1394723	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	804047	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.31	188	1866859	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	2669194	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	2847749	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	21294	2.28	ng/uL	0.00
5) Phenol-d5	7.12	99	352916	12.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.27	67	201814	12.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.47	132	295002	12.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	268202	11.47	ng/ul	0.00
19) Nitrobenzene-d5	9.11	128	131536	12.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.83	143	153181	12.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	293906	12.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	21696m	0.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	955577	14.30	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	1088905	13.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.81	143	104158	10.42	ng/ul	0.01
57) Fluorene-d10	15.55	176	804703	13.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	141370	10.69	ng/ul	0.00
70) Anthracene-d10	17.40	188	1164205	12.82	ng/ul	0.00
76) Pyrene-d10	19.69	212	1573579	14.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.67	264	1774766	13.39	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.02	163	368104	5.60	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010298.D
Acq On : 28 May 2017 04:44
Operator : SJ/MA
Sample : I3162-17
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JHSF3

Manual Integrations
APPROVED

mohammad
5/30/2017 4:41:35 PM

Quant Time: May 29 07:26:30 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 29 06:51:20 2017
Response via : Initial Calibration

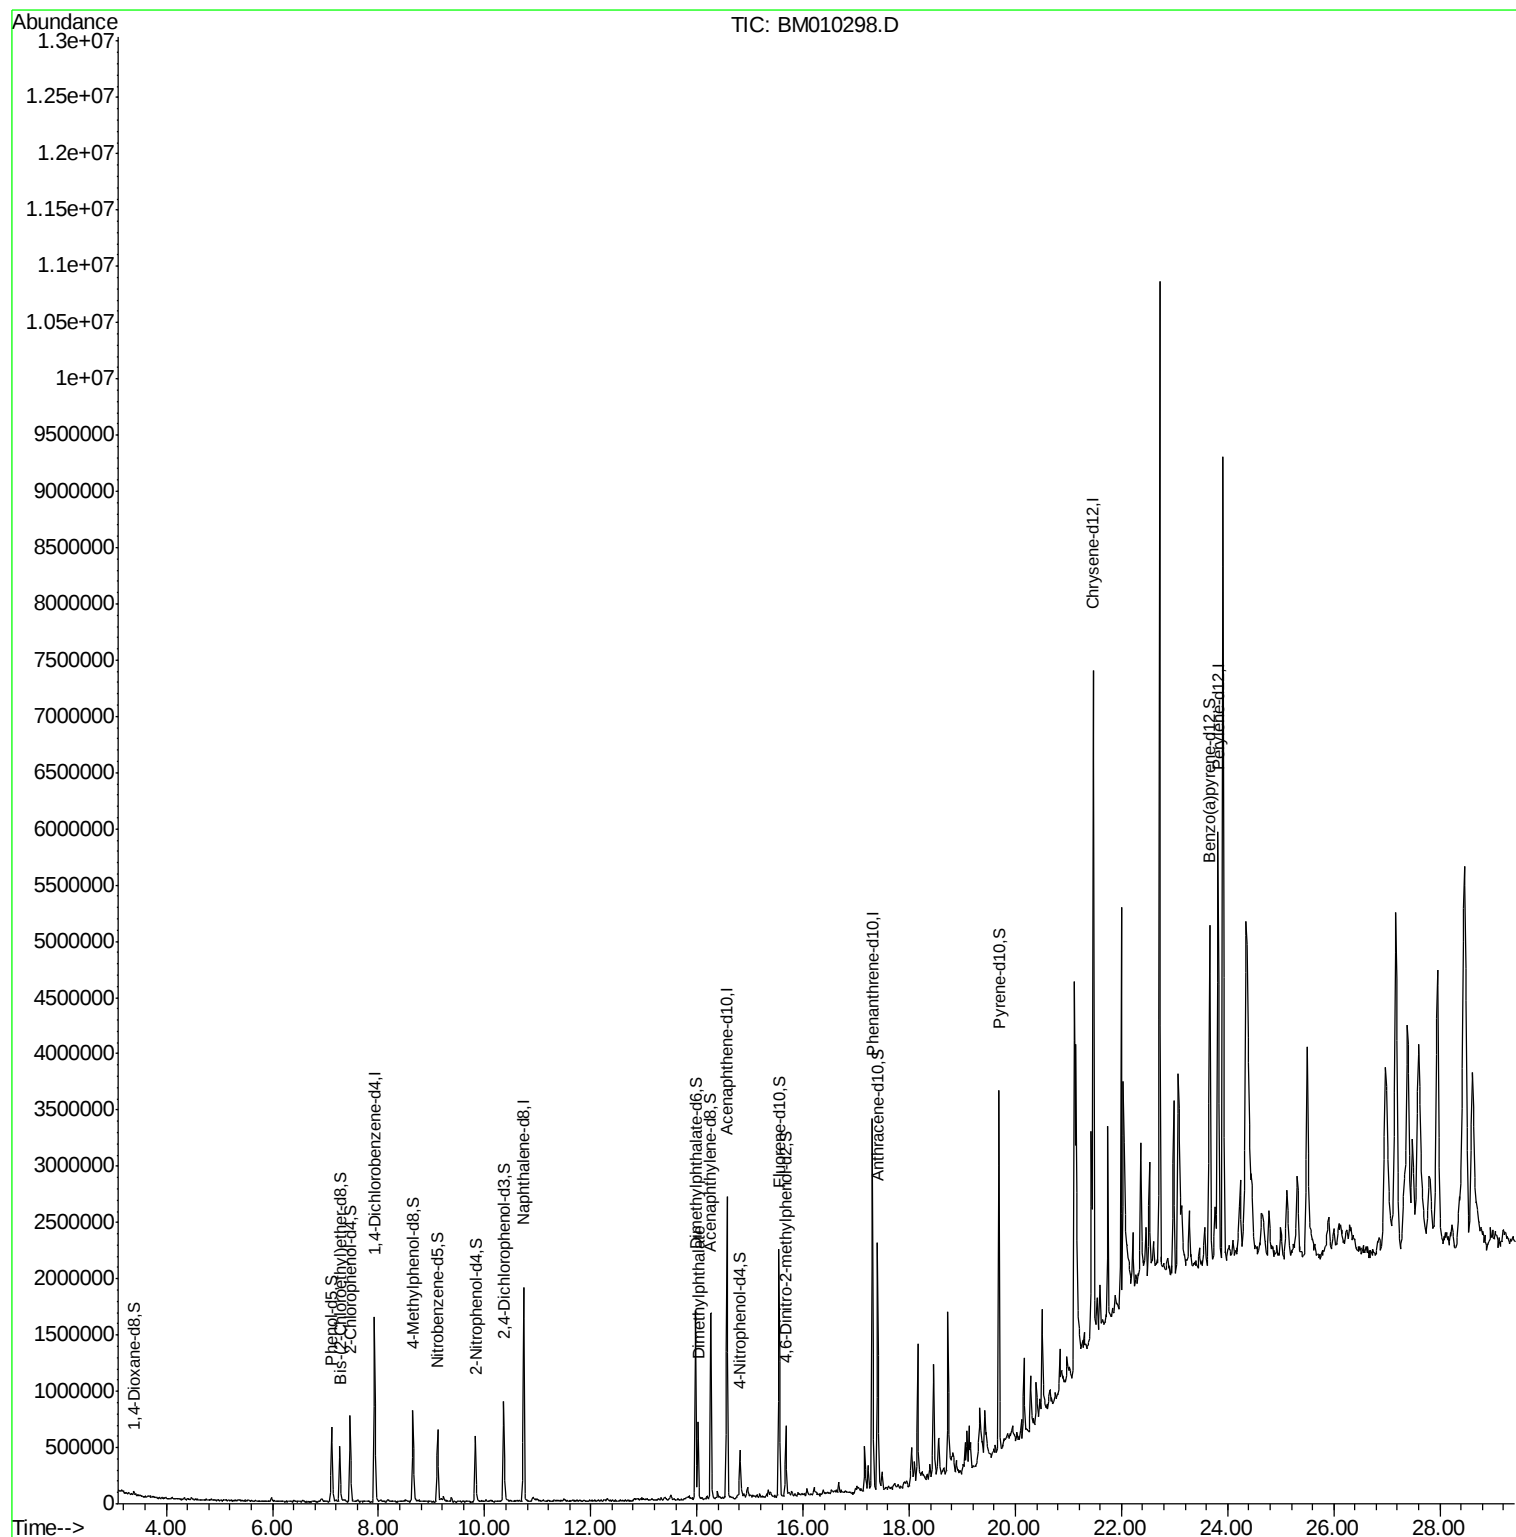

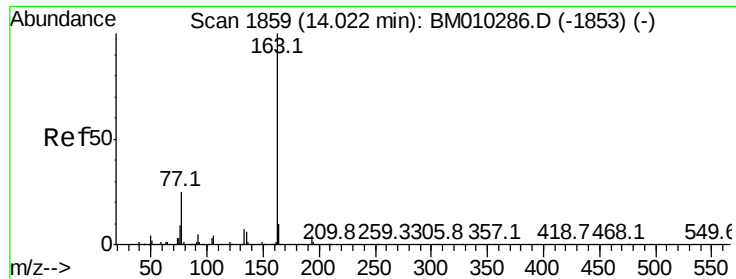

#44
 Dimethylphthalate
 Concen: 5.60 ng/ul
 RT: 14.02 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BM010298.D
 Acq: 28 May 2017 04:44

Instrument :
 BNA_M
 ClientSampleId :
 JHSF3

Tot Ion:	163	Resp:	368104
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.5	5.3
164	10.0	8.2	12.4

Manual Integrations
 APPROVED

mohammad
 5/30/2017 4:41:35 PM

