

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010278.D
 Acq On : 27 May 2017 16:44
 Operator : SJ/MA
 Sample : I3175-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDCC9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.116	679	685	696	rBV2	205302	354584	3.80%	0.469%
2	7.269	704	711	723	rBV	850107	1350742	14.47%	1.788%
3	7.469	738	745	755	rBV	1097061	1744081	18.68%	2.309%
4	7.928	817	823	833	rBV	1249805	2013769	21.57%	2.666%
5	8.651	940	946	957	rBV	681736	1100495	11.79%	1.457%
6	9.116	1018	1025	1035	rBV	1168603	1943019	20.81%	2.572%
7	9.828	1140	1146	1157	rVB	1042607	1708740	18.30%	2.262%
8	10.363	1228	1237	1249	rBV	1461229	2638088	28.26%	3.492%
9	10.734	1290	1300	1312	rBV	1513354	2561711	27.44%	3.391%
10	10.916	1323	1331	1343	rBV5	47760	132506	1.42%	0.175%
11	11.722	1463	1468	1478	rBV4	106443	281939	3.02%	0.373%
12	13.980	1845	1852	1862	rBV	3115249	4273376	45.78%	5.657%
13	14.263	1892	1900	1911	rBV	3221946	4625215	49.55%	6.123%
14	14.563	1942	1951	1959	rBV2	2149967	3362420	36.02%	4.451%
15	14.816	1988	1994	1999	rBV4	86054	186846	2.00%	0.247%
16	15.557	2113	2120	2130	rBV	4008615	5879660	62.98%	7.783%
17	15.674	2134	2140	2146	rBV	1169841	1640397	17.57%	2.171%
18	15.792	2154	2160	2166	rVB4	57266	95860	1.03%	0.127%
19	17.310	2411	2418	2426	rBV	2879742	4141603	44.37%	5.482%
20	17.410	2428	2435	2448	rVV	4421068	6363442	68.17%	8.423%
21	19.427	2774	2778	2784	rBV8	68644	114485	1.23%	0.152%
22	19.692	2818	2823	2830	rBV	5722519	7679423	82.26%	10.165%
23	21.468	3120	3125	3132	rBV	4631307	5901336	63.22%	7.812%
24	23.668	3493	3499	3506	rVB2	4933922	9335102	100.00%	12.357%
25	23.821	3519	3525	3533	rVB	3211157	6115624	65.51%	8.095%


Sum of corrected areas: 75544463

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010278.D
Acq On : 27 May 2017 16:44
Operator : SJ/MA
Sample : I3175-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC9

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

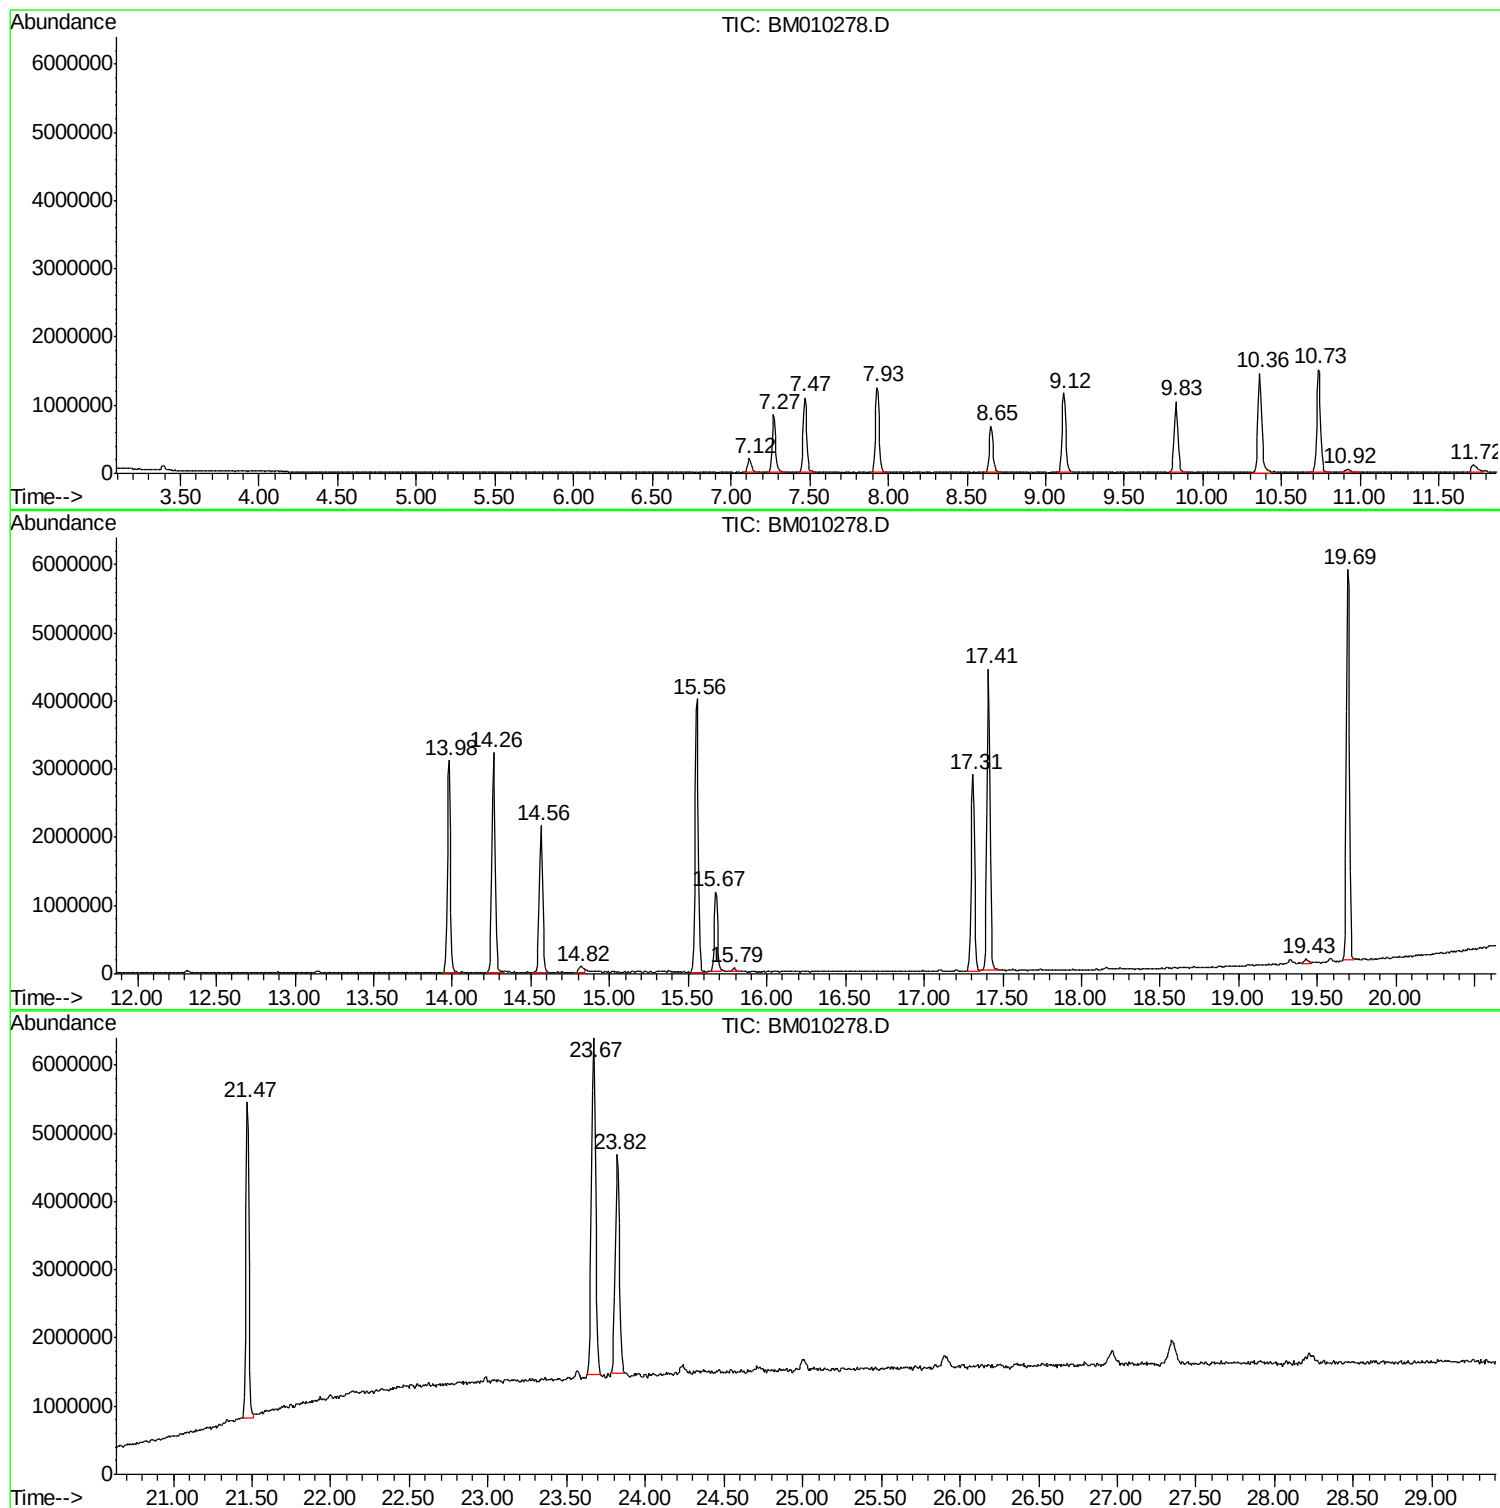

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010278.D
Acq On : 27 May 2017 16:44
Operator : SJ/MA
Sample : I3175-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010278.D
Acq On : 27 May 2017 16:44
Operator : SJ/MA
Sample : I3175-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
