

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010279.D
 Acq On : 27 May 2017 17:20
 Operator : SJ/MA
 Sample : I3175-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDCC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.116	680	685	694	rBV2	238352	409190	4.07%	0.531%
2	7.269	704	711	724	rBV	894368	1448893	14.42%	1.880%
3	7.469	738	745	752	rBV	1185780	1865752	18.57%	2.420%
4	7.928	815	823	831	rBV	1197993	1959691	19.50%	2.542%
5	8.651	938	946	962	rBV	718099	1245817	12.40%	1.616%
6	9.116	1017	1025	1036	rBV	1249060	2059727	20.50%	2.672%
7	9.828	1139	1146	1154	rBV	1113836	1801007	17.92%	2.336%
8	10.357	1229	1236	1250	rBV	1486972	2721266	27.08%	3.530%
9	10.734	1288	1300	1309	rBV	1396101	2439885	24.28%	3.165%
10	13.974	1845	1851	1858	rBV	3000347	4361881	43.40%	5.658%
11	14.263	1893	1900	1910	rBV	3314554	4768673	47.45%	6.186%
12	14.563	1941	1951	1959	rBV2	2106229	3197302	31.82%	4.148%
13	14.816	1986	1994	2000	rBV	101433	222329	2.21%	0.288%
14	15.557	2112	2120	2128	rBV	4145207	6182302	61.52%	8.020%
15	15.674	2131	2140	2147	rBV	1264829	1751775	17.43%	2.273%
16	17.310	2412	2418	2427	rBV	2735979	3843476	38.25%	4.986%
17	17.410	2428	2435	2446	rVB	4770760	6765299	67.32%	8.776%
18	18.157	2558	2562	2567	rBV5	83071	139833	1.39%	0.181%
19	19.427	2774	2778	2783	rBV6	118921	182088	1.81%	0.236%
20	19.692	2818	2823	2830	rBV	6120456	8330382	82.89%	10.807%
21	21.468	3120	3125	3133	rBV	4455757	5517367	54.90%	7.157%
22	23.668	3493	3499	3507	rVB2	5300678	10049392	100.00%	13.037%
23	23.821	3519	3525	3533	rVB	3097272	5822235	57.94%	7.553%


Sum of corrected areas: 77085562

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010279.D
Acq On : 27 May 2017 17:20
Operator : SJ/MA
Sample : I3175-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

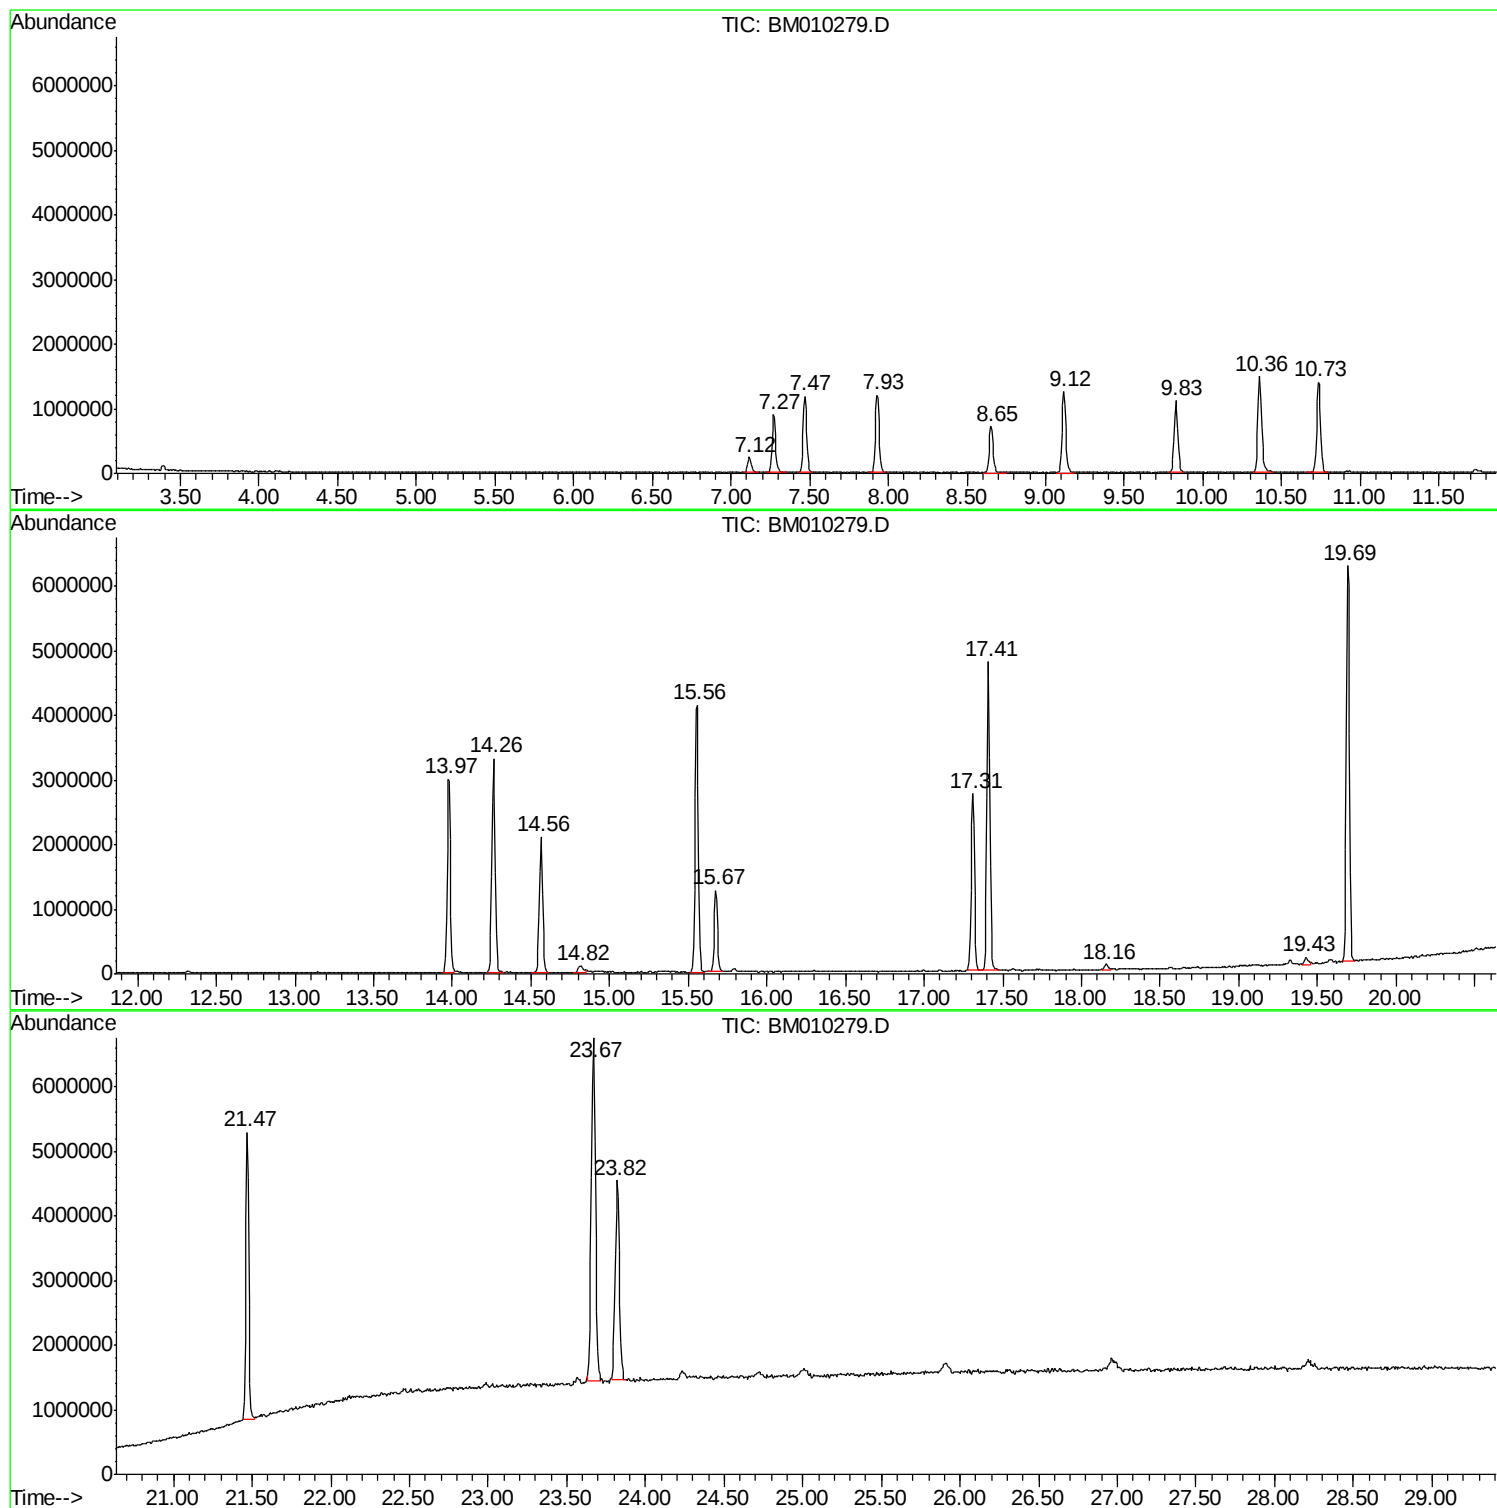

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010279.D
Acq On : 27 May 2017 17:20
Operator : SJ/MA
Sample : I3175-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010279.D
Acq On : 27 May 2017 17:20
Operator : SJ/MA
Sample : I3175-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc