

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
 Data File : BM010280.D
 Acq On : 27 May 2017 17:56
 Operator : SJ/MA
 Sample : I3175-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDCC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	48	51	58	rVB	75969	105687	1.23%	0.146%
2	7.116	678	685	695	rBV	220273	411424	4.78%	0.567%
3	7.269	704	711	723	rBV	860597	1387968	16.14%	1.912%
4	7.469	736	745	755	rBV	1126642	1826015	21.24%	2.515%
5	7.928	816	823	834	rBV	1263524	2072916	24.11%	2.855%
6	8.651	938	946	955	rBV	699768	1169179	13.60%	1.610%
7	9.116	1016	1025	1033	rBV	1188852	1955153	22.74%	2.693%
8	9.828	1139	1146	1155	rBV	1037844	1685795	19.61%	2.322%
9	10.357	1229	1236	1246	rBV	1455955	2566832	29.85%	3.536%
10	10.733	1293	1300	1310	rBV	1500340	2570284	29.89%	3.540%
11	11.739	1466	1471	1477	rBV7	39582	93200	1.08%	0.128%
12	13.980	1843	1852	1858	rBV	2855758	4047005	47.07%	5.574%
13	14.263	1893	1900	1910	rBV	2905137	4169658	48.49%	5.743%
14	14.563	1944	1951	1960	rBV2	2154682	3295648	38.33%	4.539%
15	14.816	1989	1994	2003	rBV4	83520	209304	2.43%	0.288%
16	15.557	2113	2120	2129	rBV	3962730	5676023	66.01%	7.818%
17	15.680	2134	2141	2147	rBV	1091831	1573898	18.30%	2.168%
18	17.310	2411	2418	2426	rBV	2857078	3945884	45.89%	5.435%
19	17.410	2428	2435	2446	rBV	4311036	6103041	70.98%	8.406%
20	18.151	2557	2561	2568	rBV8	113602	187967	2.19%	0.259%
21	19.427	2774	2778	2787	rBV7	128587	231782	2.70%	0.319%
22	19.692	2817	2823	2830	rBV	5588068	7469485	86.87%	10.288%
23	21.468	3120	3125	3132	rBV	4434261	5446975	63.35%	7.503%
24	23.668	3493	3499	3506	rVB	4485748	8598212	100.00%	11.843%
25	23.821	3519	3525	3535	rVB	2994786	5801881	67.48%	7.991%


Sum of corrected areas: 72601216

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052717\
Data File : BM010280.D
Acq On : 27 May 2017 17:56
Operator : SJ/MA
Sample : I3175-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

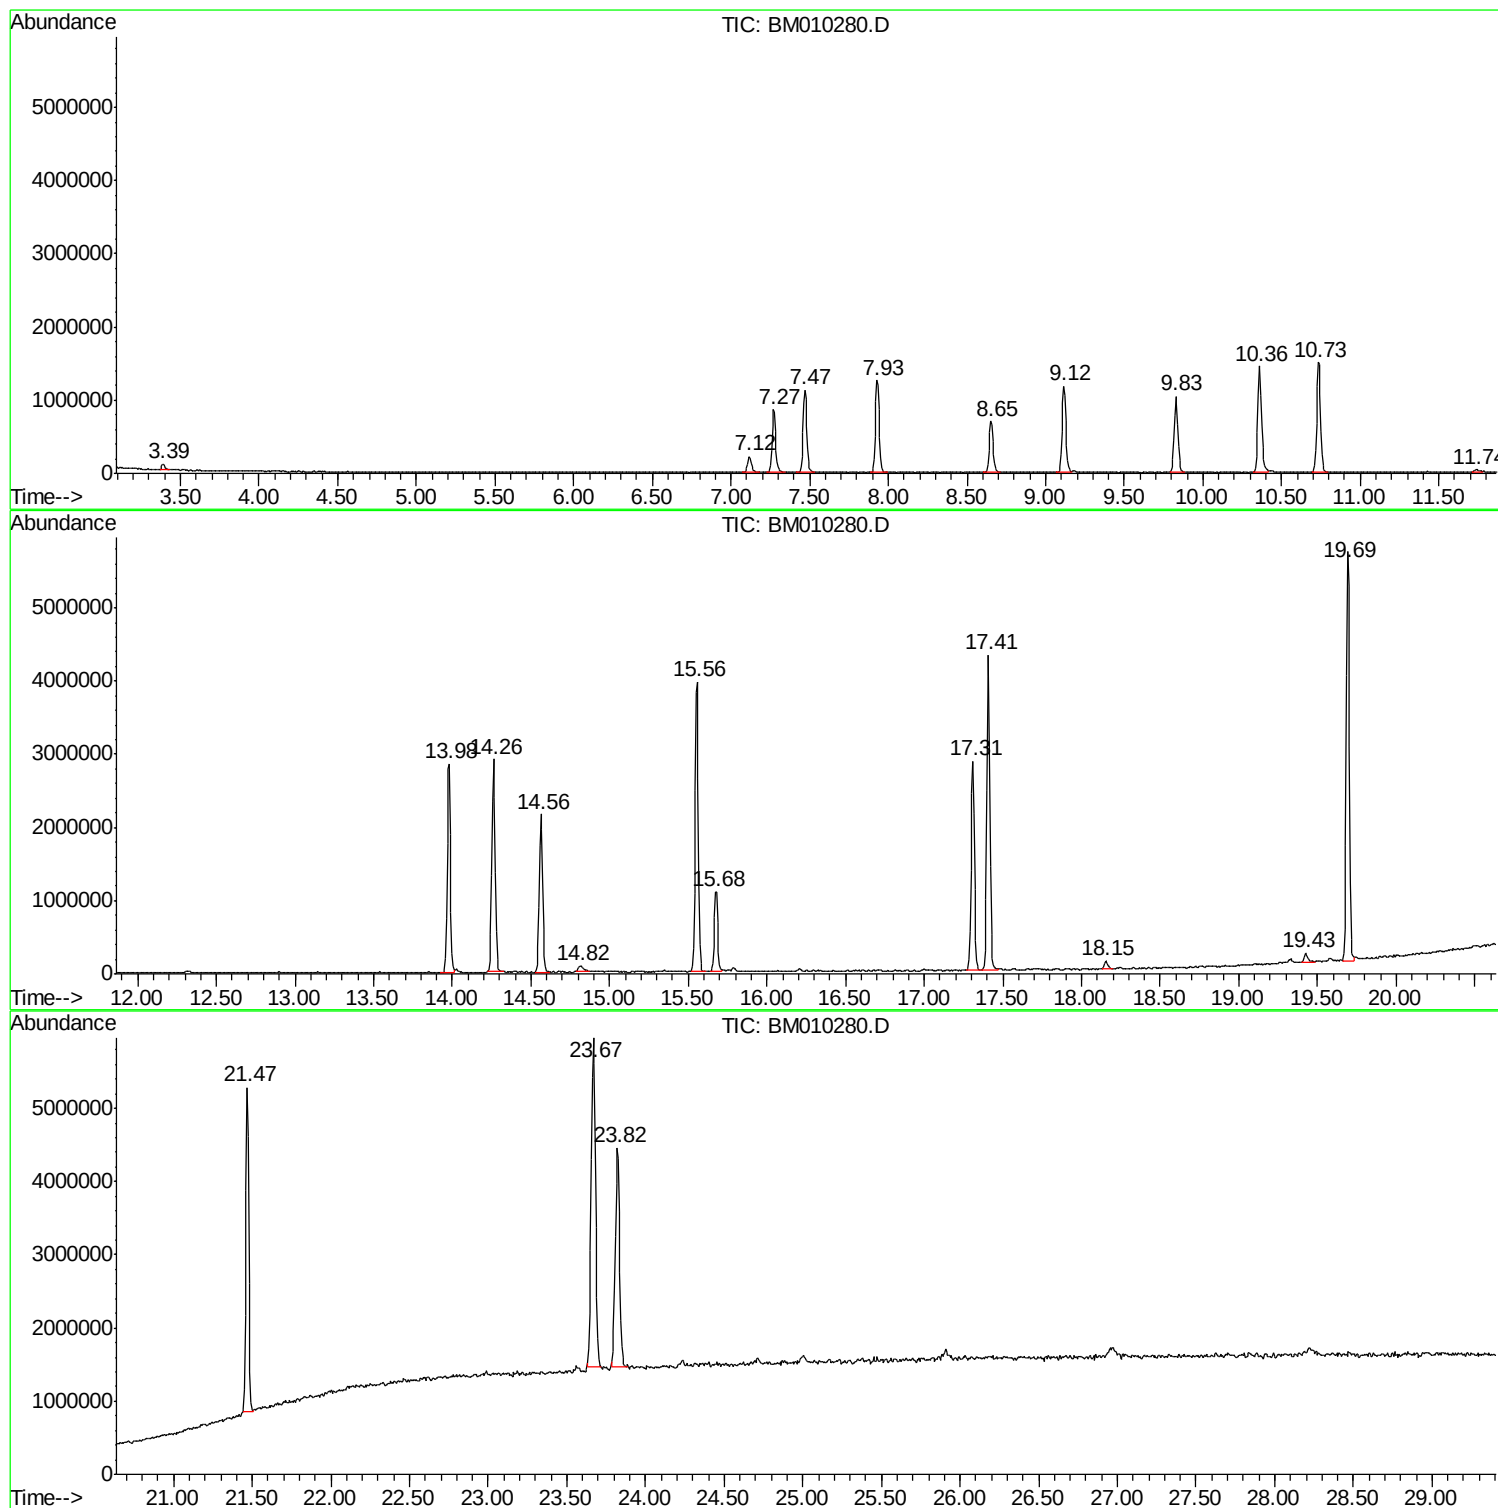

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010280.D
Acq On : 27 May 2017 17:56
Operator : SJ/MA
Sample : I3175-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052717\
Data File : BM010280.D
Acq On : 27 May 2017 17:56
Operator : SJ/MA
Sample : I3175-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDCC7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc