

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026145.D
 Acq On : 27 May 2020 14:53
 Operator : MA/SJ
 Sample : L2737-15DL2 500X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B14DL2

Quant Time: May 27 15:35:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 27 10:30:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	120225	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	490478	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	282259	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	608499	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	628939	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	654183	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0d	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.56	166	1319	0.06	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1759	0.07	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.13	176	1424	0.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	19.28	212	2877	0.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
28) Naphthalene	10.29	128	718255	23.951	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
Data File : BM026145.D
Acq On : 27 May 2020 14:53
Operator : MA/SJ
Sample : L2737-15DL2 500X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Quant Time: May 27 15:35:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 27 10:30:40 2020
Response via : Initial Calibration

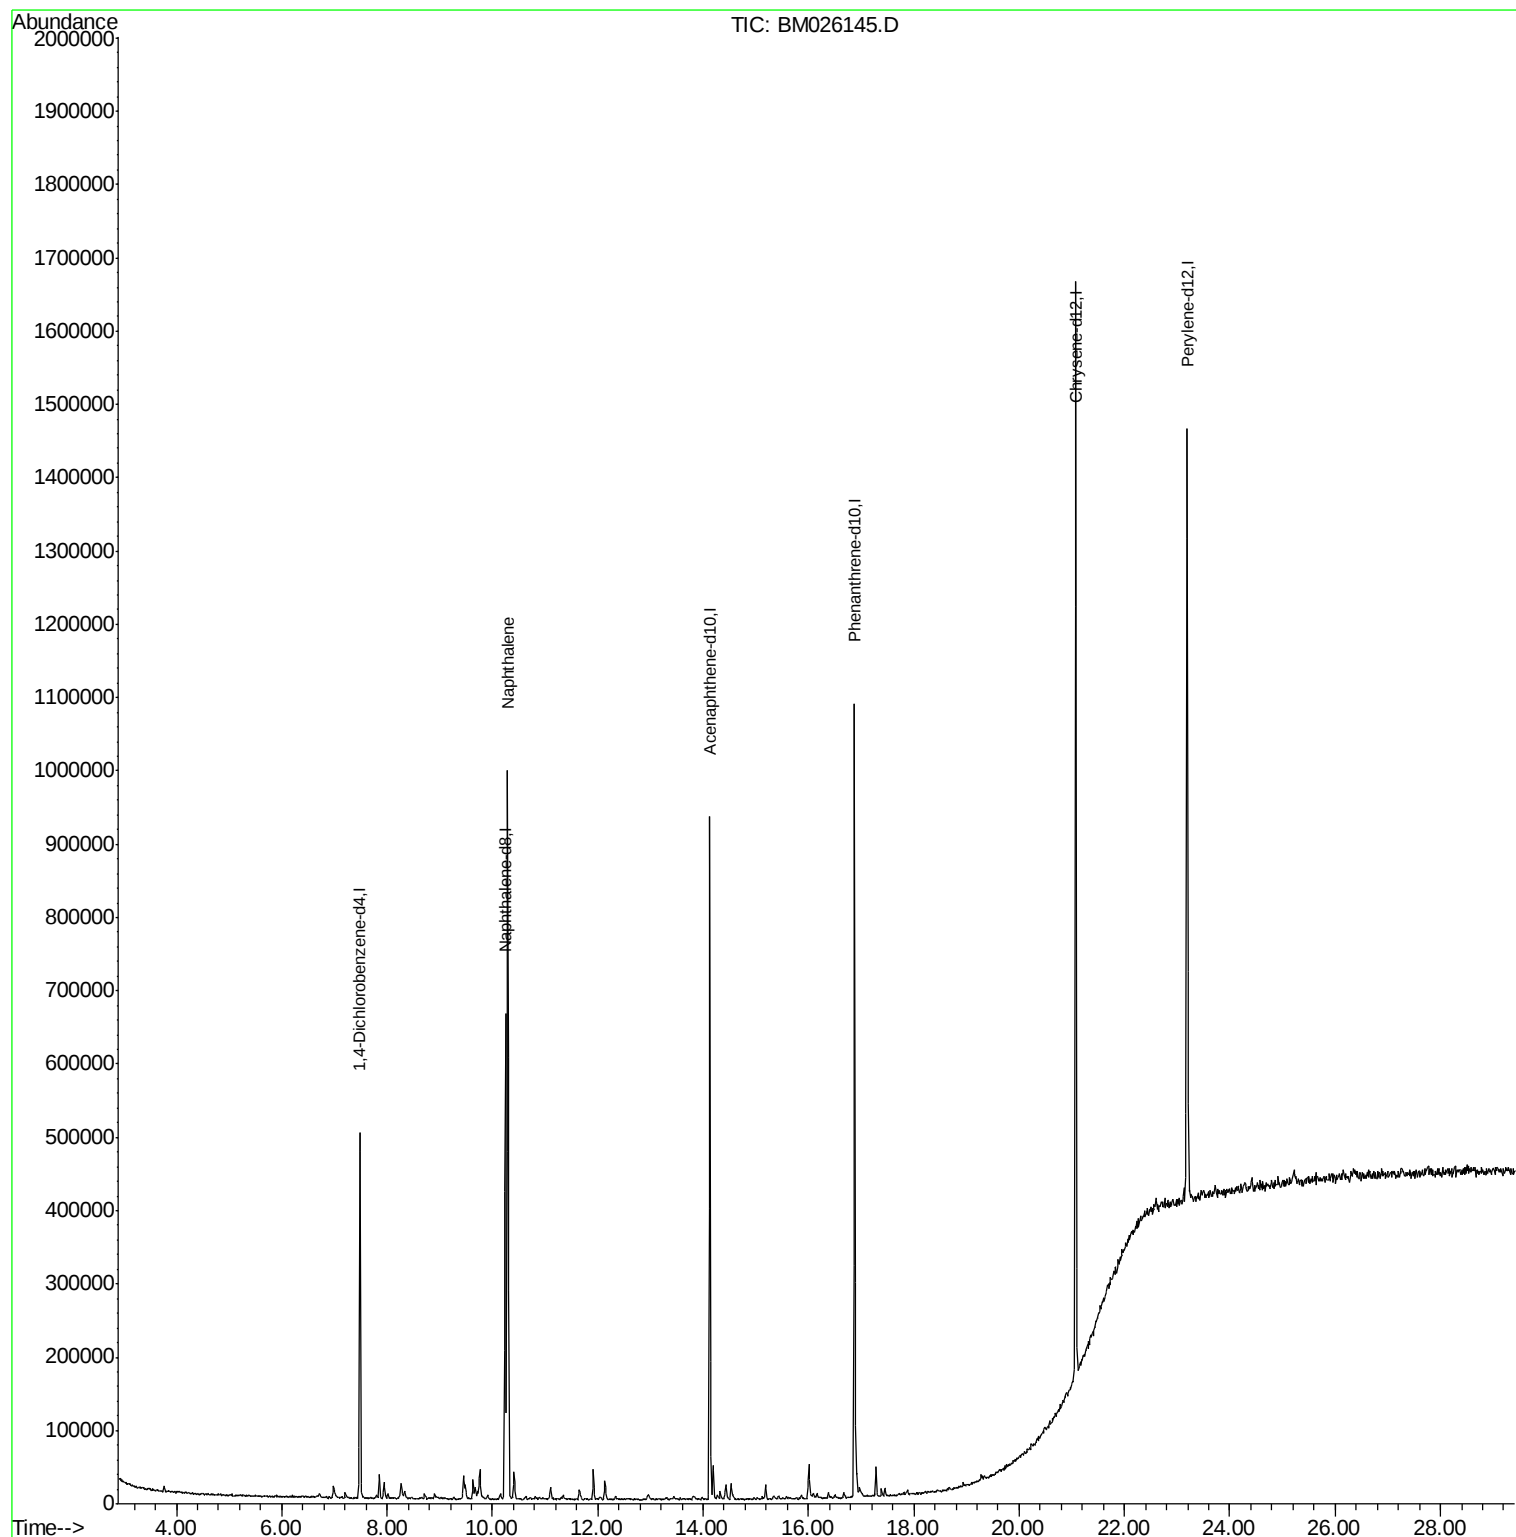


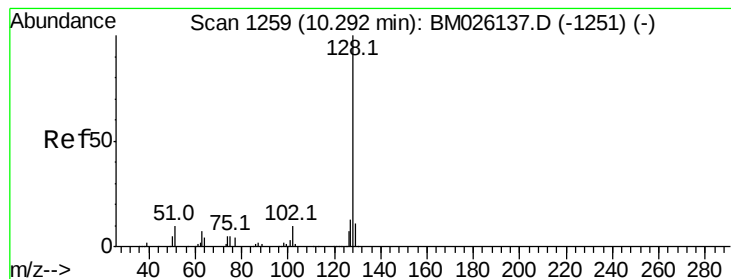

#28
Naphthalene
Concen: 23.951 ng/ul
RT: 10.29 min Scan# 1259
Delta R.T. 0.00 min
Lab File: BM026145.D
Acq: 27 May 2020 14:53

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.4	9.0	13.4
127	12.4	10.6	15.8

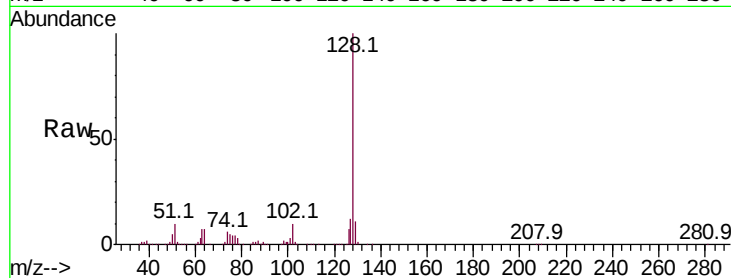

Abundance

Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

