

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026143.D
 Acq On : 27 May 2020 13:39
 Operator : MA/SJ
 Sample : L2737-13DL2 250X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B10DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.763	146	149	154	rVB3	9639	13178	0.74%	0.122%
2	5.040	364	366	370	rVB5	2234	2418	0.14%	0.022%
3	5.081	370	373	376	rBV4	2219	2599	0.15%	0.024%
4	5.928	515	517	520	rBV3	1509	2327	0.13%	0.022%
5	6.028	532	534	537	rBV4	2256	2622	0.15%	0.024%
6	6.128	548	551	553	rVB4	2149	2656	0.15%	0.025%
7	6.246	567	571	578	rVV7	1636	2911	0.16%	0.027%
8	6.710	648	650	656	rVB3	3718	5148	0.29%	0.048%
9	7.210	732	735	739	rBV4	4867	6156	0.35%	0.057%
10	7.481	774	781	790	rBV	480531	760066	42.86%	7.059%
11	7.710	819	820	824	rBV4	2520	3006	0.17%	0.028%
12	7.799	829	835	838	rVV5	7447	12535	0.71%	0.116%
13	7.851	838	844	851	rVV2	19947	35889	2.02%	0.333%
14	7.946	855	860	866	rVV	22230	37577	2.12%	0.349%
15	8.010	867	871	877	rVV4	6528	12721	0.72%	0.118%
16	8.269	909	915	923	rBV2	15143	31618	1.78%	0.294%
17	8.328	923	925	930	rVB5	4433	7102	0.40%	0.066%
18	8.475	948	950	957	rVB6	2035	4582	0.26%	0.043%
19	8.534	957	960	964	rBV5	1618	3077	0.17%	0.029%
20	8.651	979	980	984	rVB3	3128	3267	0.18%	0.030%
21	8.716	986	991	995	rVB	7827	10492	0.59%	0.097%
22	8.904	1020	1023	1027	rVB6	3462	4895	0.28%	0.045%
23	8.951	1027	1031	1032	rBV4	2064	2418	0.14%	0.022%
24	9.257	1079	1083	1086	rBV3	1930	2544	0.14%	0.024%
25	9.451	1110	1116	1120	rBV	23498	41296	2.33%	0.384%
26	9.487	1120	1122	1129	rVB6	14661	21047	1.19%	0.195%
27	9.634	1141	1147	1150	rBV	30369	44276	2.50%	0.411%
28	9.675	1150	1154	1158	rVV5	15418	27402	1.55%	0.255%
29	9.716	1158	1161	1164	rVV4	2928	5520	0.31%	0.051%
30	9.763	1164	1169	1180	rVB	32287	58958	3.32%	0.548%
31	9.875	1186	1188	1189	rBV2	4267	3595	0.20%	0.033%
32	9.893	1189	1191	1193	rVB3	2187	2889	0.16%	0.027%
33	10.151	1229	1235	1242	rBV3	6362	10445	0.59%	0.097%
34	10.245	1244	1251	1255	rBV	629177	1035909	58.42%	9.621%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026143.D
 Acq On : 27 May 2020 13:39
 Operator : MA/SJ
 Sample : L2737-13DL2 250X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B10DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	10.292	1255	1259	1267	rVB	777038	1221914	68.91%	11.349%
36	10.410	1272	1279	1284	rVV	39540	65160	3.67%	0.605%
37	10.634	1312	1317	1324	rVB7	2565	6139	0.35%	0.057%
38	10.816	1342	1348	1351	rBV7	3537	5950	0.34%	0.055%
39	10.887	1356	1360	1362	rBV4	2340	2981	0.17%	0.028%
40	11.110	1392	1398	1404	rBV5	7614	16225	0.91%	0.151%
41	11.292	1422	1429	1431	rBV7	3006	5322	0.30%	0.049%
42	11.345	1436	1438	1442	rVV4	3968	4475	0.25%	0.042%
43	11.657	1486	1491	1497	rBV7	5984	11549	0.65%	0.107%
44	11.916	1529	1535	1543	rBV	19389	33311	1.88%	0.309%
45	12.039	1551	1556	1558	rBV5	4051	6188	0.35%	0.057%
46	12.145	1567	1574	1584	rVB2	21414	36434	2.05%	0.338%
47	12.275	1593	1596	1599	rBV4	1813	3026	0.17%	0.028%
48	12.334	1603	1606	1612	rVV7	4296	7102	0.40%	0.066%
49	12.939	1702	1709	1710	rBV6	2412	3841	0.22%	0.036%
50	12.963	1710	1713	1721	rVB7	3377	7580	0.43%	0.070%
51	13.157	1742	1746	1748	rBV4	2329	2304	0.13%	0.021%
52	13.286	1764	1768	1770	rBV4	2512	3337	0.19%	0.031%
53	13.316	1770	1773	1775	rVB3	2384	2694	0.15%	0.025%
54	13.451	1791	1796	1801	rVB7	4358	6292	0.35%	0.058%
55	13.504	1803	1805	1810	rVB5	3118	3662	0.21%	0.034%
56	13.563	1812	1815	1817	rBV	4233	4618	0.26%	0.043%
57	13.686	1832	1836	1840	rVV5	3234	4930	0.28%	0.046%
58	13.816	1855	1858	1862	rBV4	5610	8589	0.48%	0.080%
59	14.128	1905	1911	1918	rVV	878847	1245341	70.23%	11.567%
60	14.192	1918	1922	1930	rVB	66320	94570	5.33%	0.878%
61	14.269	1930	1935	1939	rVB2	5266	7436	0.42%	0.069%
62	14.328	1941	1945	1952	rBV	11384	16573	0.93%	0.154%
63	14.422	1956	1961	1962	rBV4	4958	6512	0.37%	0.060%
64	14.533	1975	1980	1984	rBV	21349	33222	1.87%	0.309%
65	14.645	1997	1999	2002	rBV3	2706	3722	0.21%	0.035%
66	14.869	2032	2037	2050	rBV2	38426	78857	4.45%	0.732%
67	15.127	2075	2081	2086	rVB4	7624	11178	0.63%	0.104%
68	15.186	2086	2091	2095	rBV	28677	42390	2.39%	0.394%
69	15.345	2112	2118	2124	rVB9	3463	7975	0.45%	0.074%
70	15.498	2137	2144	2149	rVB8	2778	6083	0.34%	0.056%
71	15.822	2195	2199	2201	rBV4	2400	4051	0.23%	0.038%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026143.D
 Acq On : 27 May 2020 13:39
 Operator : MA/SJ
 Sample : L2737-13DL2 250X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B10DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.869	2201	2207	2214	rVB6	13703	28069	1.58%	0.261%
73	16.004	2224	2230	2236	rBV	30307	52552	2.96%	0.488%
74	16.051	2236	2238	2241	rVV4	6267	7861	0.44%	0.073%
75	16.092	2241	2245	2253	rVV2	31120	57063	3.22%	0.530%
76	16.169	2253	2258	2262	rVB5	5365	10704	0.60%	0.099%
77	16.380	2290	2294	2301	rVB7	7965	12619	0.71%	0.117%
78	16.510	2314	2316	2322	rVB7	3919	5378	0.30%	0.050%
79	16.680	2337	2345	2353	rBV9	12462	30607	1.73%	0.284%
80	16.798	2362	2365	2368	rBV5	2035	2607	0.15%	0.024%
81	16.874	2372	2378	2383	rBV	1041765	1457499	82.19%	13.537%
82	16.916	2383	2385	2391	rVV	52814	71087	4.01%	0.660%
83	16.980	2392	2396	2400	rVB2	13142	19661	1.11%	0.183%
84	17.080	2409	2413	2418	rBV5	5363	7945	0.45%	0.074%
85	17.157	2422	2426	2429	rBV5	1741	2583	0.15%	0.024%
86	17.204	2429	2434	2440	rBV4	9302	18847	1.06%	0.175%
87	17.286	2440	2448	2456	rVB2	53546	83890	4.73%	0.779%
88	17.386	2461	2465	2473	rVV4	9875	17494	0.99%	0.162%
89	17.451	2473	2476	2482	rVB4	11446	15652	0.88%	0.145%
90	17.721	2518	2522	2525	rBV5	5914	8183	0.46%	0.076%
91	17.804	2530	2536	2538	rBV5	6023	9232	0.52%	0.086%
92	17.880	2546	2549	2554	rVB5	5815	9036	0.51%	0.084%
93	17.945	2554	2560	2564	rBV7	6177	11519	0.65%	0.107%
94	18.104	2584	2587	2588	rBV3	3711	3788	0.21%	0.035%
95	18.945	2726	2730	2735	rBV2	10127	16405	0.93%	0.152%
96	19.151	2761	2765	2769	rBV5	5763	8891	0.50%	0.083%
97	19.280	2783	2787	2789	rBV3	10957	15432	0.87%	0.143%
98	19.339	2794	2797	2802	rVB5	13789	20155	1.14%	0.187%
99	21.074	3088	3092	3100	rBV	1315793	1733922	97.78%	16.105%
100	23.198	3447	3453	3463	rVB	1025008	1773274	100.00%	16.470%


Sum of corrected areas: 10766629

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
Data File : BM026143.D
Acq On : 27 May 2020 13:39
Operator : MA/SJ
Sample : L2737-13DL2 250X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B10DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

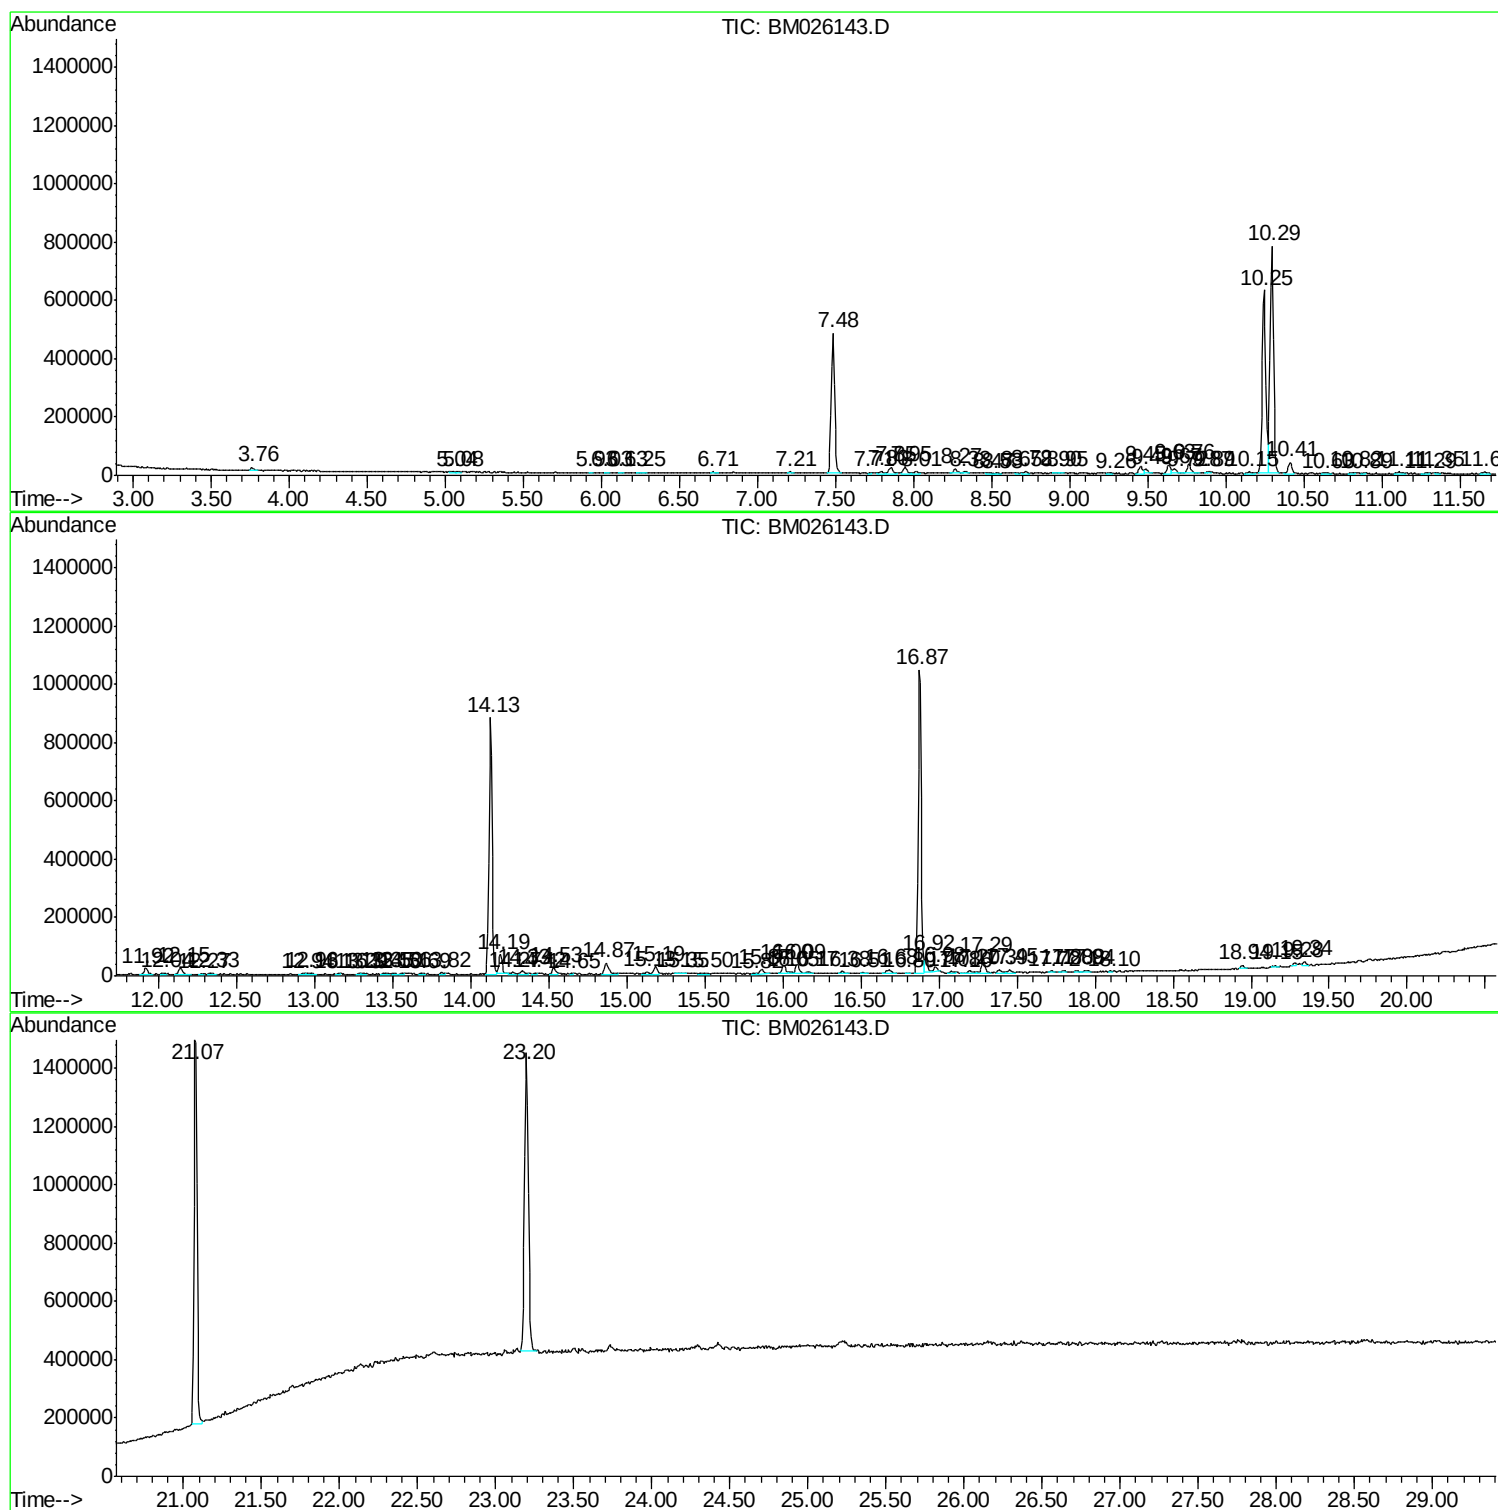

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052720\
Data File : BM026143.D
Acq On : 27 May 2020 13:39
Operator : MA/SJ
Sample : L2737-13DL2 250X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B10DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052720\
Data File : BM026143.D
Acq On : 27 May 2020 13:39
Operator : MA/SJ
Sample : L2737-13DL2 250X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B10DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc