

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026145.D
 Acq On : 27 May 2020 14:53
 Operator : MA/SJ
 Sample : L2737-15DL2 500X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B14DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.763	145	149	155	rVB2	9274	15756	0.87%	0.138%
2	4.058	197	199	204	rVB5	2046	2346	0.13%	0.021%
3	4.799	323	325	329	rBV5	2245	2640	0.15%	0.023%
4	5.334	415	416	420	rBV2	2457	2398	0.13%	0.021%
5	5.499	441	444	446	rBV3	1884	2358	0.13%	0.021%
6	6.275	573	576	579	rBV5	2516	2910	0.16%	0.026%
7	6.434	600	603	606	rBV4	2006	2561	0.14%	0.022%
8	6.599	627	631	635	rBV4	2334	3083	0.17%	0.027%
9	6.675	641	644	647	rBV5	1483	2408	0.13%	0.021%
10	6.716	647	651	657	rVB4	6123	11980	0.66%	0.105%
11	6.851	667	674	679	rVB7	2489	6023	0.33%	0.053%
12	6.899	679	682	683	rBV3	3077	2926	0.16%	0.026%
13	6.987	692	697	702	rBV	15970	28086	1.55%	0.246%
14	7.204	731	734	741	rVB3	7558	12510	0.69%	0.110%
15	7.404	763	768	770	rVB5	1626	2734	0.15%	0.024%
16	7.481	775	781	791	rVV	499297	781203	43.05%	6.852%
17	7.798	828	835	838	rBV6	5669	8730	0.48%	0.077%
18	7.851	839	844	851	rVV	33282	49315	2.72%	0.433%
19	7.940	853	859	868	rVV	22939	39032	2.15%	0.342%
20	8.010	868	871	877	rVB5	6617	10480	0.58%	0.092%
21	8.275	910	916	921	rBV3	20478	43488	2.40%	0.381%
22	8.328	921	925	932	rVV3	10656	19587	1.08%	0.172%
23	8.416	934	940	945	rBV7	1562	3883	0.21%	0.034%
24	8.628	972	976	978	rBV5	2435	3448	0.19%	0.030%
25	8.657	978	981	984	rVV5	2513	3053	0.17%	0.027%
26	8.710	987	990	995	rVV3	7859	13268	0.73%	0.116%
27	8.793	999	1004	1007	rBV5	1752	2641	0.15%	0.023%
28	8.904	1017	1023	1026	rBV7	7063	12711	0.70%	0.111%
29	8.963	1030	1033	1036	rVV5	2781	3913	0.22%	0.034%
30	9.010	1038	1041	1046	rVB6	2385	3542	0.20%	0.031%
31	9.063	1046	1050	1054	rBV6	1871	2934	0.16%	0.026%
32	9.187	1068	1071	1077	rBV6	1671	2427	0.13%	0.021%
33	9.251	1079	1082	1087	rBV7	3407	6798	0.37%	0.060%
34	9.451	1109	1116	1119	rVV	33025	52232	2.88%	0.458%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
 Data File : BM026145.D
 Acq On : 27 May 2020 14:53
 Operator : MA/SJ
 Sample : L2737-15DL2 500X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B14DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	9.481	1119	1121	1130	rVV6	19346	35407	1.95%	0.311%
36	9.634	1141	1147	1150	rBV	26804	37354	2.06%	0.328%
37	9.669	1150	1153	1158	rVV2	15445	25106	1.38%	0.220%
38	9.716	1158	1161	1163	rVV3	9102	12768	0.70%	0.112%
39	9.763	1164	1169	1178	rVB2	38400	69173	3.81%	0.607%
40	9.910	1186	1194	1199	rBV6	6393	11944	0.66%	0.105%
41	10.151	1230	1235	1241	rBV4	7384	15098	0.83%	0.132%
42	10.245	1244	1251	1255	rVV	662855	1104846	60.88%	9.691%
43	10.292	1255	1259	1271	rVV	994317	1565216	86.25%	13.730%
44	10.410	1271	1279	1285	rVB	35841	59855	3.30%	0.525%
45	10.616	1308	1314	1315	rBV6	3090	4848	0.27%	0.043%
46	10.639	1315	1318	1322	rVB5	3790	5345	0.29%	0.047%
47	10.810	1342	1347	1352	rBV5	3054	5682	0.31%	0.050%
48	10.845	1352	1353	1356	rVB3	2572	2586	0.14%	0.023%
49	10.887	1356	1360	1363	rBV3	2973	3875	0.21%	0.034%
50	11.104	1390	1397	1403	rVV	17353	30670	1.69%	0.269%
51	11.292	1425	1429	1434	rBV6	3490	6470	0.36%	0.057%
52	11.345	1434	1438	1445	rVB4	5262	6365	0.35%	0.056%
53	11.651	1484	1490	1498	rBV6	13556	28905	1.59%	0.254%
54	11.916	1529	1535	1541	rBV	41623	69362	3.82%	0.608%
55	12.034	1552	1555	1560	rVB6	3434	6324	0.35%	0.055%
56	12.139	1565	1573	1579	rBV	25743	44675	2.46%	0.392%
57	12.345	1602	1608	1610	rBV5	4176	6632	0.37%	0.058%
58	12.963	1705	1713	1719	rBV4	7132	16303	0.90%	0.143%
59	13.057	1728	1729	1735	rVB4	1984	2521	0.14%	0.022%
60	13.451	1790	1796	1801	rVB7	4057	5733	0.32%	0.050%
61	13.633	1825	1827	1832	rVB4	2042	2836	0.16%	0.025%
62	13.816	1856	1858	1862	rBV3	3384	3936	0.22%	0.035%
63	13.975	1881	1885	1889	rBV6	3603	6150	0.34%	0.054%
64	14.128	1904	1911	1917	rBV	931669	1333857	73.50%	11.700%
65	14.192	1917	1922	1931	rVB	45881	72243	3.98%	0.634%
66	14.275	1931	1936	1941	rVB	6613	9716	0.54%	0.085%
67	14.327	1941	1945	1955	rVB3	11890	20076	1.11%	0.176%
68	14.433	1955	1963	1974	rVB3	20503	44388	2.45%	0.389%
69	14.533	1974	1980	1983	rBV	21770	31445	1.73%	0.276%
70	15.122	2078	2080	2085	rVV5	3511	4663	0.26%	0.041%
71	15.186	2085	2091	2100	rVB3	20970	30504	1.68%	0.268%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
Data File : BM026145.D
Acq On : 27 May 2020 14:53
Operator : MA/SJ
Sample : L2737-15DL2 500X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Title : SVOA CALIBRATION

72	15.339	2112	2117	2119	rBV6	3529	4493	0.25%	0.039%
73	15.439	2130	2134	2137	rVB6	2861	5009	0.28%	0.044%
74	15.580	2154	2158	2163	rBV5	2963	3422	0.19%	0.030%
75	15.869	2202	2207	2212	rVB5	5958	10053	0.55%	0.088%
76	16.010	2224	2231	2238	rBV	47780	87106	4.80%	0.764%
77	16.092	2241	2245	2250	rVV5	5952	11667	0.64%	0.102%
78	16.163	2253	2257	2262	rVV2	5388	7316	0.40%	0.064%
79	16.380	2291	2294	2300	rVB5	7375	10584	0.58%	0.093%
80	16.510	2312	2316	2319	rVB4	4937	7208	0.40%	0.063%
81	16.669	2339	2343	2352	rVB5	7101	15987	0.88%	0.140%
82	16.810	2363	2367	2370	rVB5	2653	3971	0.22%	0.035%
83	16.874	2370	2378	2384	rBV	1083486	1574989	86.79%	13.815%
84	16.974	2392	2395	2406	rVB4	13019	33204	1.83%	0.291%
85	17.251	2441	2442	2444	rBV2	2417	2439	0.13%	0.021%
86	17.286	2444	2448	2453	rVB	39244	51312	2.83%	0.450%
87	17.386	2462	2465	2470	rVB4	9995	13282	0.73%	0.117%
88	17.457	2473	2477	2481	rBV2	10457	14520	0.80%	0.127%
89	17.621	2501	2505	2509	rBV6	2172	3700	0.20%	0.032%
90	17.727	2519	2523	2526	rBV4	3144	4219	0.23%	0.037%
91	17.804	2533	2536	2539	rVB5	3102	4756	0.26%	0.042%
92	17.880	2546	2549	2553	rVB6	6551	8839	0.49%	0.078%
93	18.051	2574	2578	2579	rBV4	2379	2631	0.14%	0.023%
94	18.151	2593	2595	2597	rBV3	2951	3163	0.17%	0.028%
95	18.221	2605	2607	2612	rVB5	2231	3040	0.17%	0.027%
96	18.857	2713	2715	2717	rBV3	3096	2872	0.16%	0.025%
97	18.945	2727	2730	2733	rBV4	6032	7214	0.40%	0.063%
98	19.733	2862	2864	2866	rBV3	6855	5557	0.31%	0.049%
99	21.074	3087	3092	3100	rBV	1499367	1814690	100.00%	15.918%
100	23.192	3446	3452	3463	rVB	1048136	1776751	97.91%	15.585%


Sum of corrected areas: 11400275

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052720\
Data File : BM026145.D
Acq On : 27 May 2020 14:53
Operator : MA/SJ
Sample : L2737-15DL2 500X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

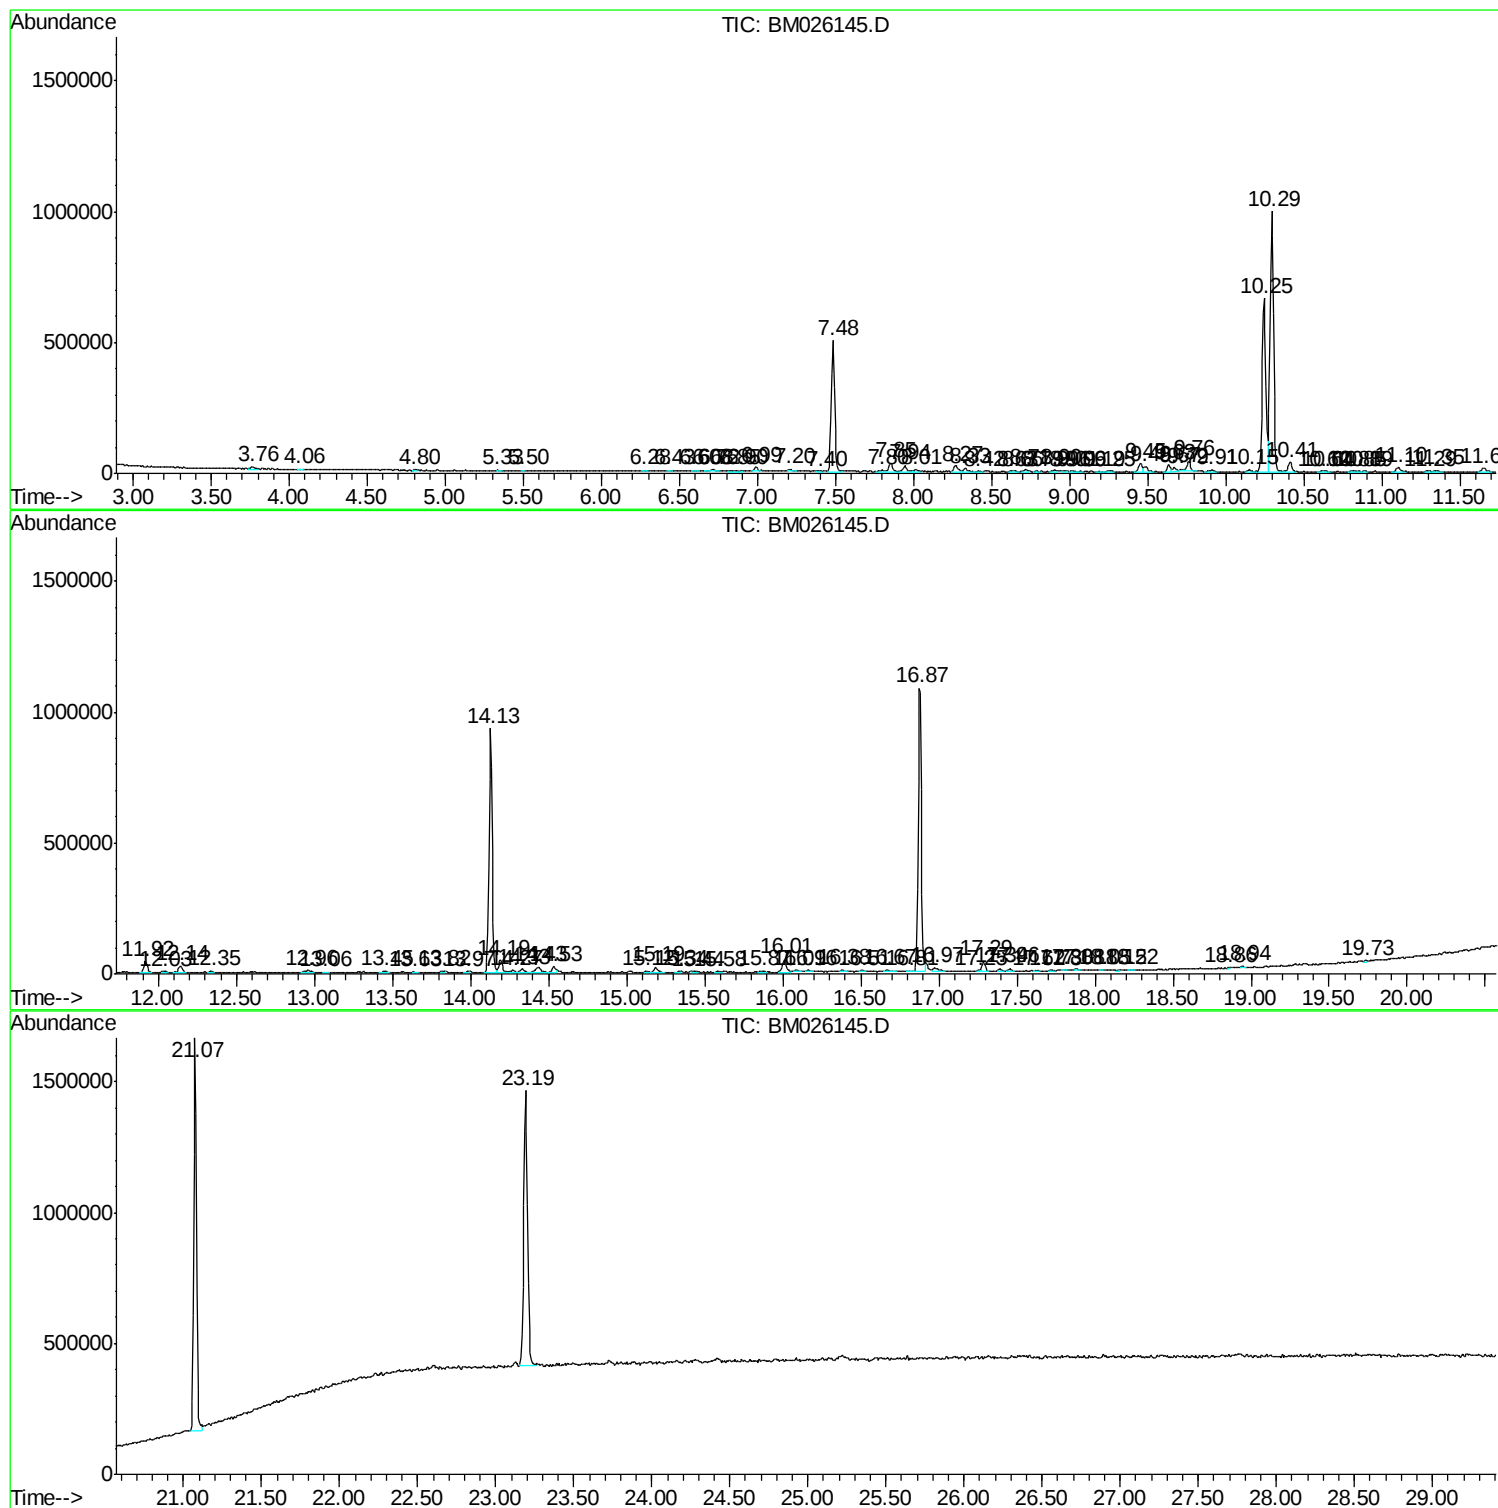

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052720\
Data File : BM026145.D
Acq On : 27 May 2020 14:53
Operator : MA/SJ
Sample : L2737-15DL2 500X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052720\
Data File : BM026145.D
Acq On : 27 May 2020 14:53
Operator : MA/SJ
Sample : L2737-15DL2 500X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B14DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc