
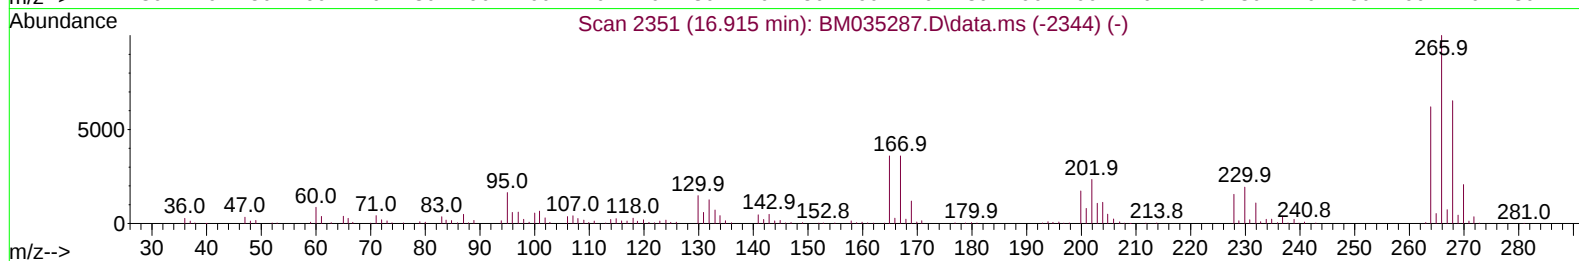
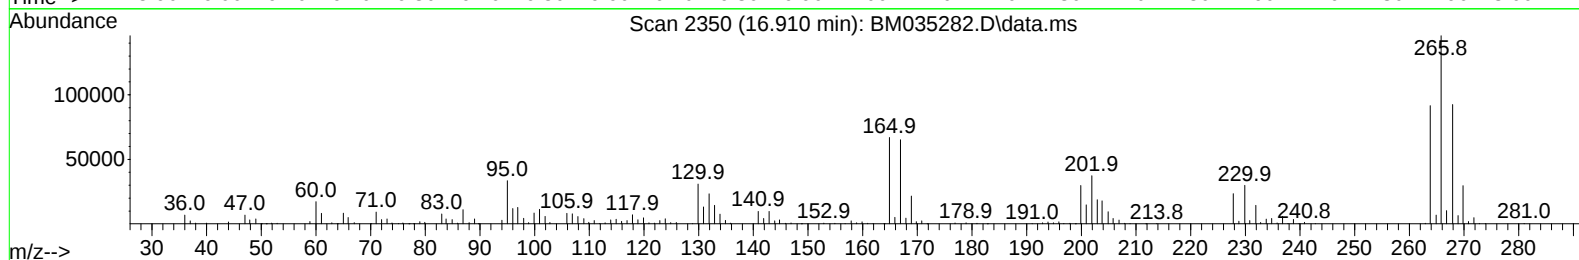


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052722\
Data File : BM035282.D
Acq On : 27 May 2022 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 14:42:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 14:33:09 2022
Response via : Initial Calibration

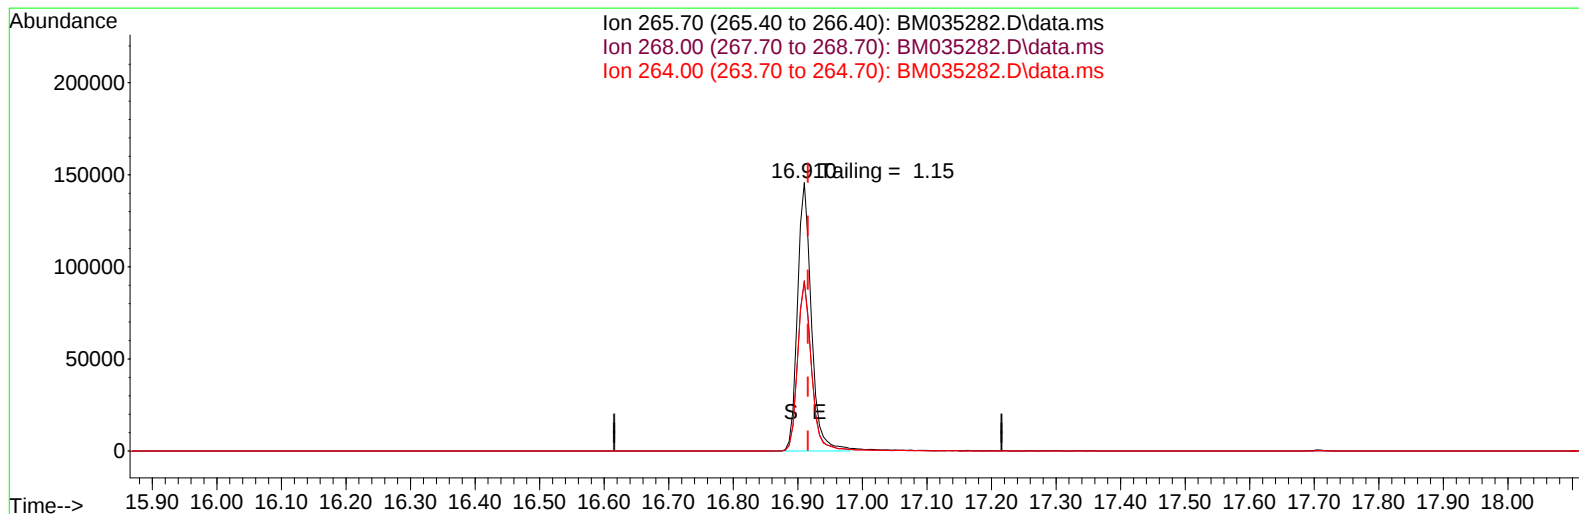

TIC: BM035282.D\data.ms

(70) Pentachlorophenol (C)




16.910min (-0.006) 0.00 ng

response 222463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.30	62.83
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052722\  
Data File : BM035282.D  
Acq On    : 27 May 2022  10:41  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 27 14:42:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 14:33:09 2022
Response via : Initial Calibration

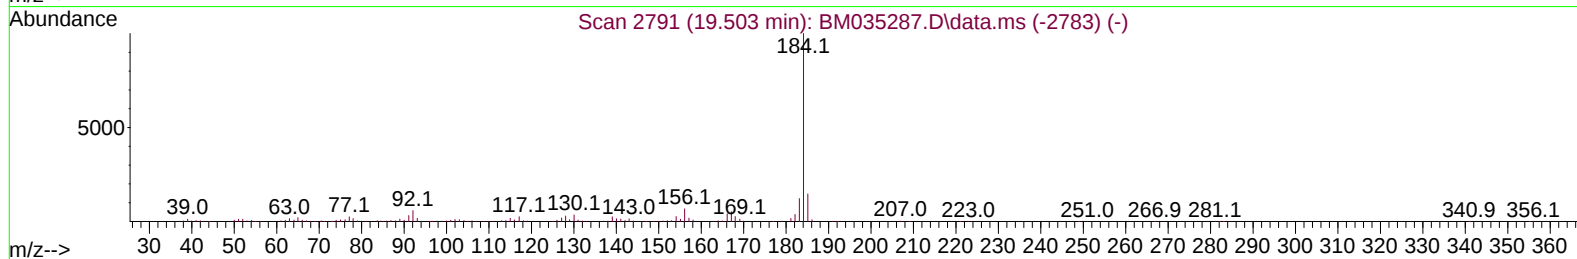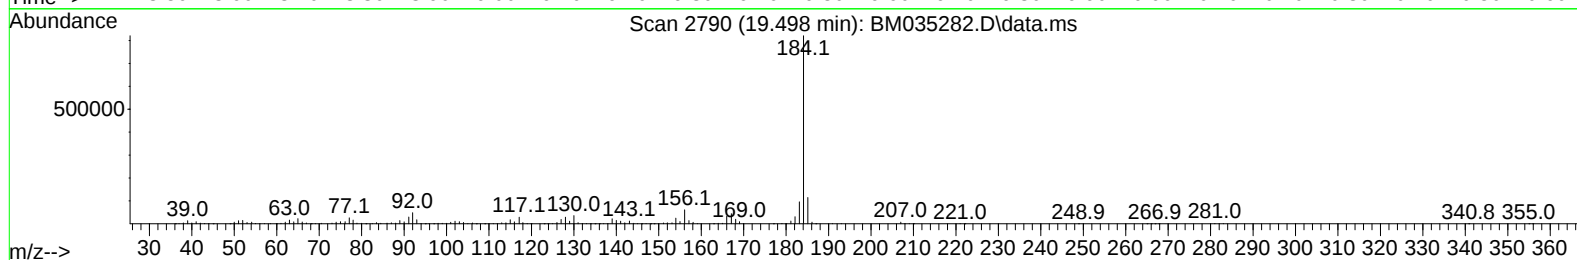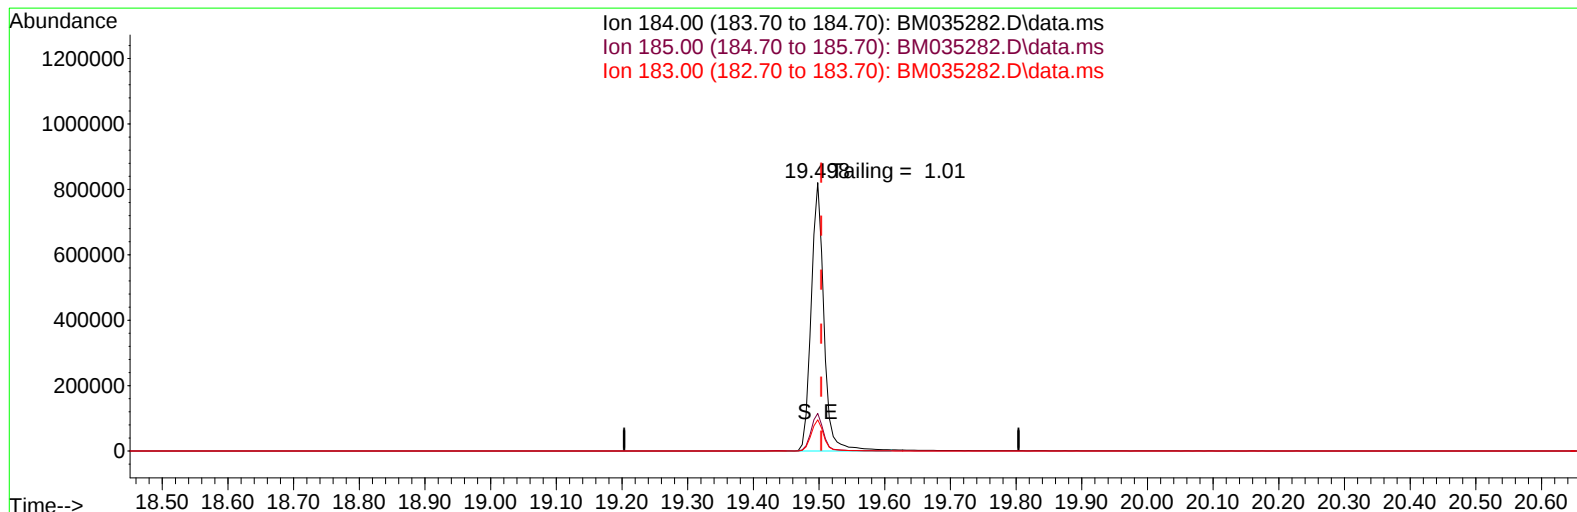

TIC: BM035282.D\data.ms

(77) Benzidine

19.498min (-0.006) 569975.17 ng

response **1117073**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.01
183.00	11.90	11.66
0.00	0.00	0.00