


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052722\
 Data File : BM035282.D
 Acq On : 27 May 2022 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 16:44:39 2022

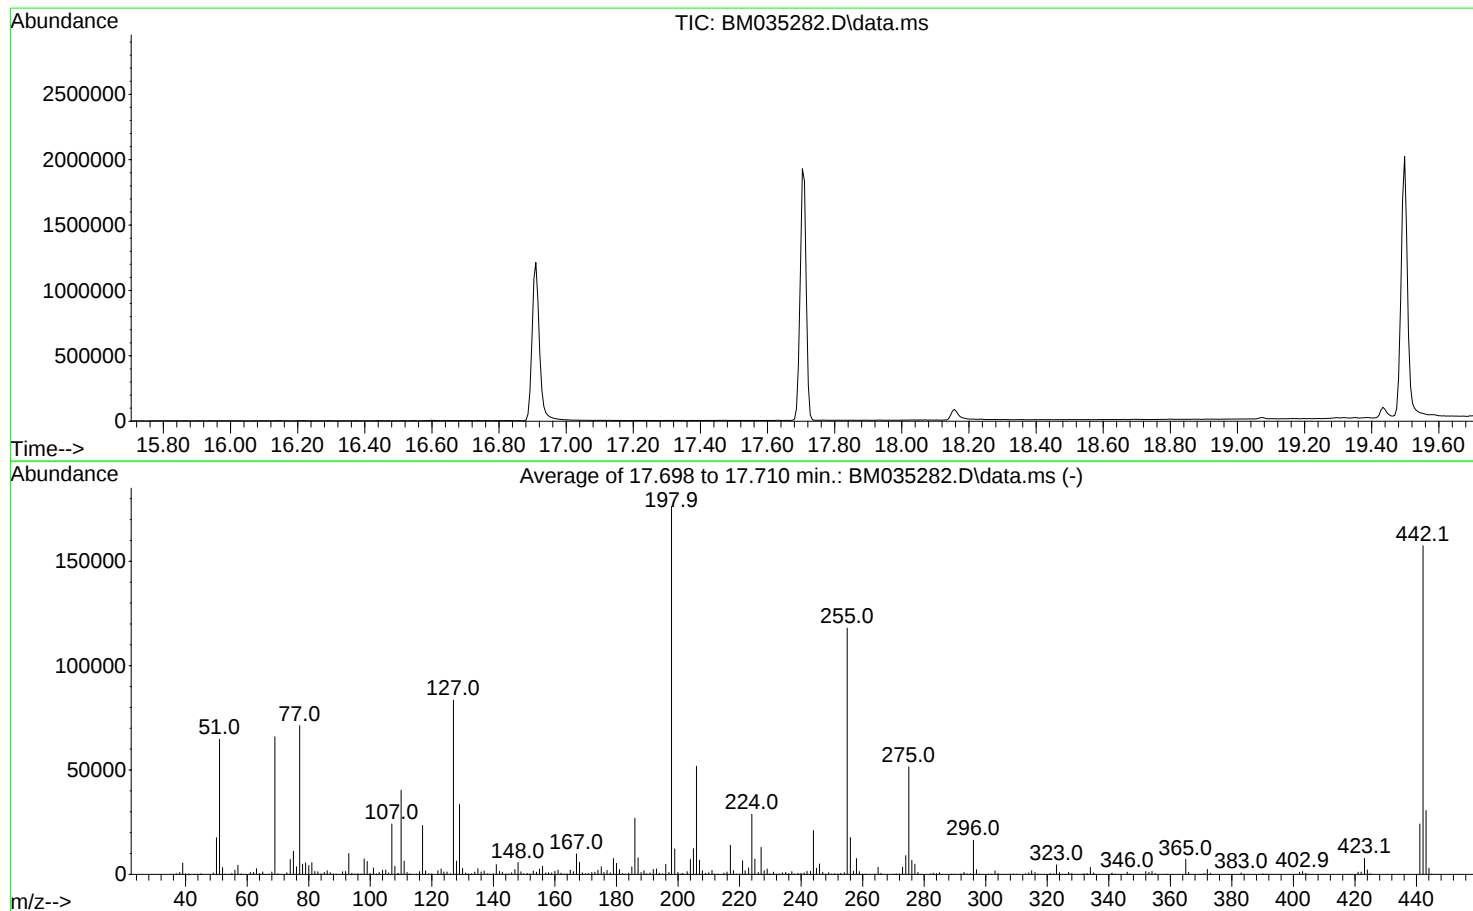

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	64712	PASS
68	69	0.00	2	1.7	1150	PASS
69	198	0.00	100	37.4	65925	PASS
70	69	0.00	2	0.5	336	PASS
127	198	10	80	47.4	83504	PASS
197	198	0.00	2	0.5	933	PASS
198	198	100	100	100.0	176259	PASS
199	198	5	9	6.9	12205	PASS
275	198	10	60	29.2	51499	PASS
365	198	1	100	4.1	7206	PASS
441	198	0.01	100	13.7	24140	PASS
442	442	50	100	100.0	157517	PASS
443	442	15	24	19.4	30595	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2022	BNA_M	<u>BM035282.D</u>
Compound Name	Response	Retention Time
DDT	647808	20.73
DDD	2357	20.29
DDE	356	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2713	650521	0.42

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052722\
Data File : BM035282.D
Acq On : 27 May 2022 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 27 14:42:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 14:33:09 2022
Response via : Initial Calibration

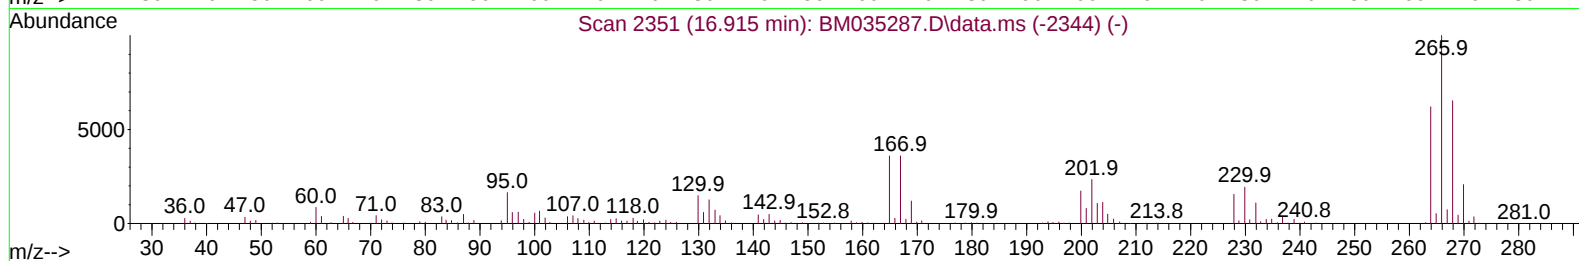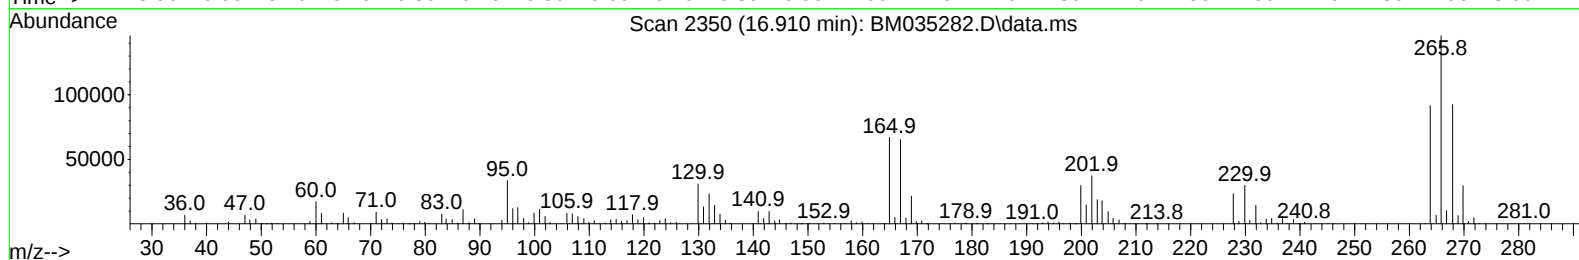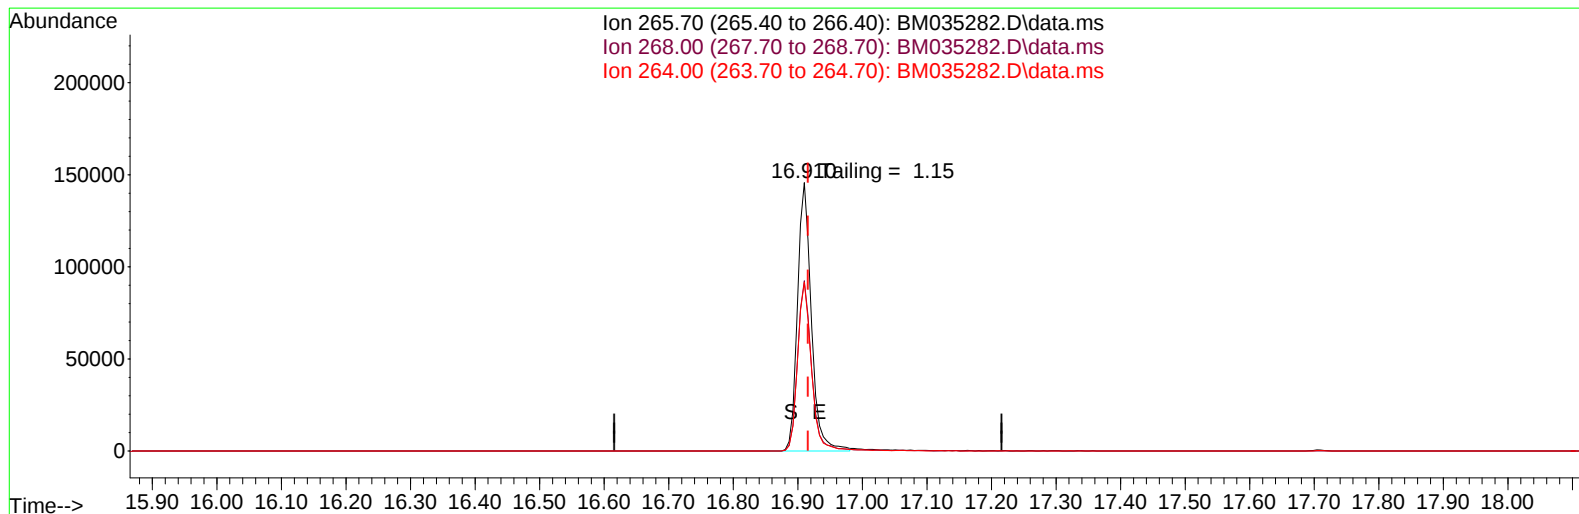

TIC: BM035282.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 0.00 ng




response 222463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.30	62.83
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052722\  
Data File : BM035282.D  
Acq On    : 27 May 2022  10:41  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 27 14:42:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri May 27 14:33:09 2022
Response via : Initial Calibration

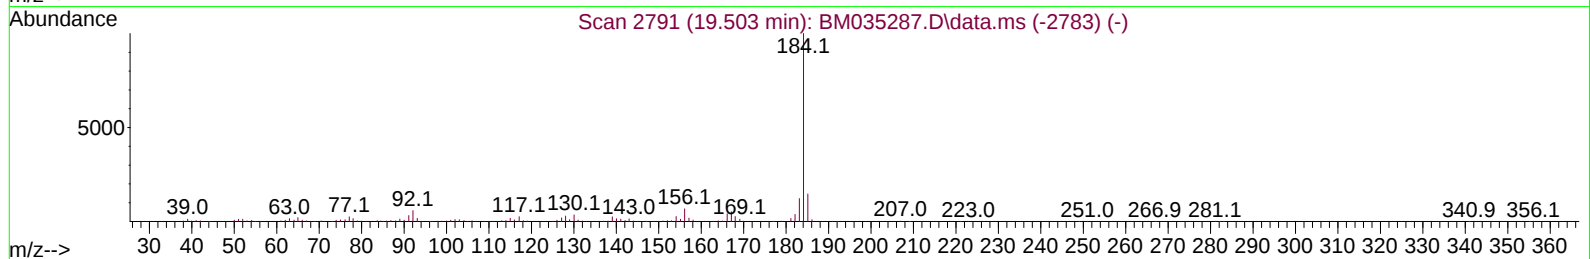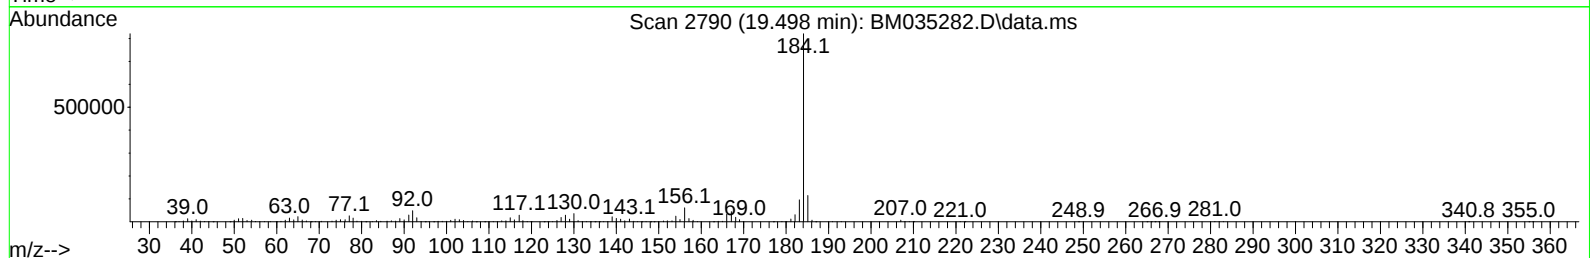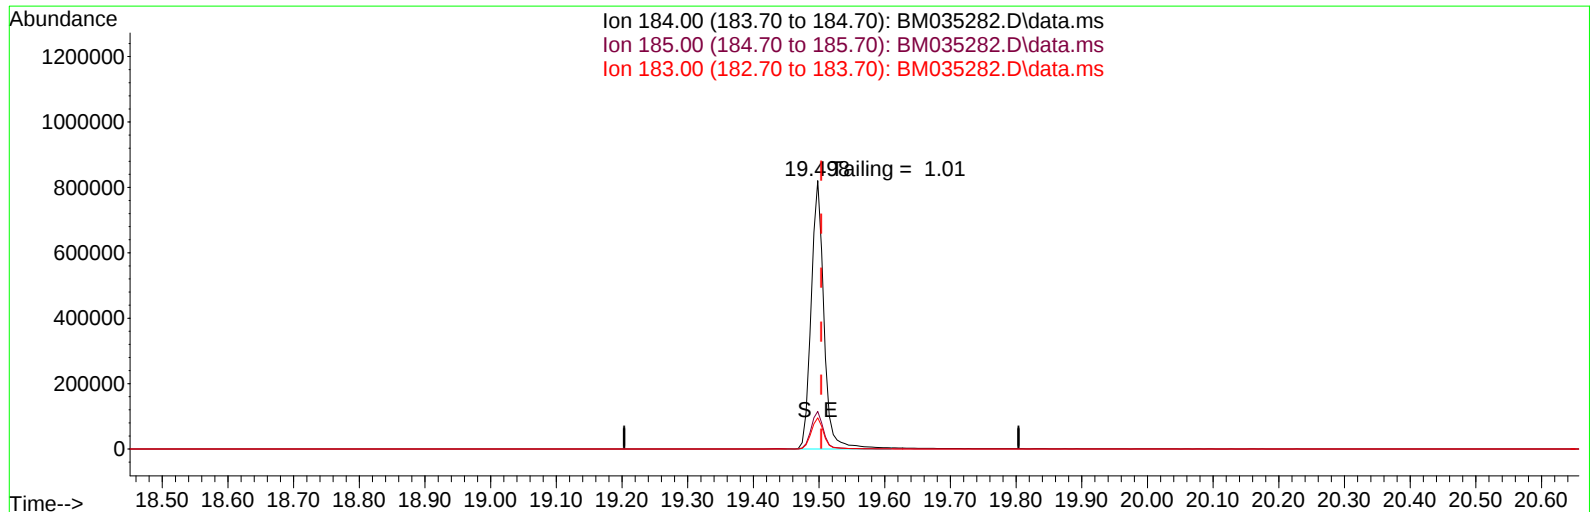

TIC: BM035282.D\data.ms

(77) Benzidine

19.498min (-0.006) 569975.17 ng

response **1117073**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.01
183.00	11.90	11.66
0.00	0.00	0.00