



bis(2-Chloroethoxy)methane

Response Ratio

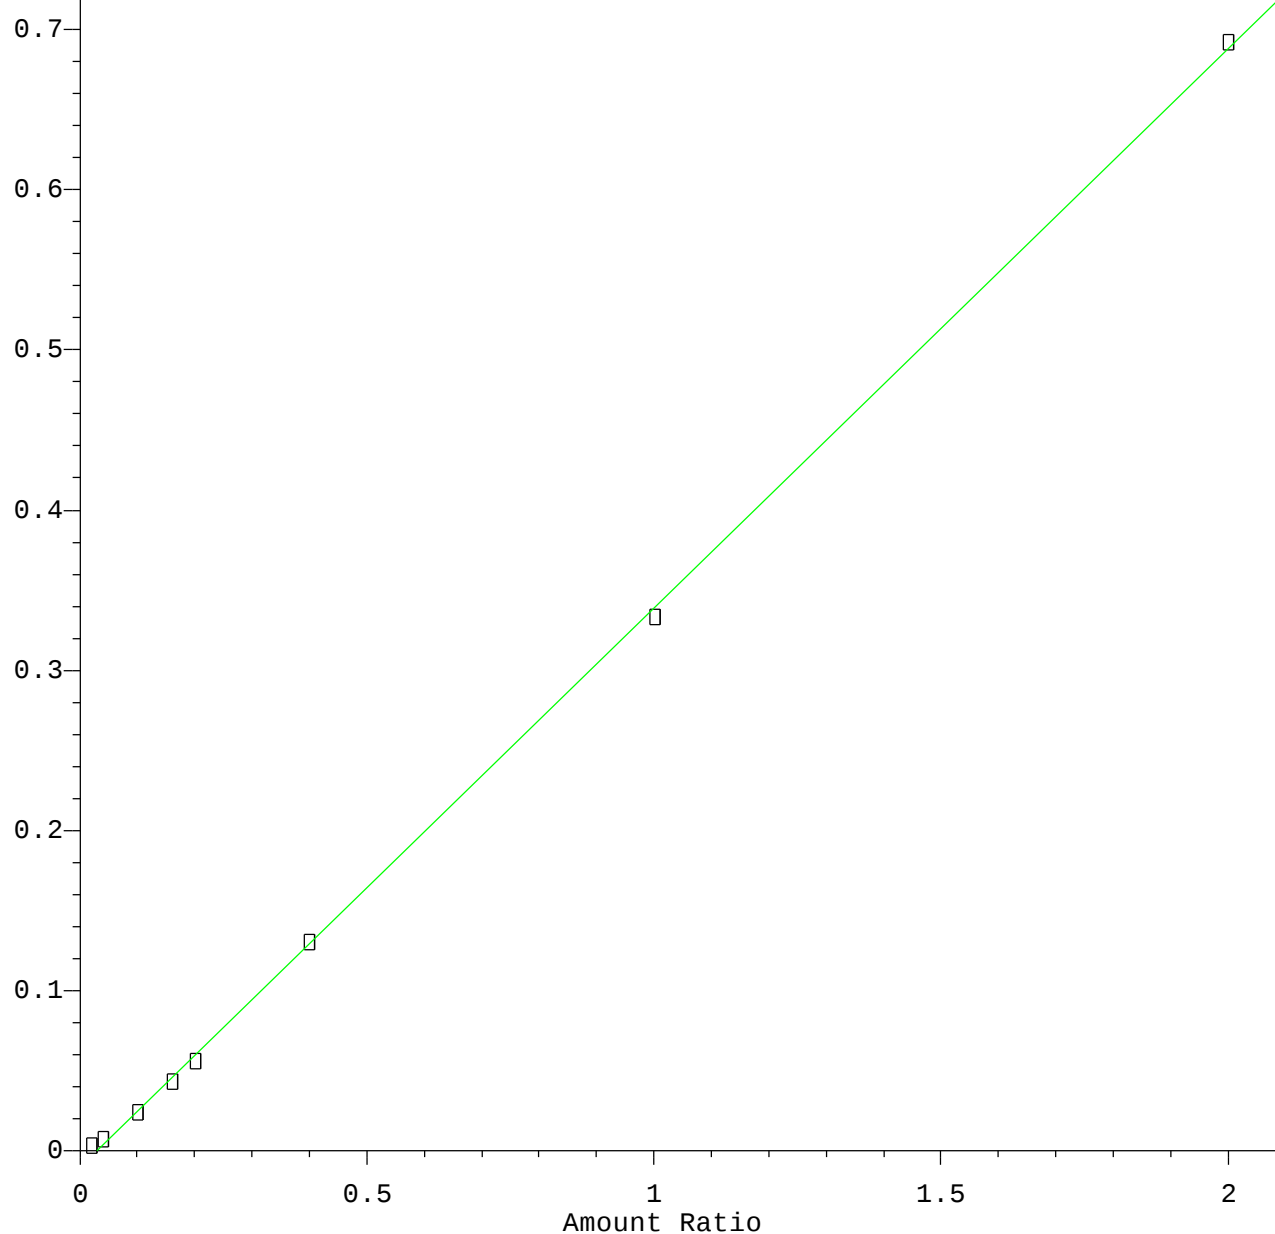

Resp Ratio = $3.49 \times 10^{-1} \times \text{Amt} - 1.01 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Calibration Table Last Updated: Thu May 28 15:41:25 2015

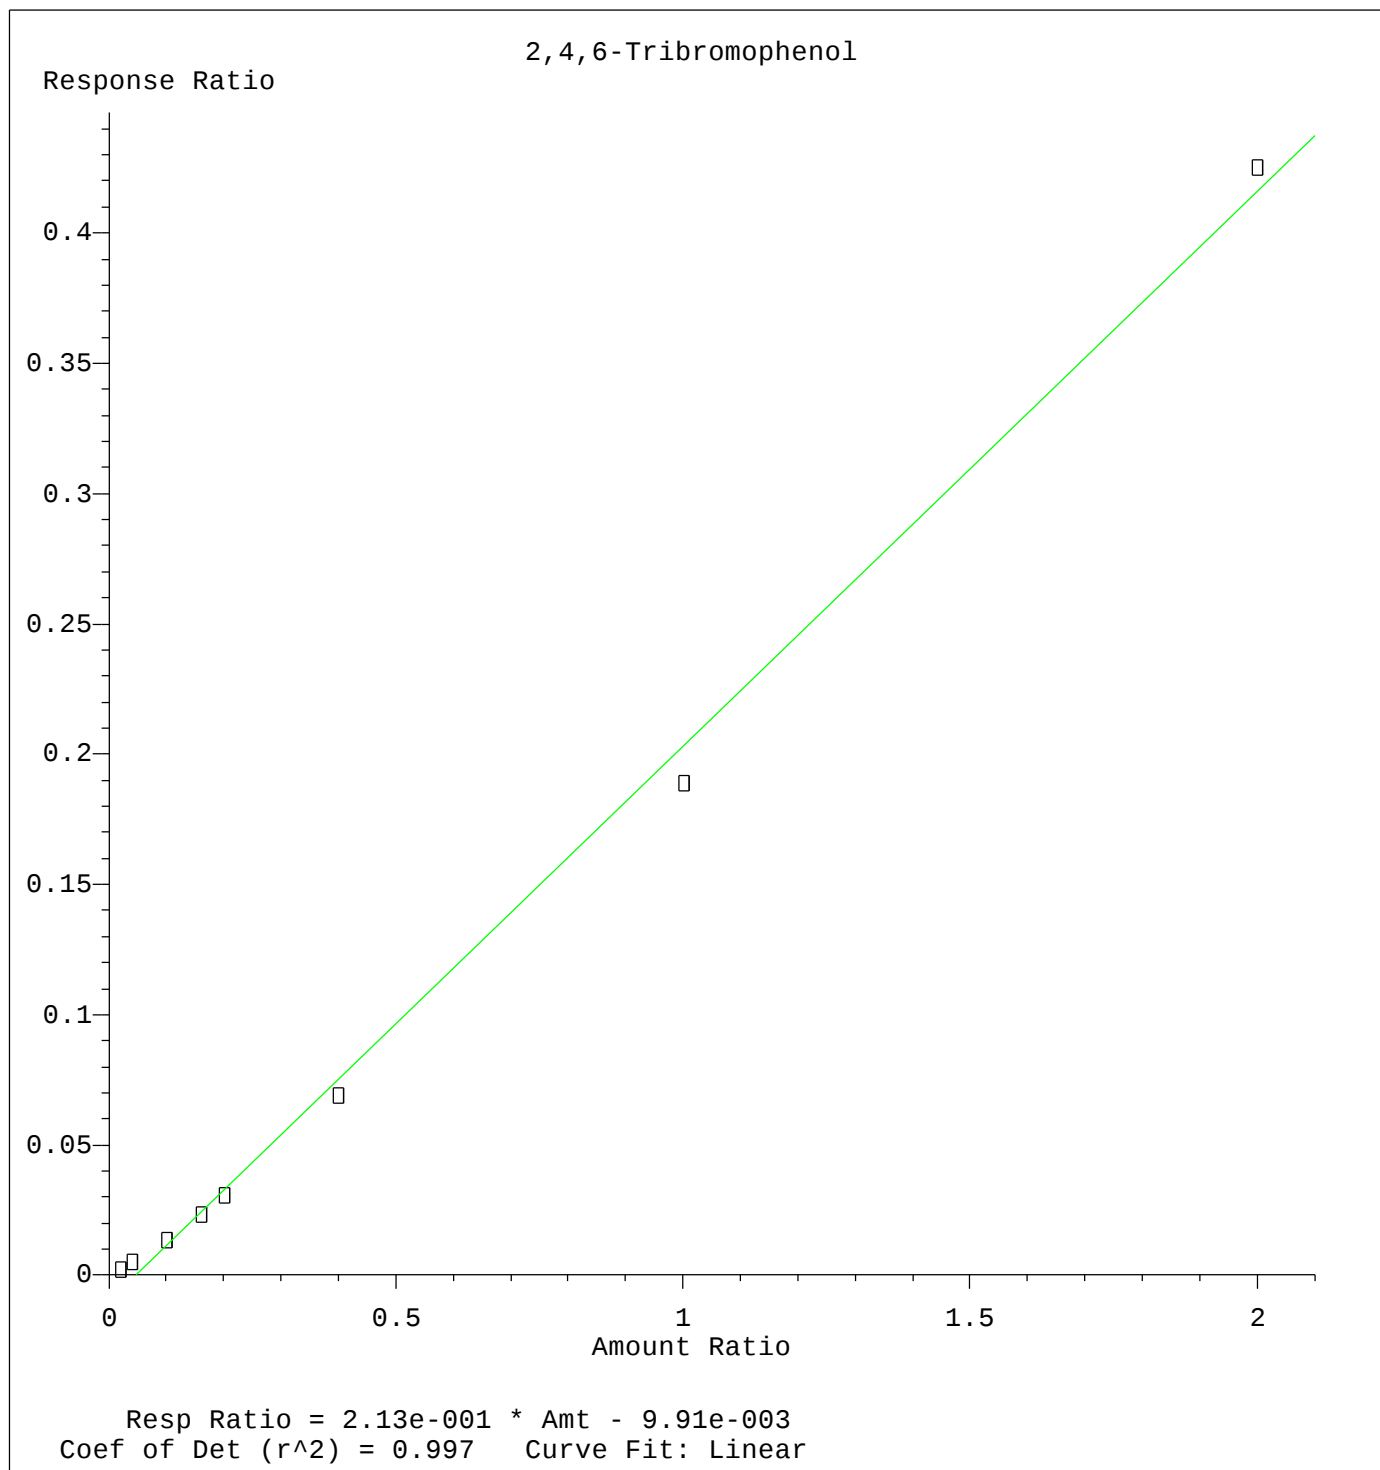

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Calibration Table Last Updated: Thu May 28 15:41:25 2015


2,6-Dinitrotoluene

Response Ratio

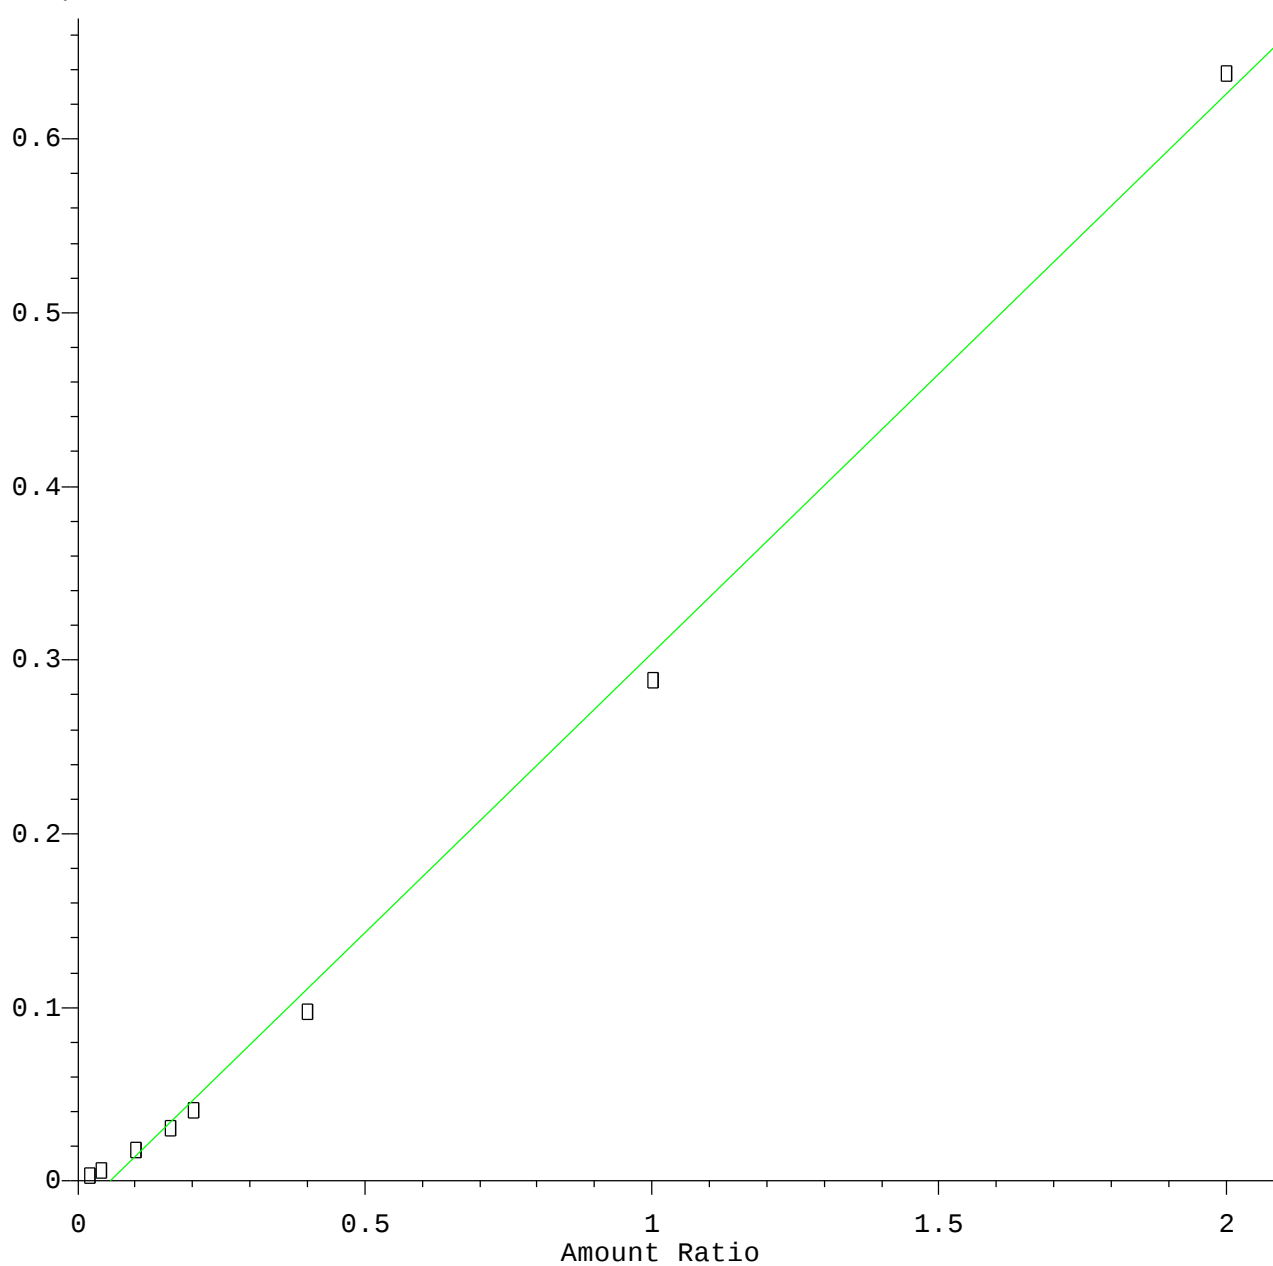

Resp Ratio = $3.22 \times 10^{-1} \times \text{Amt} - 1.76 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Calibration Table Last Updated: Thu May 28 15:41:25 2015

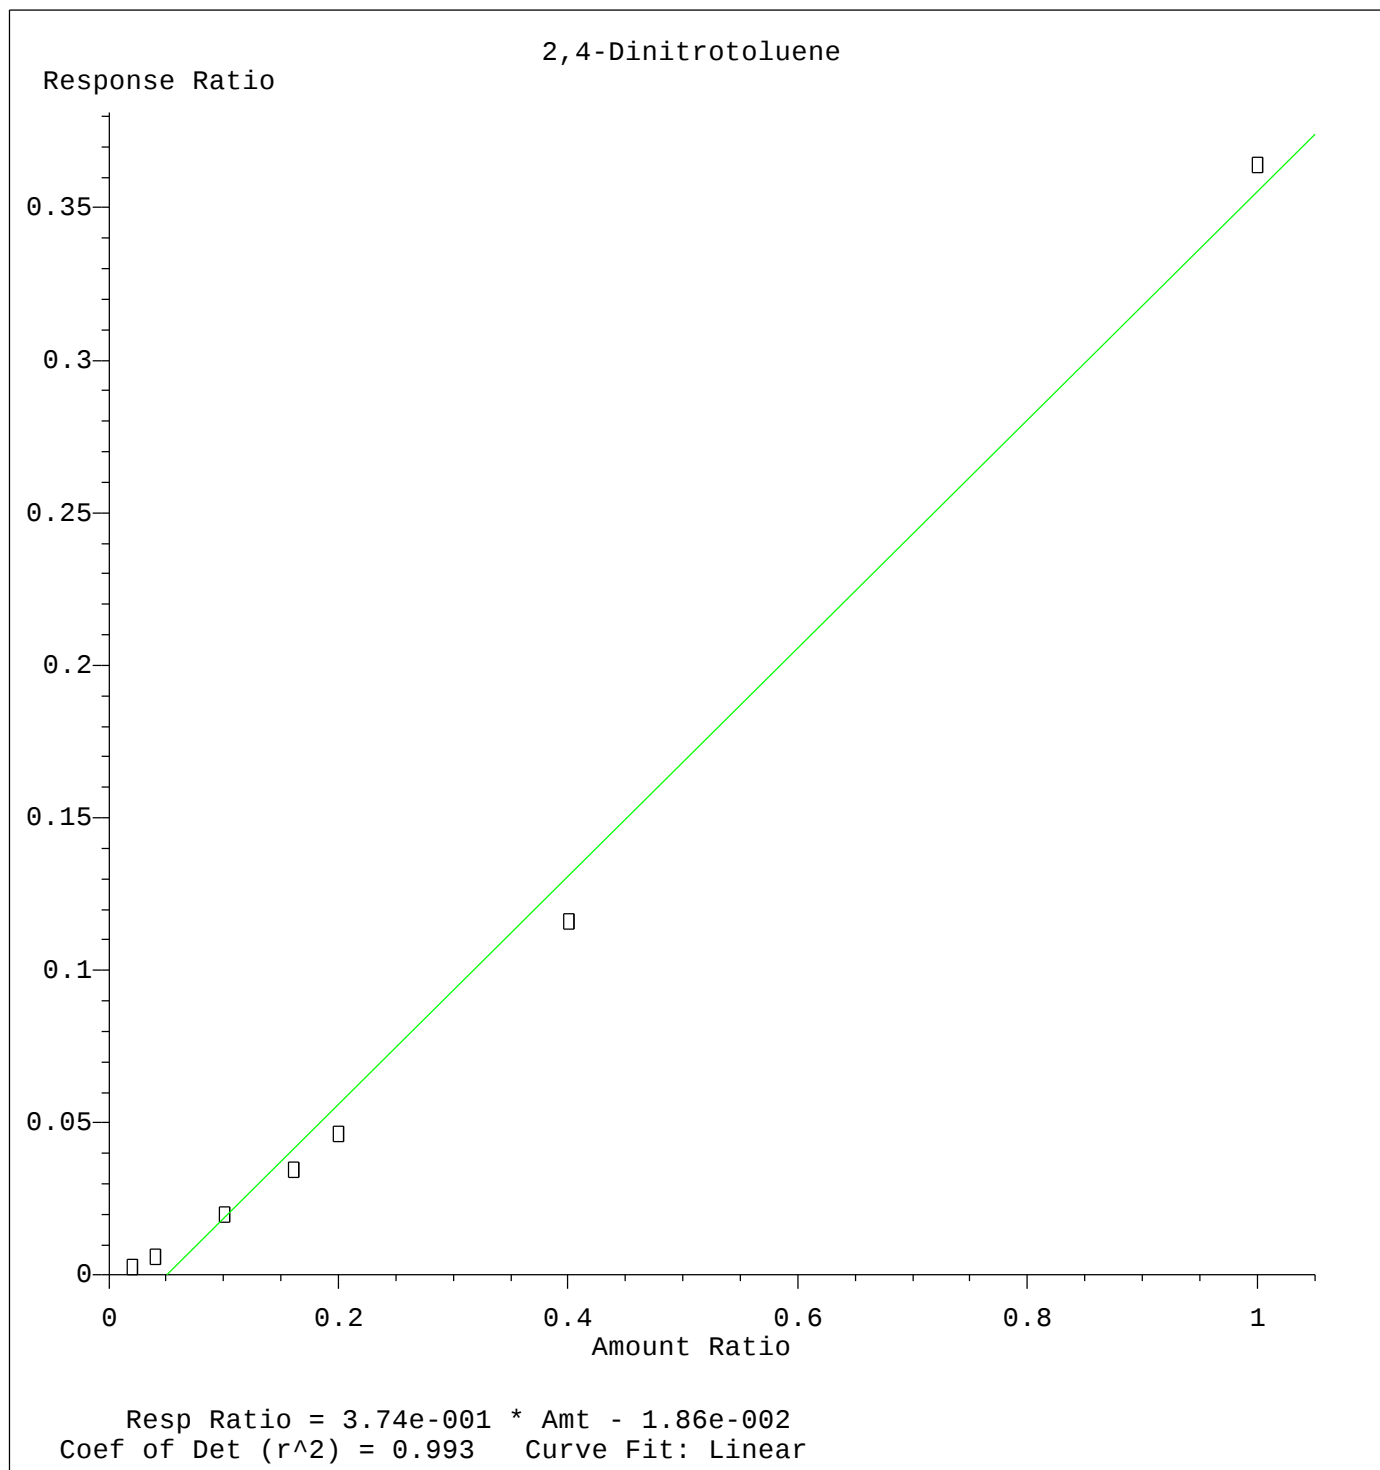

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Calibration Table Last Updated: Thu May 28 15:41:25 2015

3,3'-Dichlorobenzidine

Response Ratio

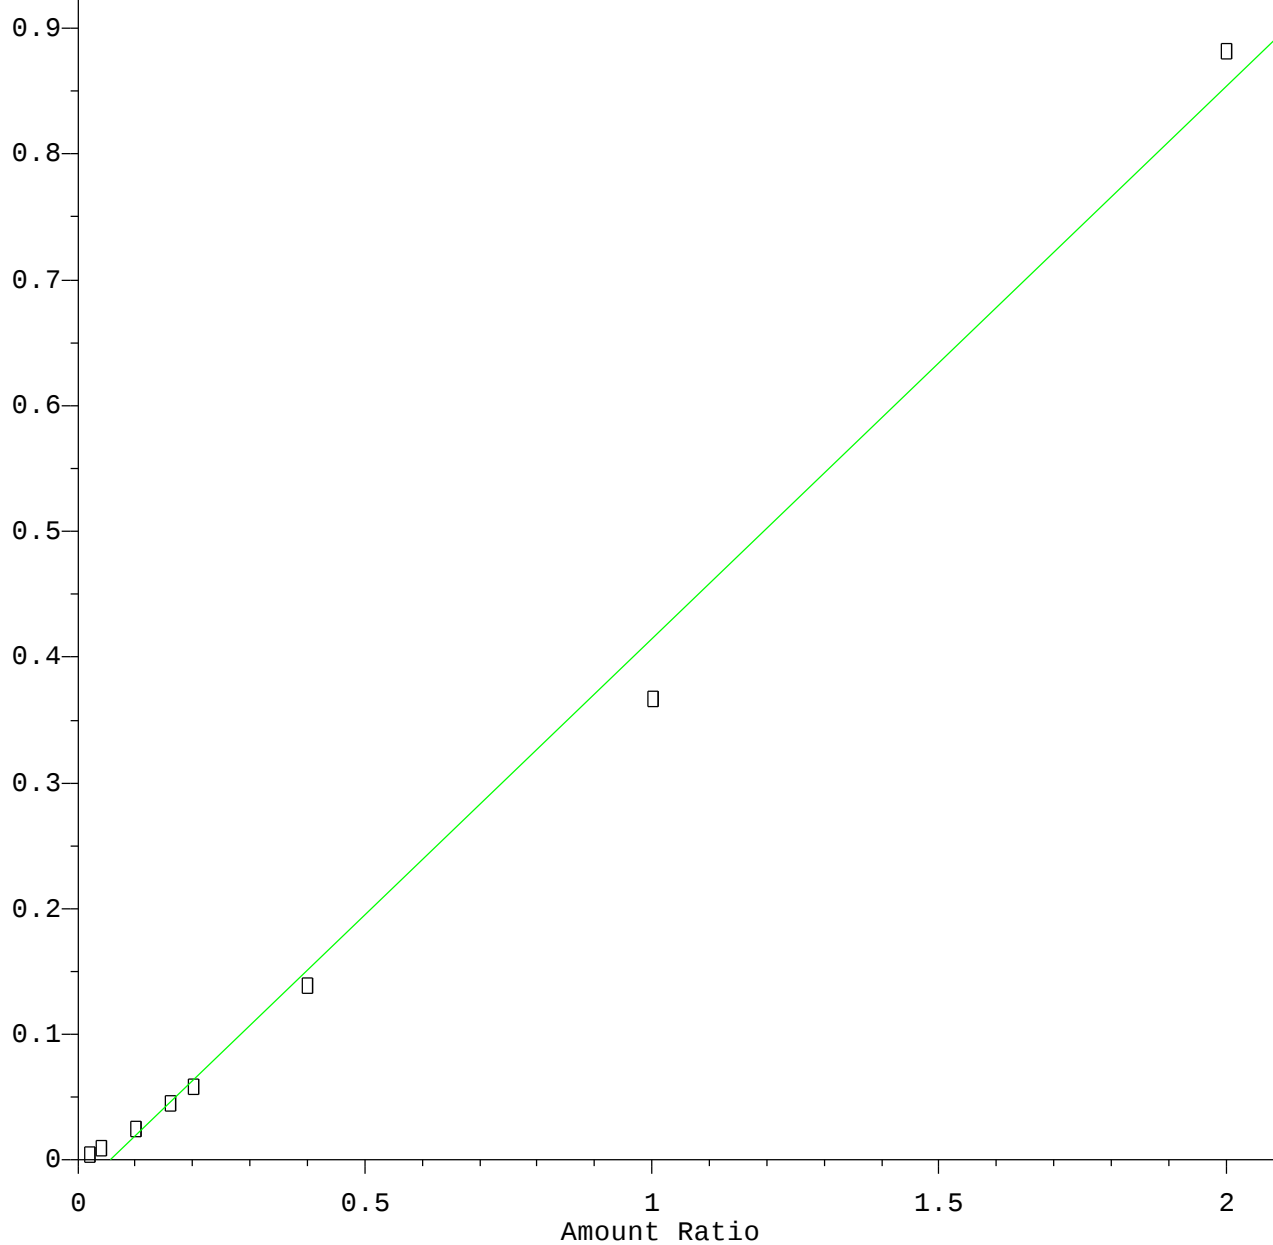

Resp Ratio = $4.39 \times 10^{-1} \times \text{Amt} - 2.47 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Calibration Table Last Updated: Thu May 28 15:41:25 2015