

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052815\
 Data File : BM001438.D
 Acq On : 28 May 2015 22:42
 Operator : TP/IZ
 Sample : G2406-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 KM-SP-002-150518

Quant Time: May 29 04:12:30 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 03:45:53 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	11569	5.00	ng	0.00
6) Naphthalene-d8	10.16	136	38041	5.00	ng	0.00
9) Acenaphthene-d10	14.07	164	23592	5.00	ng	0.00
15) Phenanthrene-d10	16.81	188	54822	5.00	ng	0.00
17) Chrysene-d12	21.02	240	50627	5.00	ng	0.00
21) Perylene-d12	23.11	264	43471	5.00	ng	0.00
System Monitoring Compounds						
2) 2-Fluorophenol	4.97	112	15696	8.86	ng	0.00
3) Phenol-d6	6.57	99	19368	10.36	ng	-0.03
7) Nitrobenzene-d5	8.53	82	12568	6.19	ng	0.00
10) 2,4,6-Tribromophenol	15.57	330	7556	7.75	ng	0.00
11) 2-Fluorobiphenyl	12.68	172	39722	6.07	ng	0.00
18) Terphenyl-d14	19.47	244	38774	6.16	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052815\
Data File : BM001438.D
Acq On : 28 May 2015 22:42
Operator : TP/IZ
Sample : G2406-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
KM-SP-002-150518

Quant Time: May 29 04:12:30 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 03:45:53 2015
Response via : Initial Calibration

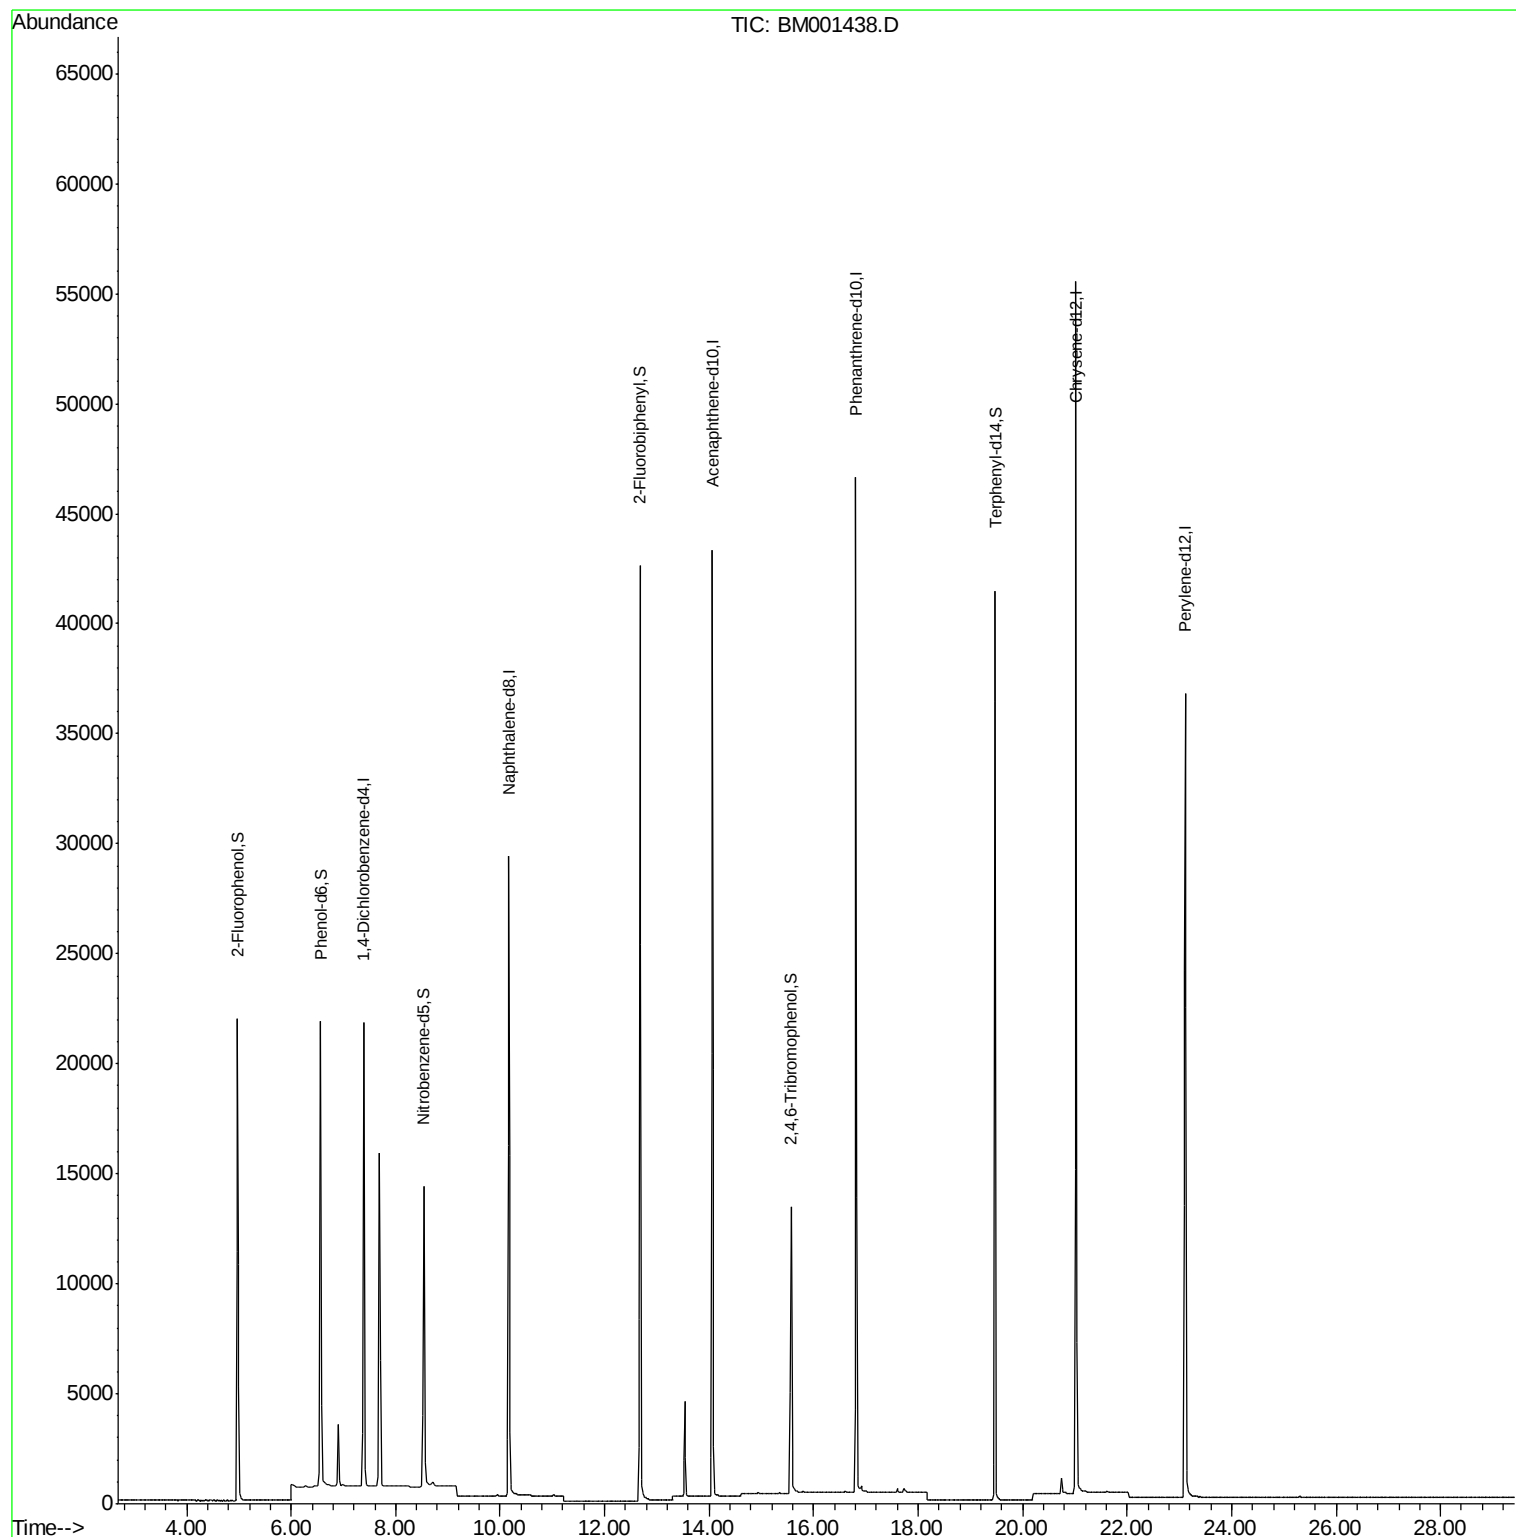

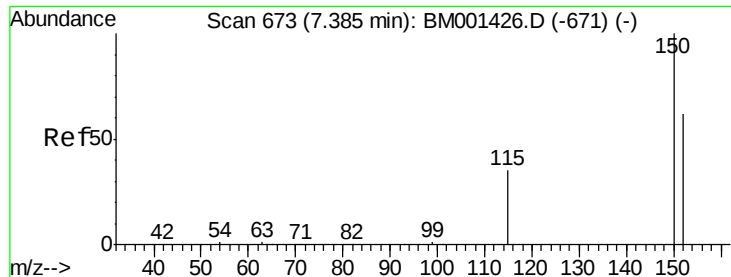


#1




1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.38 min Scan# 673
Delta R.T. 0.00 min
Lab File: BM001438.D
Acq: 28 May 2015 22:42

Instrument :
BNA_M
ClientSampleId :
KM-SP-002-150518

Tgt Ion:152 Resp: 11569
Ion Ratio Lower Upper
152 100
150 152.1 128.4 192.6
115 46.7 45.6 68.4

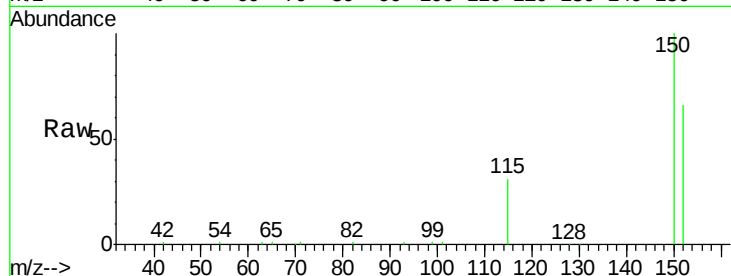


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

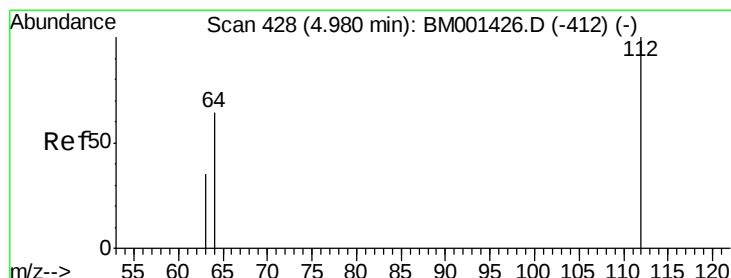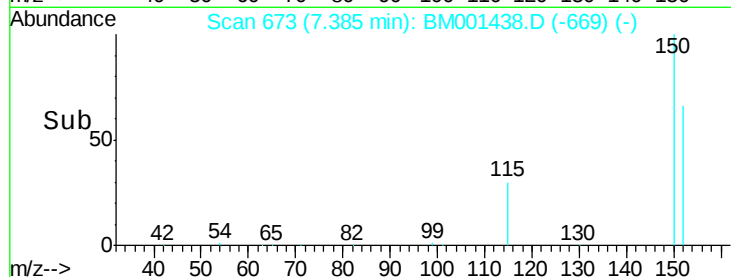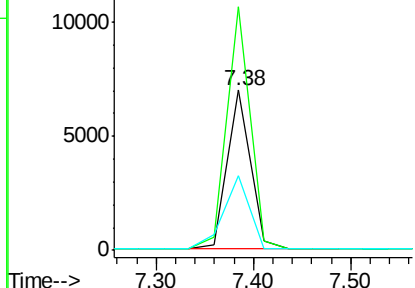



#2


2-Fluorophenol
Concen: 8.86 ng
RT: 4.97 min Scan# 427
Delta R.T. -0.01 min
Lab File: BM001438.D
Acq: 28 May 2015 22:42

Tgt Ion:112 Resp: 15696
Ion Ratio Lower Upper
112 100
64 64.1 52.1 78.1
63 35.6 30.2 45.2

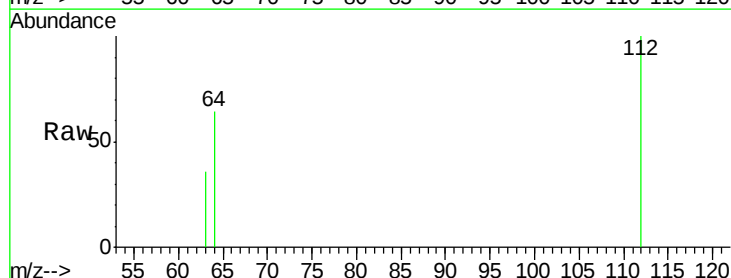

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

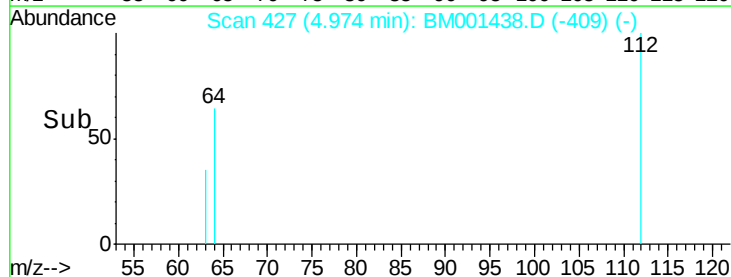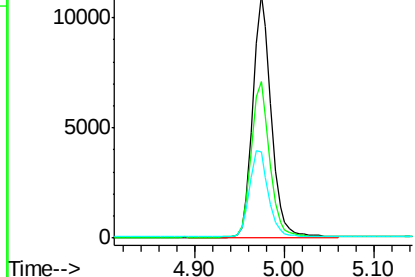

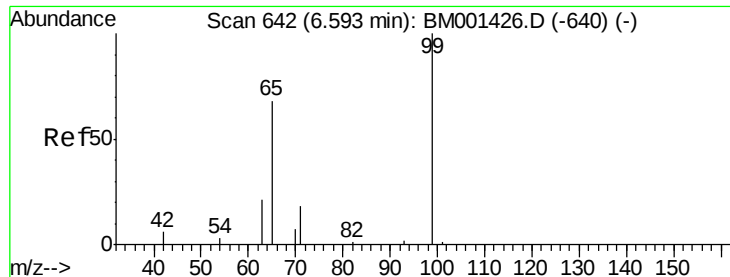

#3

Phenol-d6

Concen: 10.36 ng

RT: 6.57 min Scan# 641

Delta R.T. -0.03 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42

Instrument :

BNA_M

ClientSampleId :

KM-SP-002-150518


Tgt Ion: 99 Resp: 19368

Ion Ratio Lower Upper

99 100

42 30.2 13.7 20.5#




71 49.4 19.8 29.6#

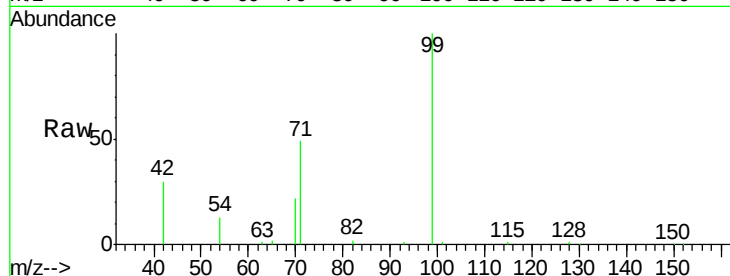

Abundance Ion 99.00 (98.70 to 99.70): BM001426.D (-640) (-)

Ion 42.00 (41.70 to 42.70): BM001426.D (-640) (-)

Ion 71.00 (70.70 to 71.70): BM001426.D (-640) (-)

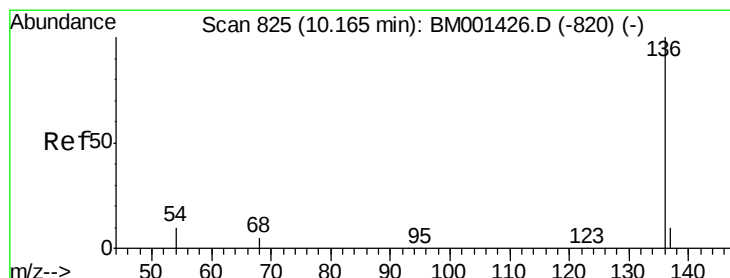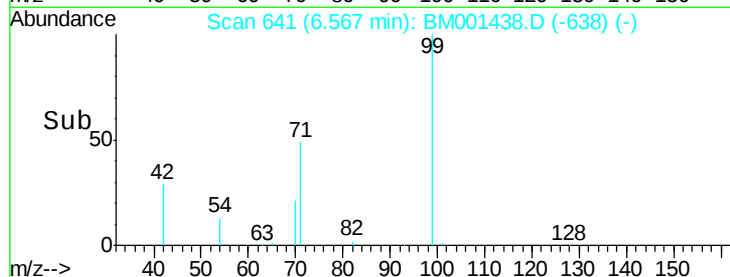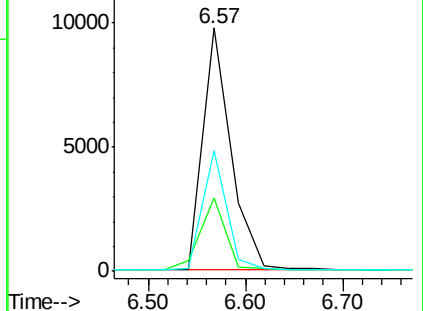

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.16 min Scan# 825

Delta R.T. 0.00 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42

Tgt Ion: 136 Resp: 38041


Ion Ratio Lower Upper

136 100

137 10.8 8.3 12.5

54 8.7 8.2 12.4

68 5.0 4.5 6.7


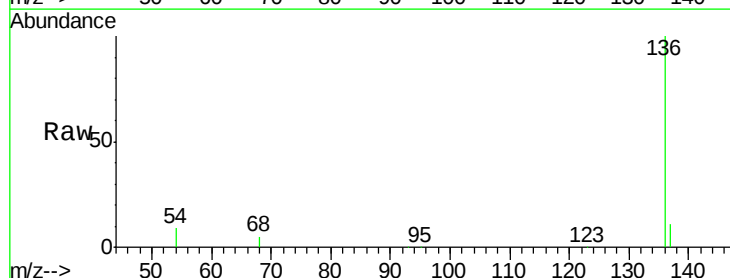



Abundance Ion 136.00 (135.70 to 136.70): BM001426.D (-820) (-)

Ion 137.00 (136.70 to 137.70): BM001426.D (-820) (-)

Ion 54.00 (53.70 to 54.70): BM001426.D (-820) (-)

Ion 68.00 (67.70 to 68.70): BM001426.D (-820) (-)

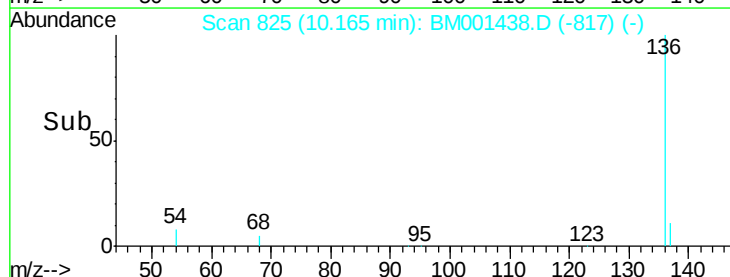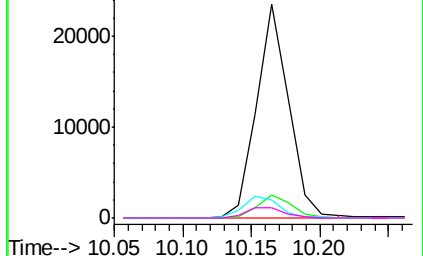

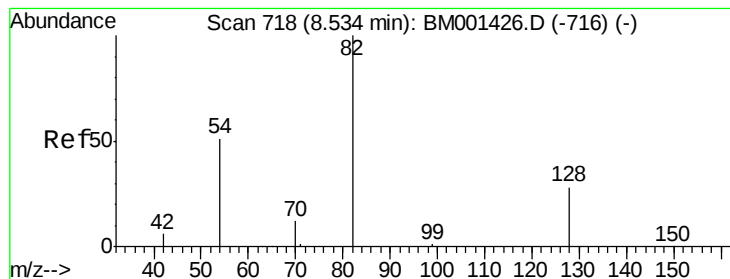

#7

Nitrobenzene-d5

Concen: 6.19 ng

RT: 8.53 min Scan# 718

Delta R.T. 0.00 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42

Instrument :

BNA_M

ClientSampleId :

KM-SP-002-150518


Tgt Ion: 82 Resp: 12568

Ion Ratio Lower Upper

82 100

128 38.1 24.4 36.6#




54 38.3 42.3 63.5#

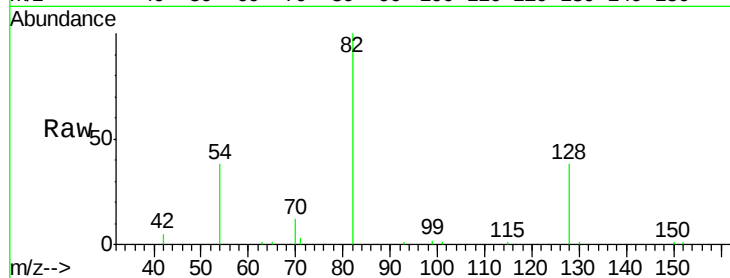

Abundance Ion 82.00 (81.70 to 82.70): BM001426.D (-716) (-)

Ion 128.00 (127.70 to 128.70): BM001426.D (-716) (-)

Ion 54.00 (53.70 to 54.70): BM001426.D (-716) (-)

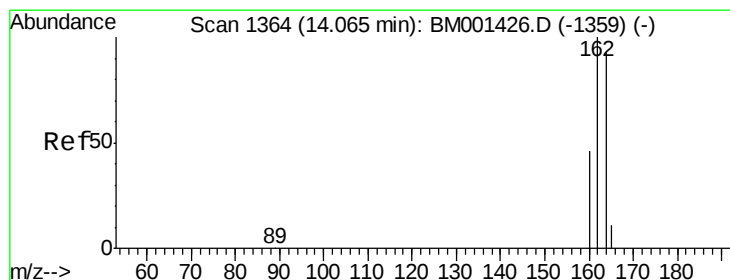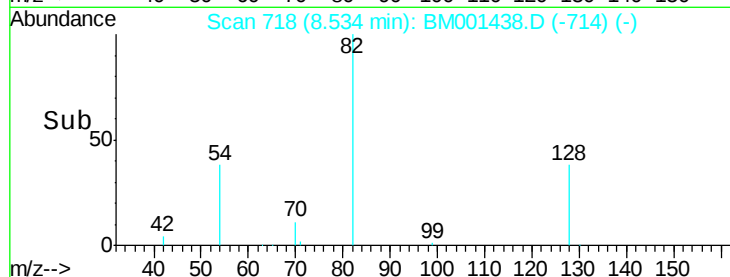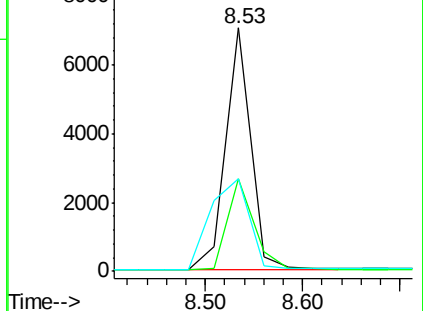

#9

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.07 min Scan# 1364

Delta R.T. 0.00 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42


Tgt Ion: 164 Resp: 23592

Ion Ratio Lower Upper

164 100

162 104.0 86.2 129.2



160 46.1 39.4 59.2

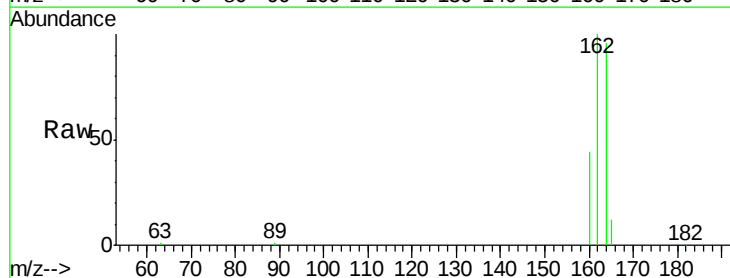


Abundance Ion 164.00 (163.70 to 164.70): BM001426.D (-1359) (-)

Ion 162.00 (161.70 to 162.70): BM001426.D (-1359) (-)

Ion 160.00 (159.70 to 160.70): BM001426.D (-1359) (-)

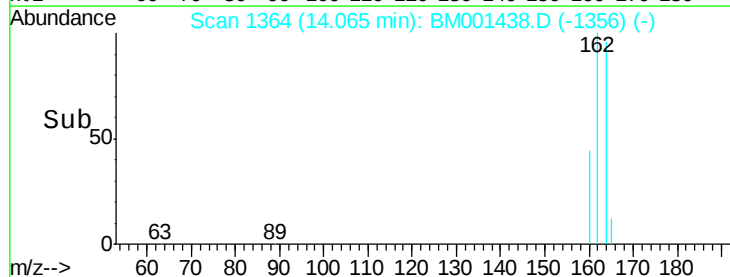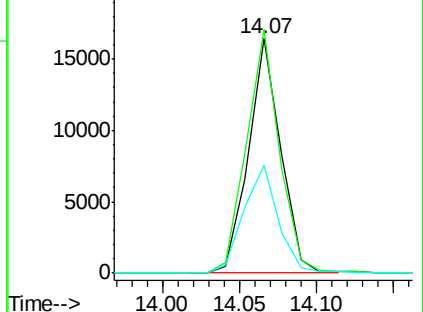


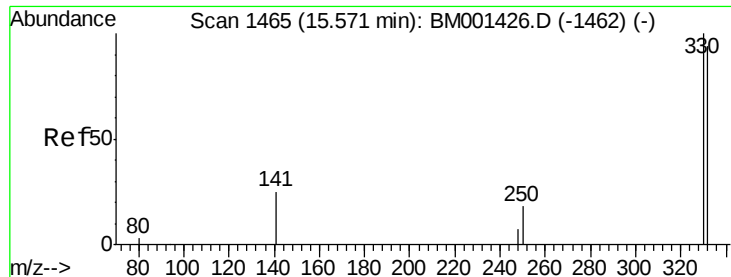




#10
 2,4,6-Tribromophenol
 Concen: 7.75 ng
 RT: 15.57 min Scan# 1465
 Delta R.T. 0.00 min
 Lab File: BM001438.D
 Acq: 28 May 2015 22:42

Instrument :
 BNA_M
 ClientSampleId :
 KM-SP-002-150518

Tgt Ion:330 Resp: 7556
 Ion Ratio Lower Upper
 330 100
 332 97.4 76.3 114.5
 141 43.5 35.0 52.4

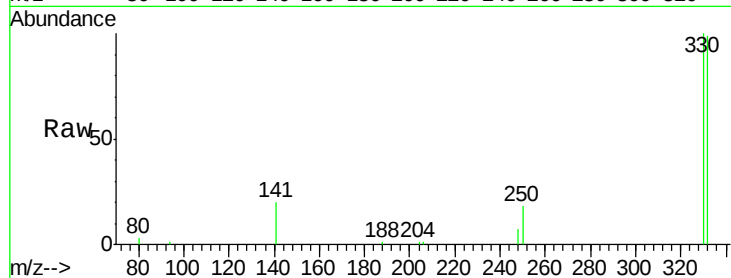


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

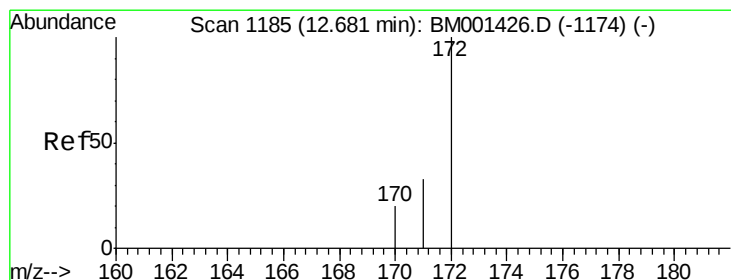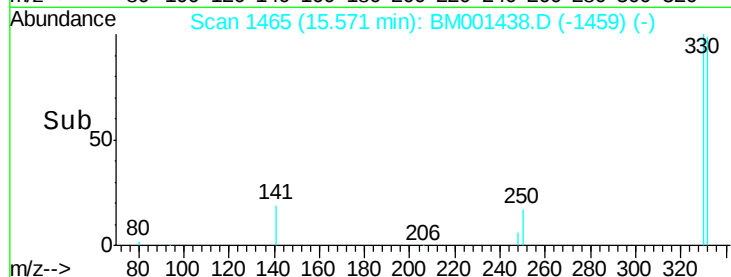
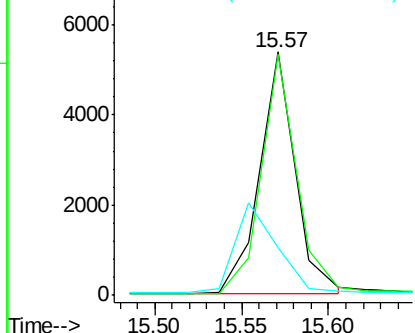



#11
 2-Fluorobiphenyl
 Concen: 6.07 ng
 RT: 12.68 min Scan# 1184
 Delta R.T. -0.01 min
 Lab File: BM001438.D
 Acq: 28 May 2015 22:42

Tgt Ion:172 Resp: 39722
 Ion Ratio Lower Upper
 172 100
 171 34.8 26.9 40.3
 170 23.2 17.1 25.7

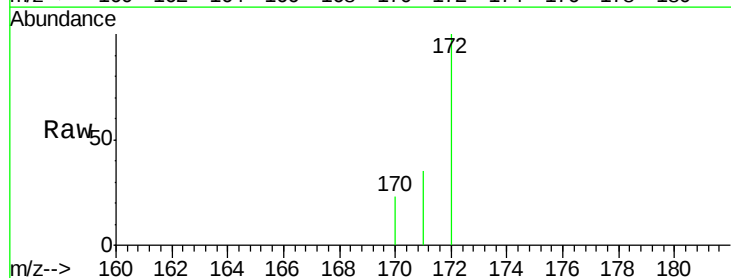

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

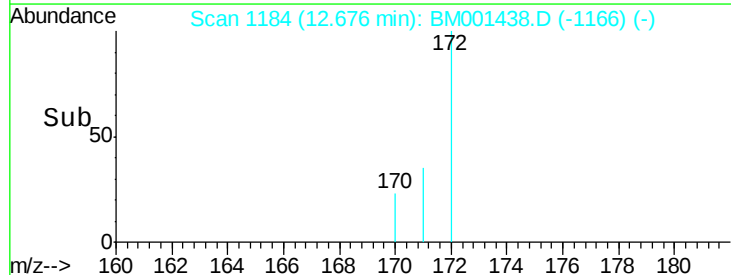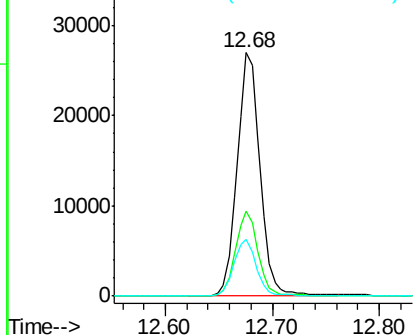

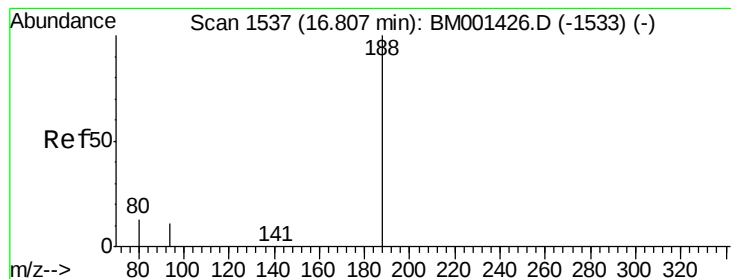

#15

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.81 min Scan# 1537

Delta R.T. 0.00 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42

Instrument :

BNA_M

ClientSampleId :

KM-SP-002-150518


Tgt Ion:188 Resp: 54822

Ion Ratio Lower Upper

188 100

94 10.3 9.0 13.4




80 11.5 10.6 15.8

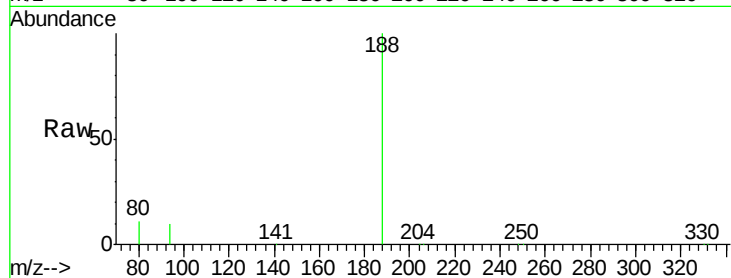

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

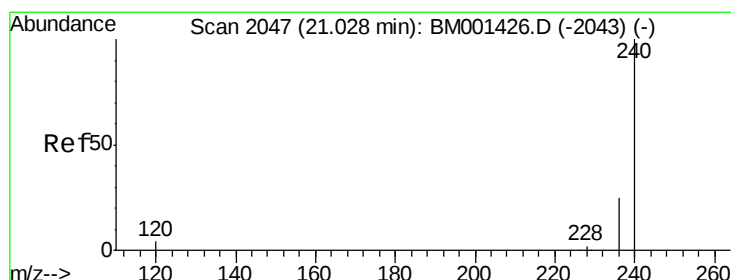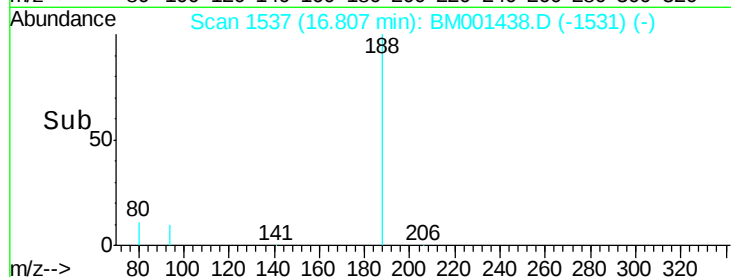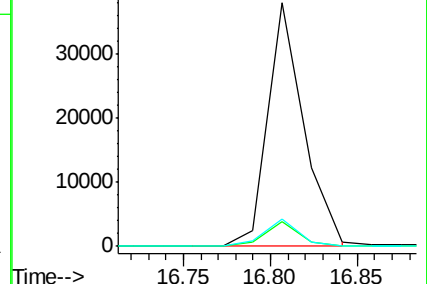

#17

Chrysene-d12

Concen: 5.00 ng

RT: 21.02 min Scan# 2046

Delta R.T. -0.01 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42


Tgt Ion:240 Resp: 50627

Ion Ratio Lower Upper

240 100

120 6.0 3.2 4.8#



236 26.5 19.8 29.6

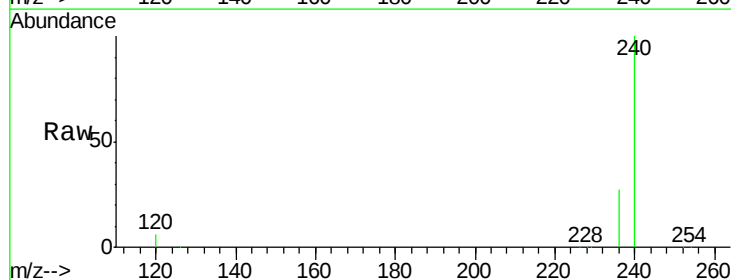


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

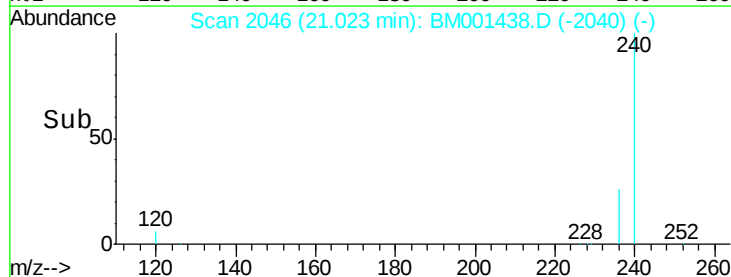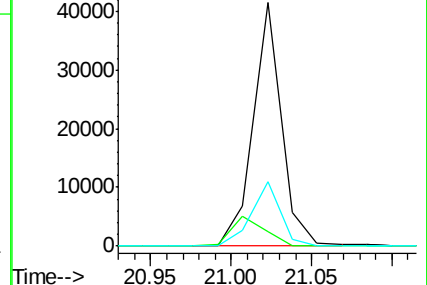

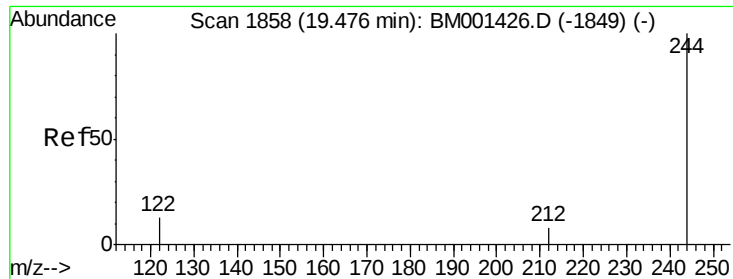

#18

Terphenyl-d14

Concen: 6.16 ng

RT: 19.47 min Scan# 1857

Delta R.T. -0.01 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42

Instrument :

BNA_M

ClientSampleId :

KM-SP-002-150518


Tgt Ion:244 Resp: 38774

Ion Ratio Lower Upper

244 100

212 9.3 7.4 11.2




122 15.9 11.4 17.0

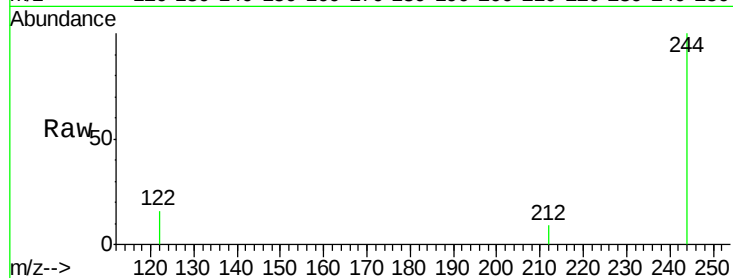

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

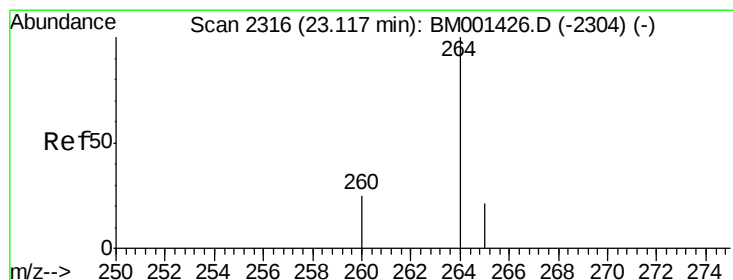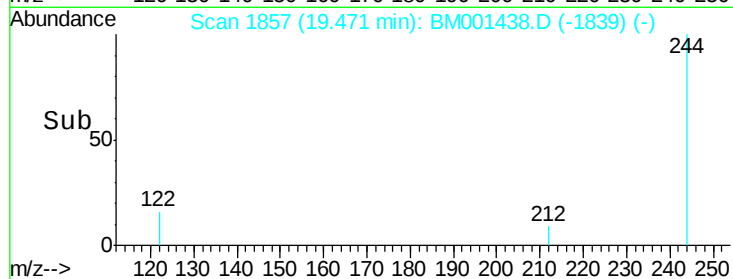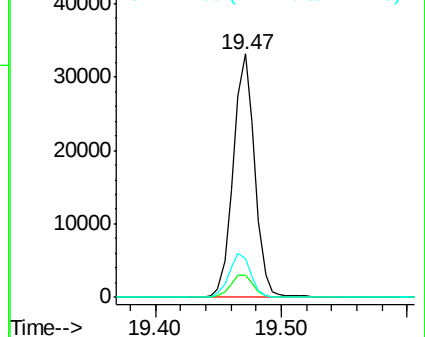

#21

Perylene-d12

Concen: 5.00 ng

RT: 23.11 min Scan# 2313

Delta R.T. -0.01 min

Lab File: BM001438.D

Acq: 28 May 2015 22:42


Tgt Ion:264 Resp: 43471

Ion Ratio Lower Upper

264 100

260 25.0 20.1 30.1

265 21.6 17.3 25.9

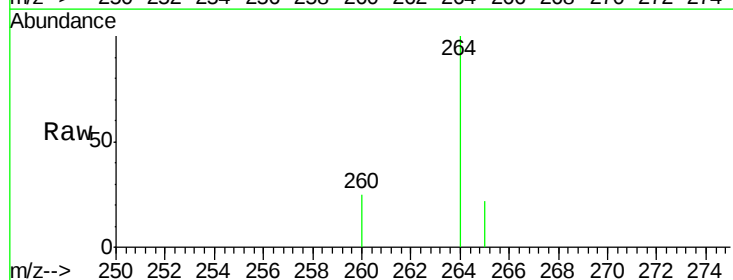

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

