


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052815\
 Data File : BM001422.D
 Acq On : 28 May 2015 09:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM052815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 15:41:25 2015

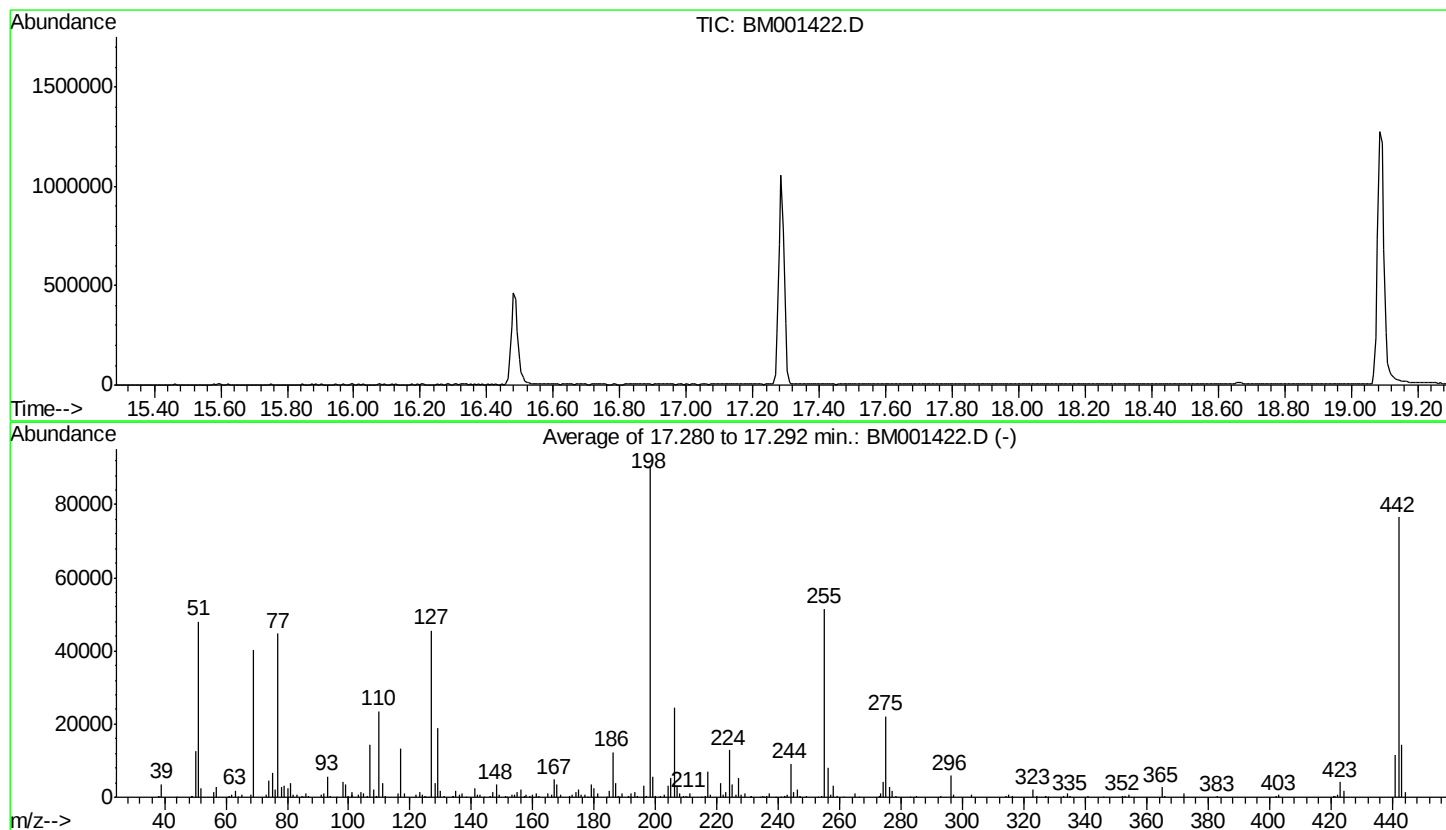

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	48016	PASS
68	69	0.00	2	1.9	767	PASS
69	198	0.00	100	44.5	40312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	45597	PASS
197	198	0.00	2	0.5	496	PASS
198	198	100	100	100.0	90677	PASS
199	198	5	9	6.3	5744	PASS
275	198	10	60	24.5	22208	PASS
365	198	1	100	2.9	2653	PASS
441	442	0.01	24	15.0	11451	PASS
442	198	50	100	84.4	76514	PASS
443	442	15	24	18.7	14341	PASS