


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052815\
 Data File : BM001435.D
 Acq On : 28 May 2015 20:17
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 18:41:08 2015

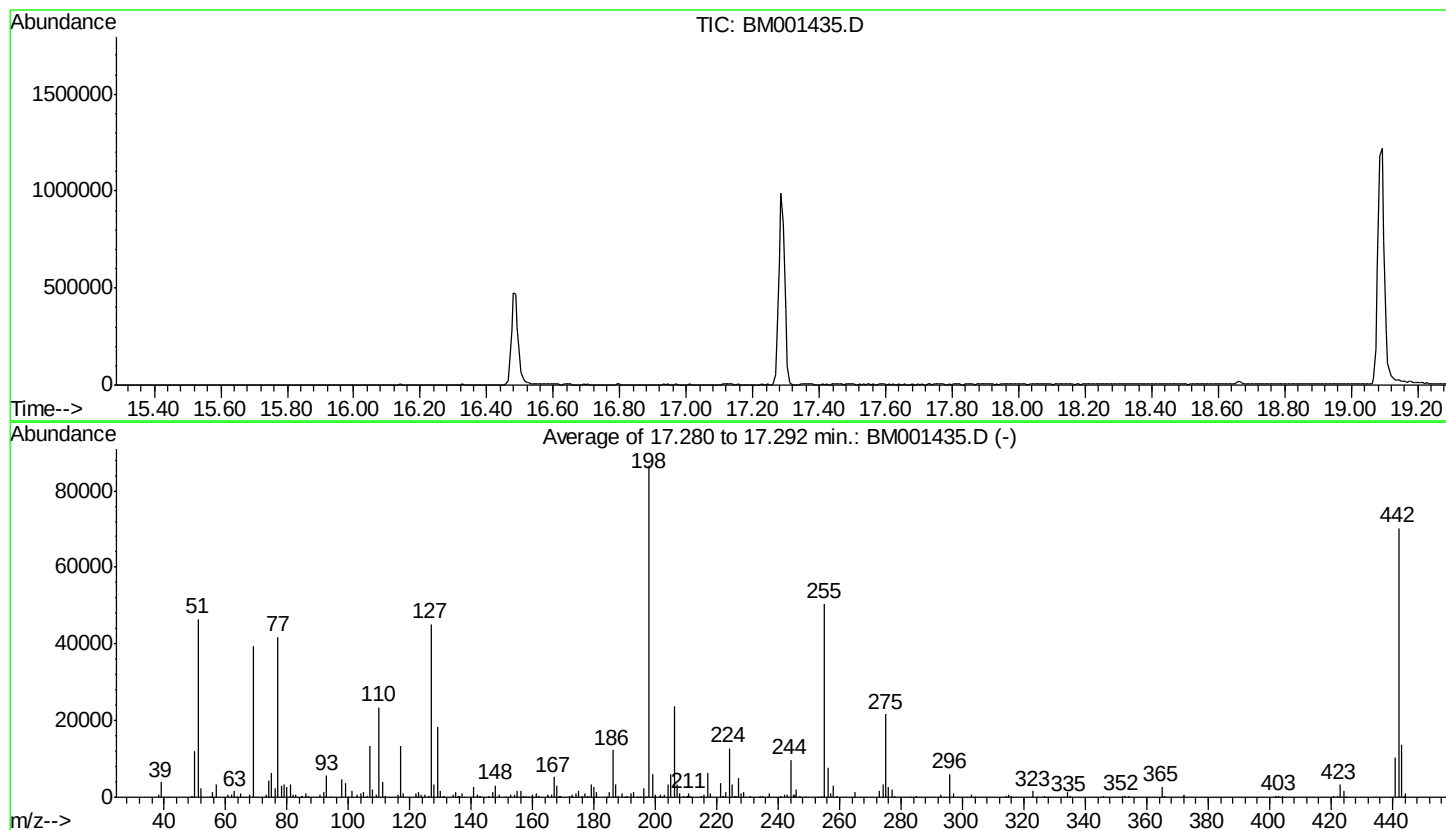

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.7	46482	PASS
68	69	0.00	2	1.6	643	PASS
69	198	0.00	100	45.7	39581	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	45186	PASS
197	198	0.00	2	0.1	126	PASS
198	198	100	100	100.0	86546	PASS
199	198	5	9	7.1	6133	PASS
275	198	10	60	25.0	21602	PASS
365	198	1	100	3.3	2833	PASS
441	442	0.01	24	15.0	10529	PASS
442	198	50	100	81.2	70261	PASS
443	442	15	24	19.3	13555	PASS