

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
 Data File : BM026157.D
 Acq On : 28 May 2020 13:40
 Operator : MA/SJ
 Sample : L2781-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	27	30	37	rVB	17798	21125	0.85%	0.100%
2	3.463	96	98	101	rVB4	2737	2846	0.11%	0.013%
3	3.599	118	121	125	rVB6	4321	5308	0.21%	0.025%
4	3.681	130	135	140	rBV	20421	30871	1.24%	0.146%
5	3.763	145	149	154	rVB3	9638	14627	0.59%	0.069%
6	3.987	183	187	191	rVB4	7437	9119	0.37%	0.043%
7	4.298	238	240	246	rVB5	2367	3053	0.12%	0.014%
8	4.387	252	255	261	rVB7	4465	7558	0.30%	0.036%
9	4.657	297	301	308	rBV	28644	43475	1.74%	0.206%
10	5.263	400	404	405	rBV4	2787	3133	0.13%	0.015%
11	5.545	445	452	455	rBV5	2600	5167	0.21%	0.024%
12	5.651	466	470	473	rBV4	2266	3007	0.12%	0.014%
13	6.245	568	571	575	rVB5	2060	2537	0.10%	0.012%
14	6.675	634	644	656	rBV	241509	411791	16.52%	1.949%
15	6.834	666	671	682	rBV	184426	294972	11.83%	1.396%
16	7.022	696	703	712	rBV	242562	387056	15.52%	1.832%
17	7.087	712	714	718	rVV4	3225	3949	0.16%	0.019%
18	7.134	718	722	727	rVB6	5095	8519	0.34%	0.040%
19	7.481	774	781	790	rBV	593663	899179	36.07%	4.256%
20	7.575	791	797	801	rVB5	6111	9950	0.40%	0.047%
21	8.198	897	903	914	rBV	267810	419852	16.84%	1.987%
22	8.304	917	921	929	rVB	12639	21407	0.86%	0.101%
23	8.622	969	975	984	rBV	214457	367594	14.74%	1.740%
24	8.722	988	992	996	rVV2	14517	20341	0.82%	0.096%
25	8.816	1004	1008	1010	rBV5	1844	3042	0.12%	0.014%
26	9.098	1050	1056	1061	rBV	11557	17689	0.71%	0.084%
27	9.339	1091	1097	1106	rBV	160110	262167	10.52%	1.241%
28	9.880	1183	1189	1201	rBV	231687	412975	16.56%	1.955%
29	9.969	1203	1204	1212	rVB7	2835	4224	0.17%	0.020%
30	10.239	1243	1250	1260	rBV	755064	1240290	49.75%	5.871%
31	10.392	1268	1276	1291	rBV	199052	383155	15.37%	1.814%
32	10.592	1308	1310	1313	rVB4	2553	2550	0.10%	0.012%
33	10.822	1346	1349	1353	rBV6	1554	2818	0.11%	0.013%
34	10.916	1363	1365	1370	rVB4	2221	3097	0.12%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
 Data File : BM026157.D
 Acq On : 28 May 2020 13:40
 Operator : MA/SJ
 Sample : L2781-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	11.463	1455	1458	1460	rBV3	2740	2963	0.12%	0.014%
36	11.722	1498	1502	1504	rVB4	2925	3339	0.13%	0.016%
37	11.774	1509	1511	1514	rVV3	4029	4938	0.20%	0.023%
38	11.845	1517	1523	1529	rVB9	5095	11741	0.47%	0.056%
39	12.033	1552	1555	1558	rVB4	2322	2922	0.12%	0.014%
40	12.069	1558	1561	1562	rBV3	2776	3140	0.13%	0.015%
41	12.180	1578	1580	1581	rBV2	3188	2813	0.11%	0.013%
42	12.204	1581	1584	1588	rVB5	4463	6260	0.25%	0.030%
43	12.269	1590	1595	1601	rVB9	4607	8918	0.36%	0.042%
44	12.321	1601	1604	1606	rBV3	2411	3208	0.13%	0.015%
45	12.610	1650	1653	1656	rBV5	4752	5431	0.22%	0.026%
46	12.674	1661	1664	1669	rVB7	5986	9529	0.38%	0.045%
47	12.745	1672	1676	1677	rBV4	4610	4222	0.17%	0.020%
48	12.816	1685	1688	1692	rBV6	2147	3221	0.13%	0.015%
49	12.851	1692	1694	1695	rBV2	3193	3081	0.12%	0.015%
50	12.904	1700	1703	1709	rVB7	12081	20376	0.82%	0.096%
51	12.951	1709	1711	1712	rBV2	3540	3413	0.14%	0.016%
52	12.974	1712	1715	1718	rBV5	5794	6926	0.28%	0.033%
53	13.045	1724	1727	1737	rBV5	9040	21335	0.86%	0.101%
54	13.133	1740	1742	1744	rBV3	4082	3496	0.14%	0.017%
55	13.174	1747	1749	1754	rVB6	5950	7782	0.31%	0.037%
56	13.233	1757	1759	1761	rBV2	3017	2926	0.12%	0.014%
57	13.363	1779	1781	1784	rVB4	4065	3893	0.16%	0.018%
58	13.457	1793	1797	1799	rBV5	6782	9424	0.38%	0.045%
59	13.551	1806	1813	1817	rBV	445159	639292	25.64%	3.026%
60	13.598	1817	1821	1827	rVB	238431	331958	13.31%	1.571%
61	13.721	1840	1842	1848	rVB6	10034	11618	0.47%	0.055%
62	13.816	1848	1858	1864	rBV	443288	699921	28.07%	3.313%
63	13.927	1874	1877	1880	rBV4	15385	19050	0.76%	0.090%
64	14.127	1902	1911	1920	rVB	1027476	1527525	61.27%	7.231%
65	14.227	1923	1928	1932	rBV8	19322	33335	1.34%	0.158%
66	14.357	1944	1950	1963	rBV	121250	268541	10.77%	1.271%
67	14.762	2017	2019	2023	rBV5	15980	23852	0.96%	0.113%
68	15.021	2059	2063	2068	rBV7	29123	56496	2.27%	0.267%
69	15.127	2075	2081	2087	rBV	621540	888282	35.63%	4.205%
70	15.257	2099	2103	2113	rVB3	140537	213391	8.56%	1.010%
71	16.533	2316	2320	2328	rBV	477444	701667	28.14%	3.321%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
Data File : BM026157.D
Acq On : 28 May 2020 13:40
Operator : MA/SJ
Sample : L2781-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Title : SVOA CALIBRATION

72	16.874	2373	2378	2388	rVV	1321867	1780183	71.40%	8.427%
73	16.974	2390	2395	2407	rVB	671602	956309	38.36%	4.527%
74	18.315	2620	2623	2627	rBV5	38832	49930	2.00%	0.236%
75	19.274	2781	2786	2795	rBV	891259	1203748	48.28%	5.698%
76	20.821	3046	3049	3055	rBV	164807	218123	8.75%	1.033%
77	21.074	3087	3092	3097	rBV	1984385	2382367	95.55%	11.277%
78	23.056	3425	3429	3437	rVB	707972	1142980	45.84%	5.410%
79	23.191	3446	3452	3461	rVB	1354980	2493211	100.00%	11.802%


Sum of corrected areas: 21125519

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
Data File : BM026157.D
Acq On : 28 May 2020 13:40
Operator : MA/SJ
Sample : L2781-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

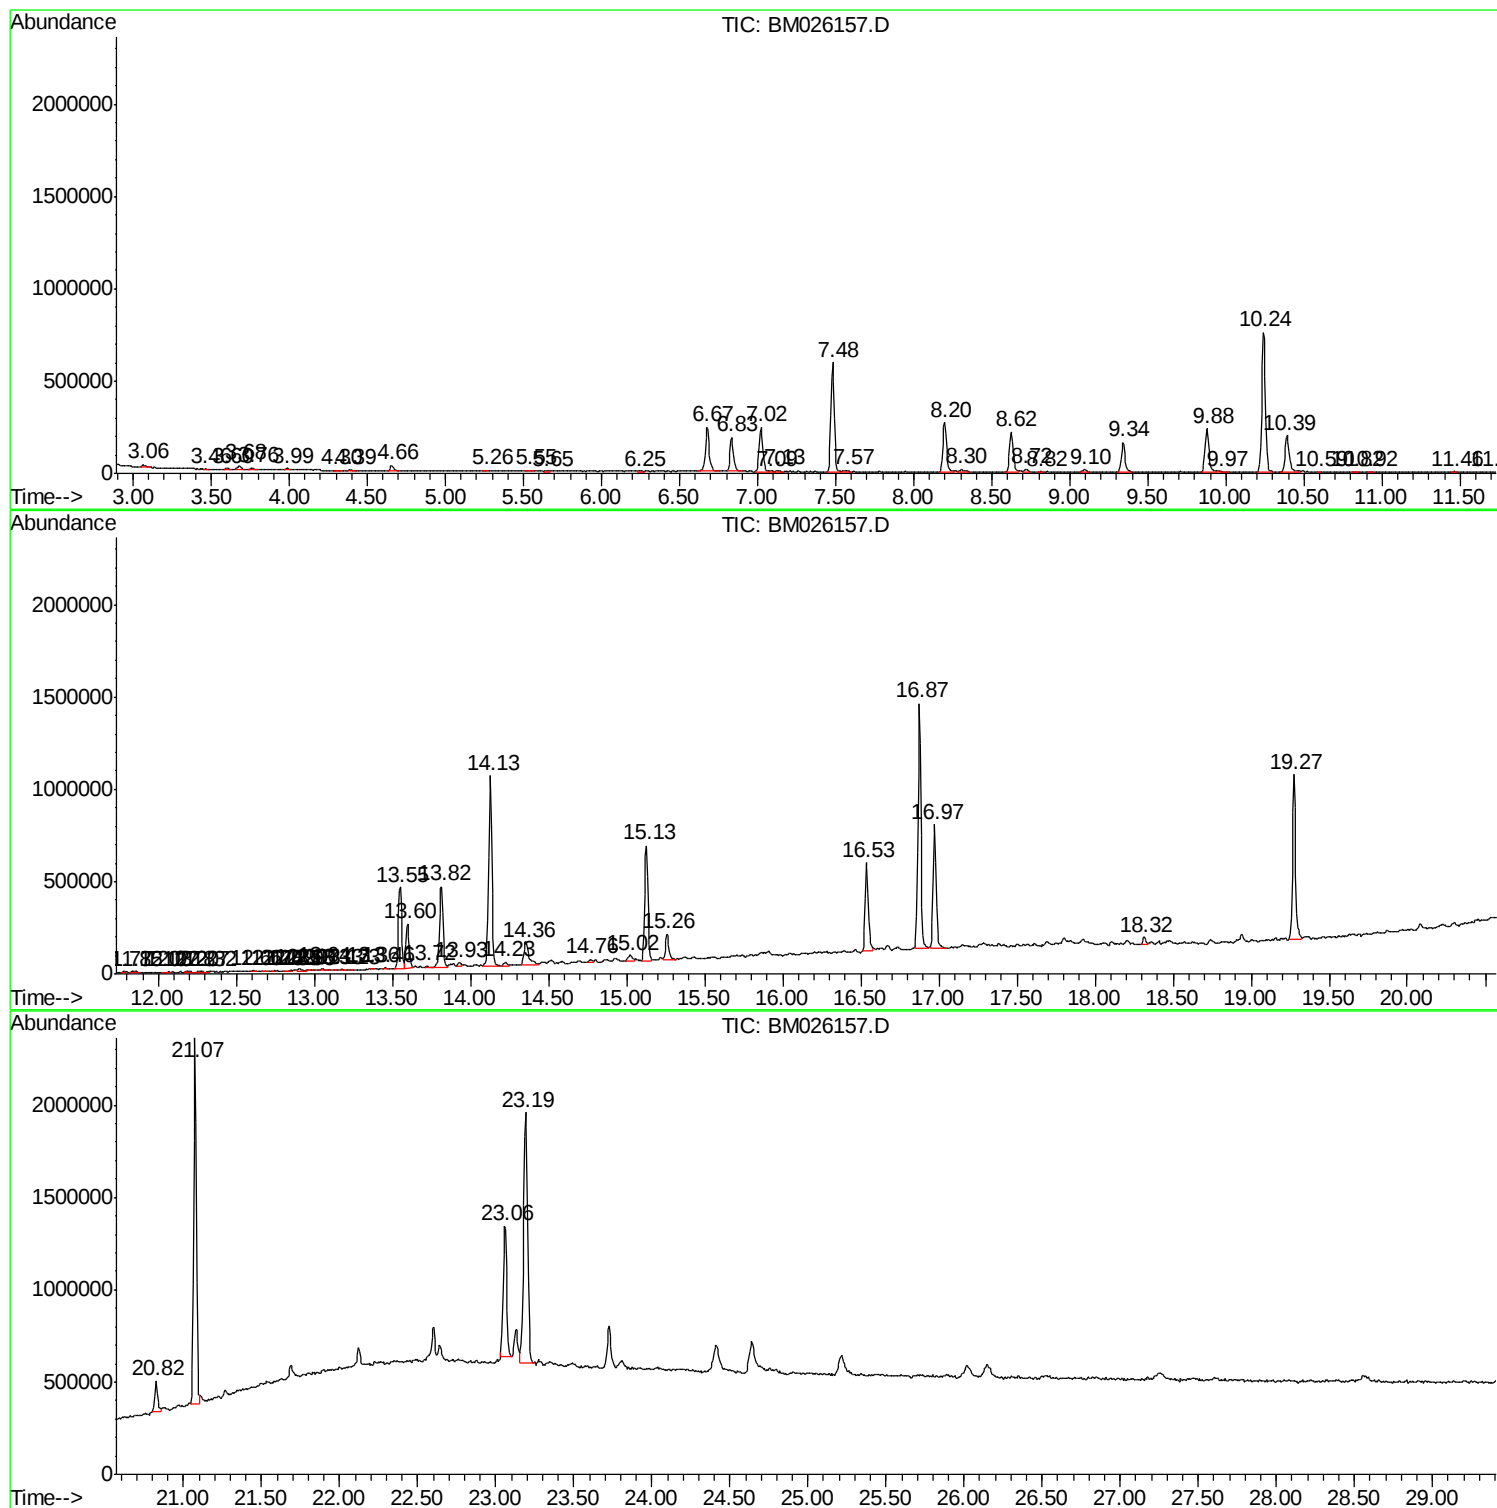

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052820\
Data File : BM026157.D
Acq On : 28 May 2020 13:40
Operator : MA/SJ
Sample : L2781-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052820\
Data File : BM026157.D
Acq On : 28 May 2020 13:40
Operator : MA/SJ
Sample : L2781-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc