

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
 Data File : BM026167.D
 Acq On : 28 May 2020 22:19
 Operator : MA/SJ
 Sample : L2781-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	27	30	39	rVB	21528	32837	1.00%	0.104%
2	3.557	110	114	119	rBV2	14748	22042	0.67%	0.070%
3	3.599	119	121	125	rVB5	6155	5510	0.17%	0.017%
4	3.675	130	134	141	rVV2	20043	35444	1.08%	0.112%
5	3.763	145	149	157	rVB3	10414	17132	0.52%	0.054%
6	3.981	183	186	191	rVB2	18443	26026	0.79%	0.082%
7	4.381	251	254	259	rVV3	11474	14647	0.45%	0.046%
8	4.651	296	300	307	rVV	38781	58048	1.77%	0.184%
9	5.540	447	451	456	rVB6	4561	7097	0.22%	0.022%
10	6.640	633	638	639	rVV	33352	44534	1.36%	0.141%
11	6.675	639	644	659	rVB	342569	566213	17.24%	1.794%
12	6.828	665	670	684	rVB	281257	439245	13.37%	1.392%
13	7.016	696	702	713	rVB	341224	539942	16.44%	1.711%
14	7.122	718	720	728	rVB9	6260	10820	0.33%	0.034%
15	7.481	774	781	790	rBV	668299	1049197	31.94%	3.325%
16	7.563	790	795	801	rVB3	7827	14851	0.45%	0.047%
17	8.192	896	902	911	rBV2	356025	562117	17.11%	1.781%
18	8.304	916	921	930	rVB	22280	40331	1.23%	0.128%
19	8.622	965	975	988	rBV	336774	562735	17.13%	1.783%
20	8.839	1010	1012	1018	rVB5	4079	7062	0.22%	0.022%
21	9.092	1050	1055	1059	rBV2	15603	24019	0.73%	0.076%
22	9.339	1090	1097	1111	rBV	261814	420788	12.81%	1.333%
23	9.875	1179	1188	1203	rBV	370614	616892	18.78%	1.955%
24	10.239	1243	1250	1262	rVB	941707	1509407	45.95%	4.783%
25	10.386	1268	1275	1290	rBV	300313	554543	16.88%	1.757%
26	11.786	1507	1513	1516	rBV5	5071	10110	0.31%	0.032%
27	11.839	1519	1522	1527	rVB4	6964	10928	0.33%	0.035%
28	12.057	1554	1559	1563	rVB6	2556	5195	0.16%	0.016%
29	12.480	1627	1631	1635	rBV5	3941	6514	0.20%	0.021%
30	12.733	1671	1674	1679	rVB6	5812	7775	0.24%	0.025%
31	12.974	1712	1715	1719	rVB4	6301	7418	0.23%	0.024%
32	13.051	1721	1728	1733	rBV7	8852	17523	0.53%	0.056%
33	13.545	1806	1812	1817	rBV	680977	945626	28.79%	2.997%
34	13.592	1817	1820	1827	rVB	332661	453180	13.80%	1.436%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
 Data File : BM026167.D
 Acq On : 28 May 2020 22:19
 Operator : MA/SJ
 Sample : L2781-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	13.810	1851	1857	1868	rBV	691135	981493	29.88%	3.110%
36	14.057	1896	1899	1903	rBV5	4614	6552	0.20%	0.021%
37	14.127	1903	1911	1918	rVV	1329977	1926705	58.66%	6.106%
38	14.180	1918	1920	1925	rVB4	6971	10693	0.33%	0.034%
39	14.351	1943	1949	1962	rBV2	206790	386013	11.75%	1.223%
40	14.527	1971	1979	1981	rBV8	4910	7973	0.24%	0.025%
41	14.580	1983	1988	1994	rVV3	41881	63780	1.94%	0.202%
42	14.686	2004	2006	2011	rVB4	3986	5071	0.15%	0.016%
43	14.963	2050	2053	2056	rBV4	4161	5565	0.17%	0.018%
44	15.021	2060	2063	2066	rVB3	6136	6038	0.18%	0.019%
45	15.127	2074	2081	2087	rBV	863805	1240569	37.77%	3.931%
46	15.180	2087	2090	2095	rVB2	15733	21423	0.65%	0.068%
47	15.257	2098	2103	2116	rBV	267130	384757	11.71%	1.219%
48	15.368	2116	2122	2125	rVB6	8786	13021	0.40%	0.041%
49	15.633	2164	2167	2169	rVV4	4625	6113	0.19%	0.019%
50	15.857	2198	2205	2207	rBV6	4837	7399	0.23%	0.023%
51	16.239	2266	2270	2275	rVB8	6549	8942	0.27%	0.028%
52	16.427	2298	2302	2303	rBV3	6186	6784	0.21%	0.021%
53	16.539	2317	2321	2327	rVB7	8751	14312	0.44%	0.045%
54	16.610	2330	2333	2336	rBV5	4093	5637	0.17%	0.018%
55	16.662	2338	2342	2344	rVV3	7746	10454	0.32%	0.033%
56	16.692	2344	2347	2351	rVB3	10644	14536	0.44%	0.046%
57	16.804	2361	2366	2369	rBV7	3602	4859	0.15%	0.015%
58	16.874	2369	2378	2382	rBV	1655497	2292571	69.80%	7.265%
59	16.915	2382	2385	2389	rVV	272197	351140	10.69%	1.113%
60	16.974	2389	2395	2408	rVV2	896486	1342935	40.89%	4.256%
61	17.068	2408	2411	2416	rVB7	9091	14257	0.43%	0.045%
62	17.280	2440	2447	2453	rBV	30710	55116	1.68%	0.175%
63	17.404	2464	2468	2474	rVB8	8757	13552	0.41%	0.043%
64	17.457	2474	2477	2480	rBV4	5085	6996	0.21%	0.022%
65	17.562	2492	2495	2497	rBV4	4003	6234	0.19%	0.020%
66	17.751	2523	2527	2531	rVV	29843	43184	1.31%	0.137%
67	17.798	2531	2535	2542	rVV	52048	75094	2.29%	0.238%
68	17.874	2544	2548	2553	rVV4	12453	24346	0.74%	0.077%
69	17.939	2554	2559	2563	rVV2	58622	92737	2.82%	0.294%
70	17.980	2563	2566	2571	rVV	21731	29688	0.90%	0.094%
71	18.056	2575	2579	2581	rBV5	4414	7011	0.21%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
 Data File : BM026167.D
 Acq On : 28 May 2020 22:19
 Operator : MA/SJ
 Sample : L2781-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	18.104	2583	2587	2590	rVB6	8323	12117	0.37%	0.038%
73	18.256	2610	2613	2616	rBV	33077	41989	1.28%	0.133%
74	18.292	2616	2619	2627	rVB3	37163	53443	1.63%	0.169%
75	18.356	2628	2630	2633	rVV3	4747	4844	0.15%	0.015%
76	18.504	2652	2655	2660	rBV5	9599	13738	0.42%	0.044%
77	18.562	2662	2665	2668	rVV3	8069	10144	0.31%	0.032%
78	18.598	2668	2671	2674	rVV5	11544	13329	0.41%	0.042%
79	18.680	2681	2685	2689	rBV3	27557	43777	1.33%	0.139%
80	18.739	2692	2695	2698	rVB4	10796	16853	0.51%	0.053%
81	18.815	2705	2708	2717	rBV5	24903	50637	1.54%	0.160%
82	18.939	2721	2729	2737	rBV	898421	1177487	35.85%	3.731%
83	19.274	2780	2786	2789	rBV	1213162	1735111	52.83%	5.498%
84	19.303	2789	2791	2800	rVV	687847	744025	22.65%	2.358%
85	19.380	2800	2804	2810	rVB4	26661	43920	1.34%	0.139%
86	19.486	2819	2822	2828	rVB	31231	37771	1.15%	0.120%
87	19.768	2867	2870	2873	rBV5	29973	51290	1.56%	0.163%
88	19.809	2873	2877	2881	rVB	99075	131139	3.99%	0.416%
89	19.909	2890	2894	2897	rBV2	84512	93322	2.84%	0.296%
90	19.962	2900	2903	2906	rVB5	50711	65765	2.00%	0.208%
91	20.762	3036	3039	3041	rBV	55817	58052	1.77%	0.184%
92	20.797	3042	3045	3046	rBV	55351	62865	1.91%	0.199%
93	20.821	3046	3049	3053	rVV3	156881	198105	6.03%	0.628%
94	21.074	3085	3092	3096	rBV2	2168809	3284608	100.00%	10.409%
95	21.109	3096	3098	3105	rVB	488539	503782	15.34%	1.596%
96	22.568	3341	3346	3349	rBV	477692	900398	27.41%	2.853%
97	23.009	3417	3421	3424	rBV	232245	359328	10.94%	1.139%
98	23.056	3424	3429	3433	rVV	651293	1007216	30.66%	3.192%
99	23.097	3433	3436	3439	rVV	181459	242960	7.40%	0.770%
100	23.191	3446	3452	3457	rBV	1439344	2459188	74.87%	7.793%


Sum of corrected areas: 31556501

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052820\
Data File : BM026167.D
Acq On : 28 May 2020 22:19
Operator : MA/SJ
Sample : L2781-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

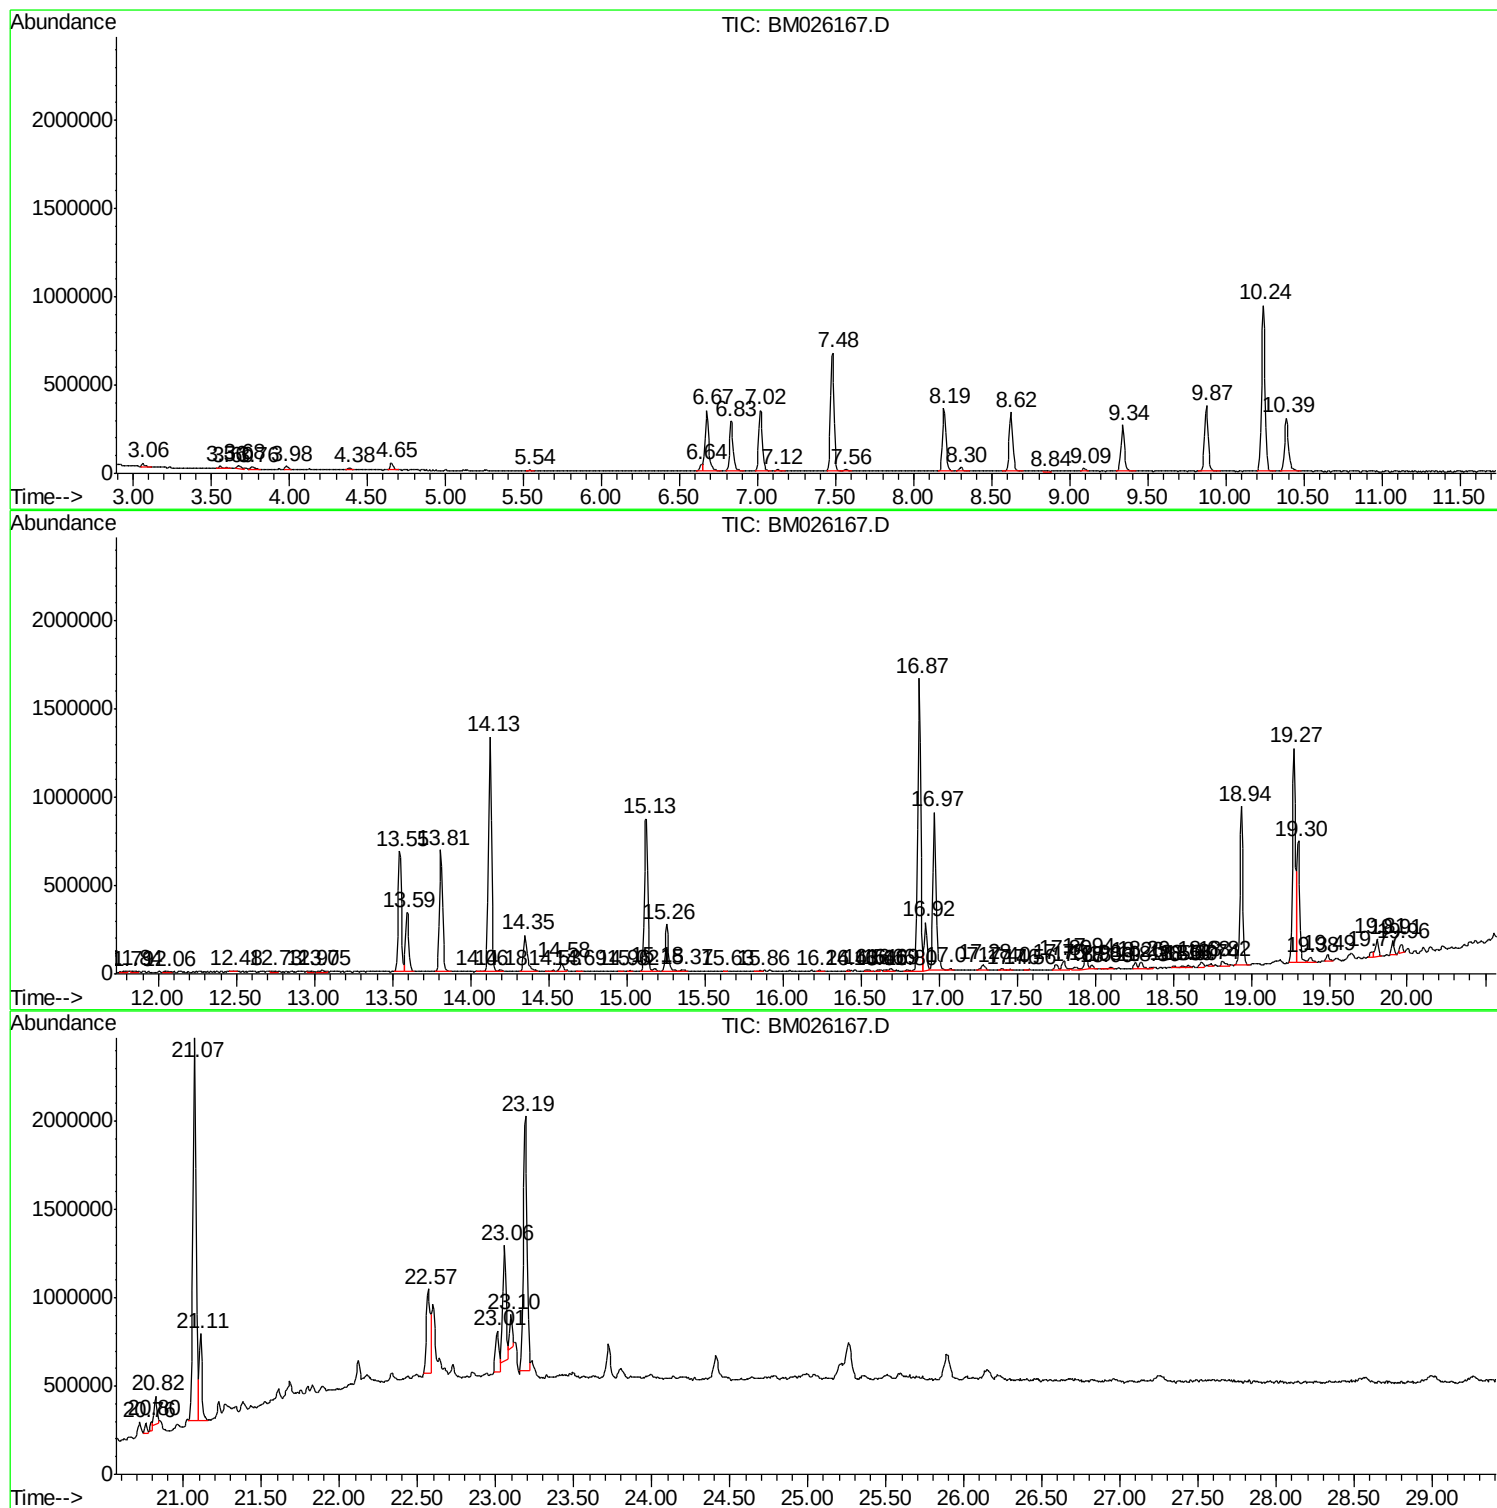

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052820\
Data File : BM026167.D
Acq On : 28 May 2020 22:19
Operator : MA/SJ
Sample : L2781-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052820\
Data File : BM026167.D
Acq On : 28 May 2020 22:19
Operator : MA/SJ
Sample : L2781-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc