

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035309.D
 Acq On : 28 May 2022 14:47
 Operator : CG/JU
 Sample : N2931-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P009-SS003-0006-01

Quant Time: May 29 00:33:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 16:44:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	103256	20.000	ng	0.00
21) Naphthalene-d8	10.675	136	370490	20.000	ng	0.00
39) Acenaphthene-d10	14.510	164	217177	20.000	ng	0.00
64) Phenanthrene-d10	17.251	188	483947	20.000	ng	# 0.00
76) Chrysene-d12	21.433	240	635887	20.000	ng	# 0.00
86) Perylene-d12	23.803	264	708802	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	537464	96.107	ng	0.00
7) Phenol-d6	7.045	99	669897	92.510	ng	0.00
23) Nitrobenzene-d5	9.033	82	424945	63.139	ng	0.00
42) 2,4,6-Tribromophenol	15.998	330	268236	95.206	ng	0.00
45) 2-Fluorobiphenyl	13.133	172	1011773	64.605	ng	0.00
79) Terphenyl-d14	19.880	244	1875623	52.267	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	20.574	149	63637	3.988	ng	Qvalue 91
84) Bis(2-ethylhexyl)phtha...	21.350	149	57311	2.540	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035309.D
Acq On : 28 May 2022 14:47
Operator : CG/JU
Sample : N2931-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01

Quant Time: May 29 00:33:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 16:44:39 2022
Response via : Initial Calibration




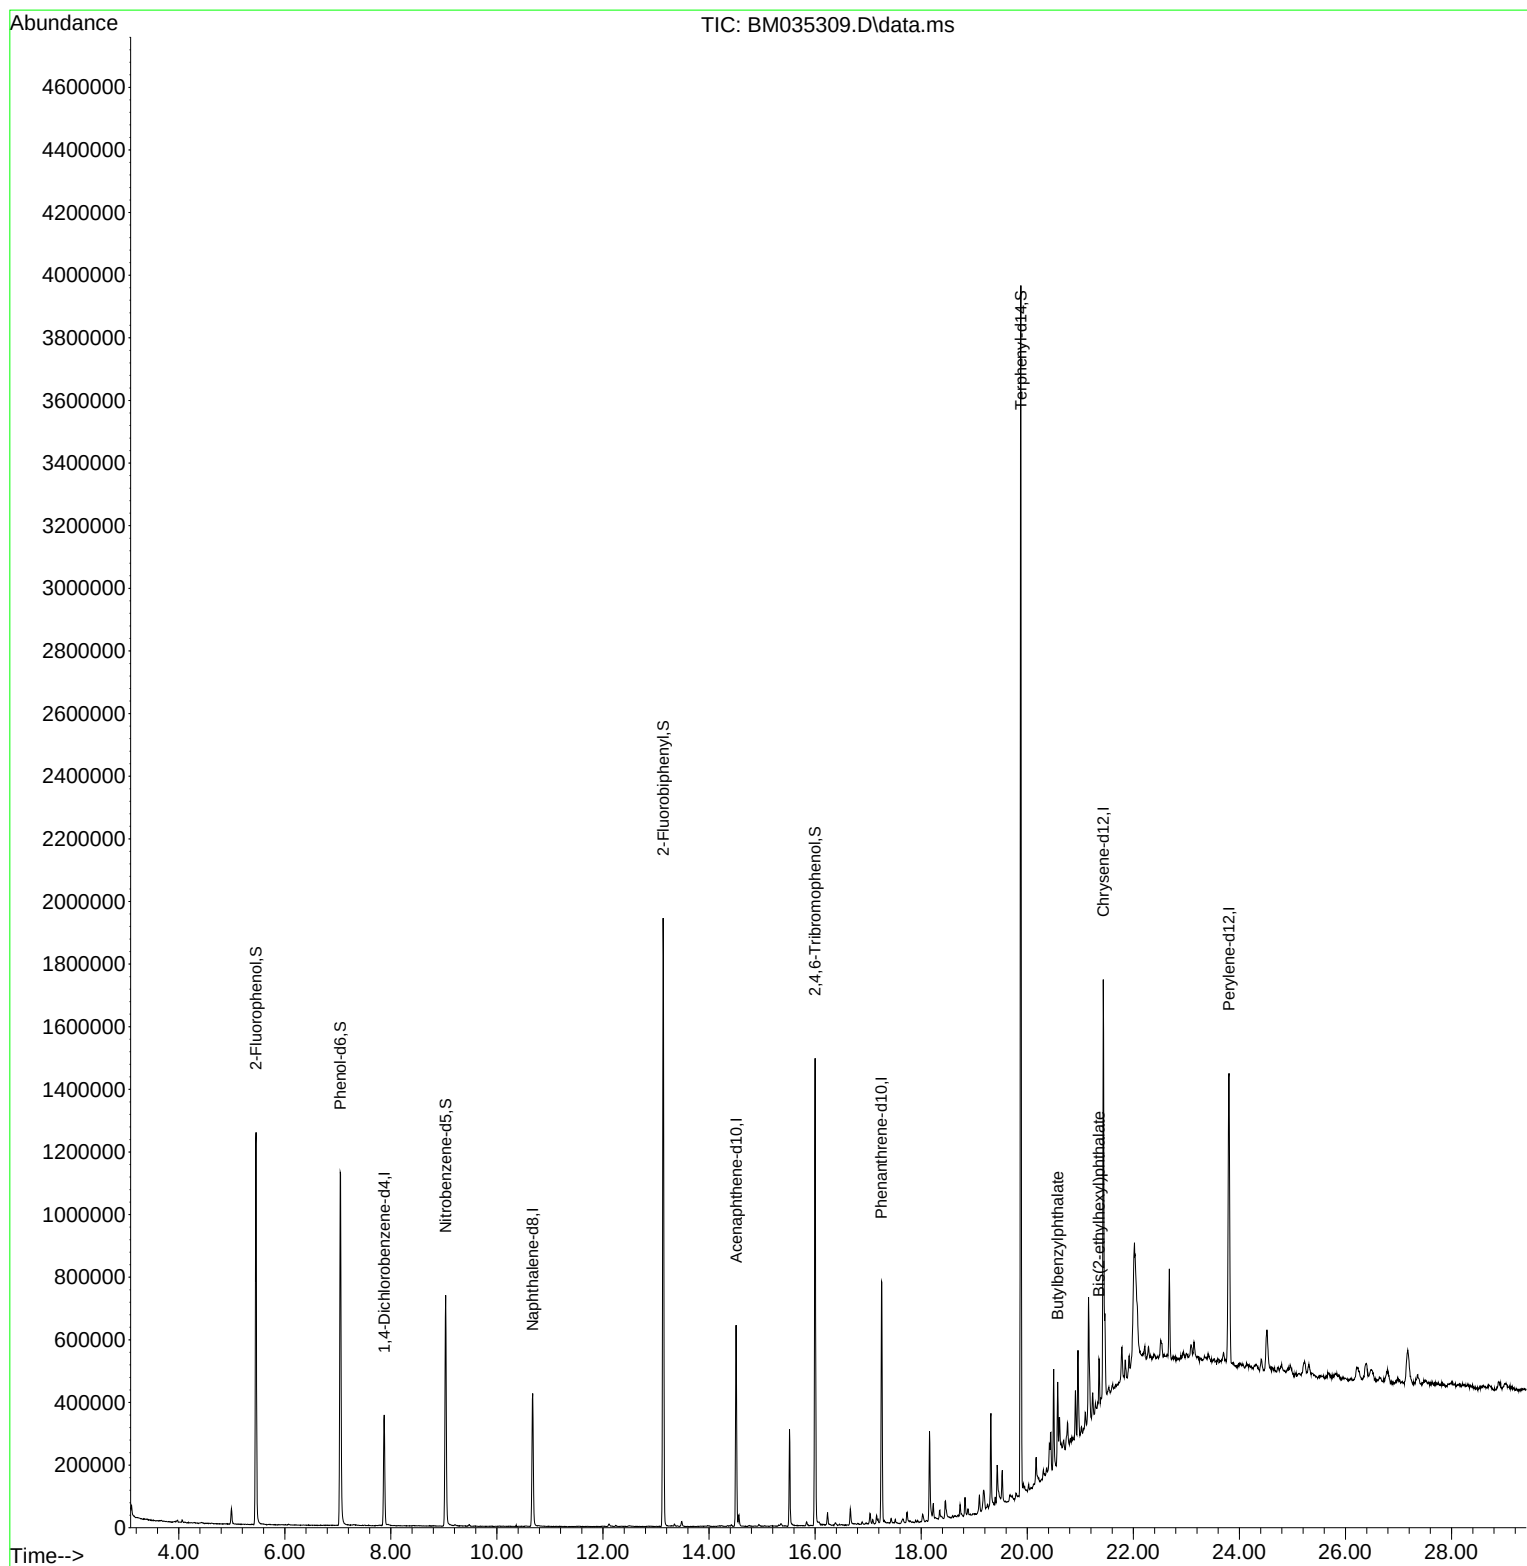


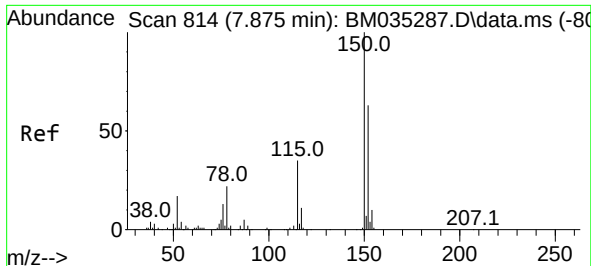

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.875 min Scan# 814
Delta R.T. -0.000 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47




Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01


Tgt Ion:152 Resp: 103256
Ion Ratio Lower Upper
152 100
150 154.5 124.9 187.3
115 55.5 47.9 71.9

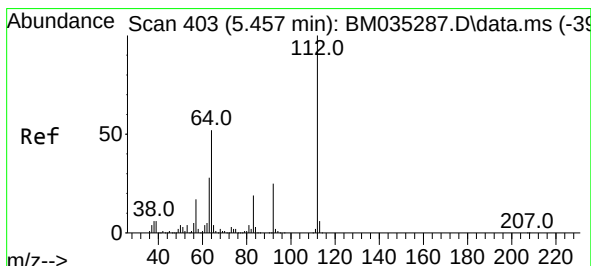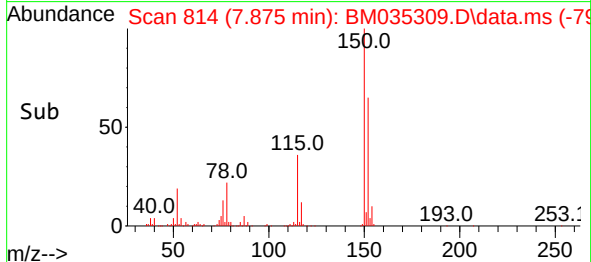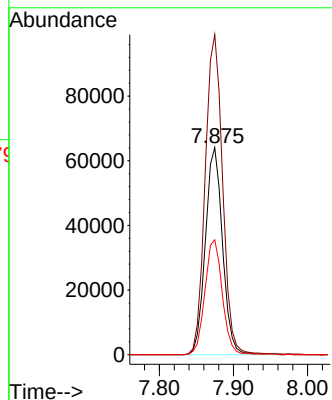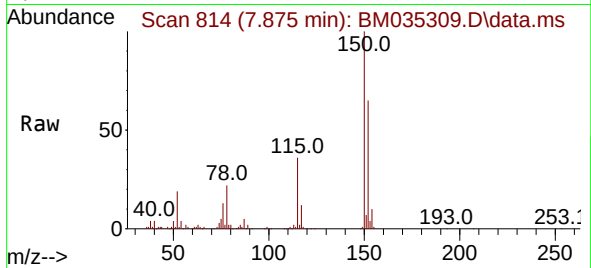

#5
2-Fluorophenol
Concen: 96.107 ng
RT: 5.457 min Scan# 403
Delta R.T. 0.000 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47

Tgt Ion:112 Resp: 537464
Ion Ratio Lower Upper
112 100
64 55.5 47.8 71.6
63 30.5 26.6 40.0


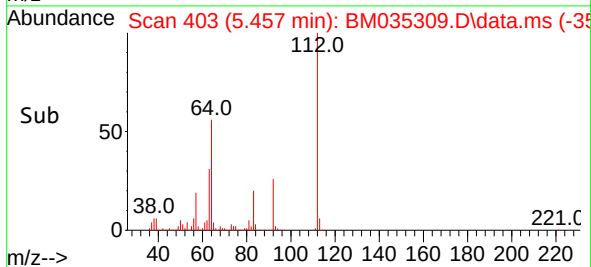
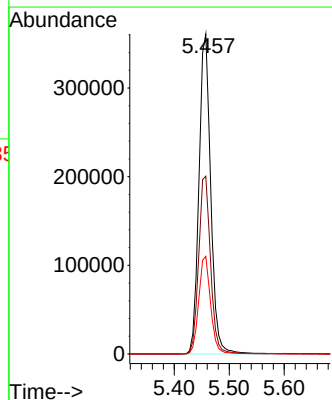
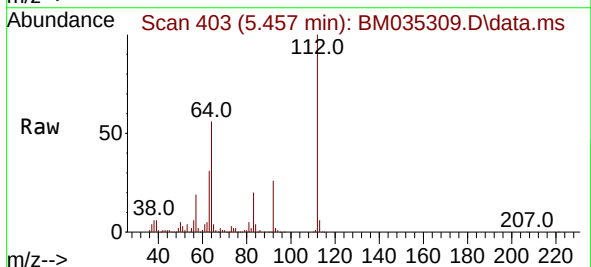


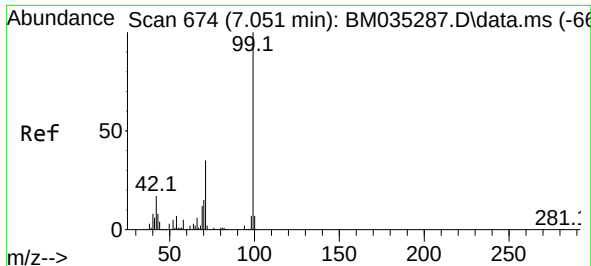

#7
Phenol-d6
Concen: 92.510 ng
RT: 7.045 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47




Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01


Tgt Ion: 99 Resp: 669897
Ion Ratio Lower Upper
99 100
42 19.7 18.8 28.2
71 35.4 30.2 45.2

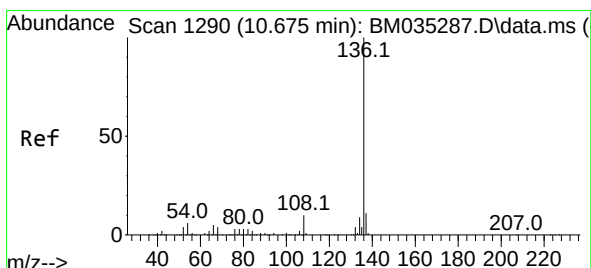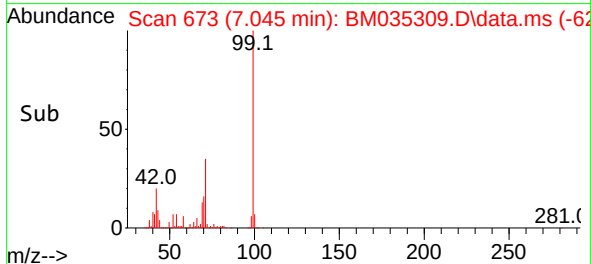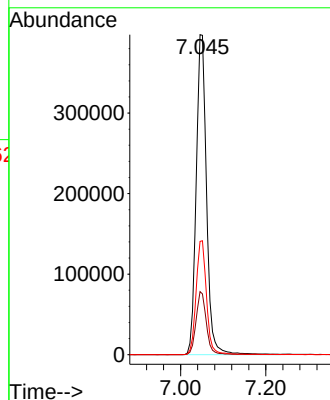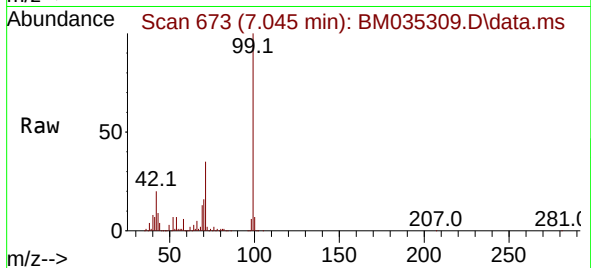

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.675 min Scan# 1290
Delta R.T. -0.000 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47

Tgt Ion: 136 Resp: 370490
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 7.0 7.0 10.4
68 4.9 4.3 6.5


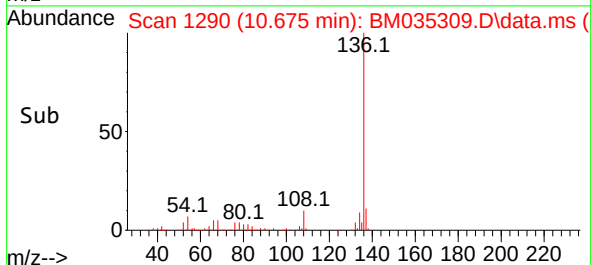
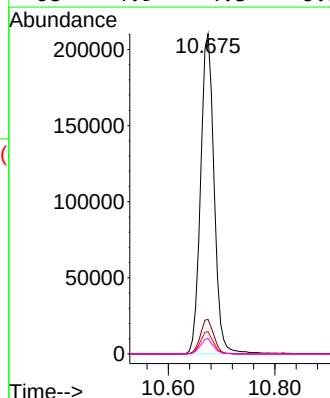
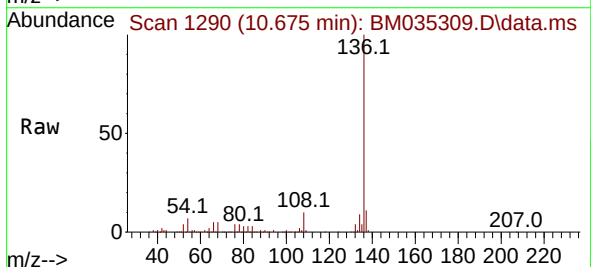


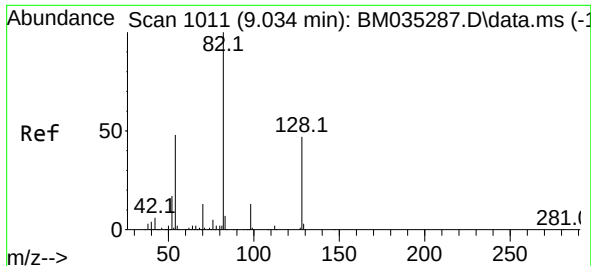

#23
Nitrobenzene-d5
Concen: 63.139 ng
RT: 9.033 min Scan# 1011
Delta R.T. -0.001 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47




Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01


Tgt Ion: 82 Resp: 424945
Ion Ratio Lower Upper
82 100
128 46.6 33.7 50.5
54 50.0 43.2 64.8

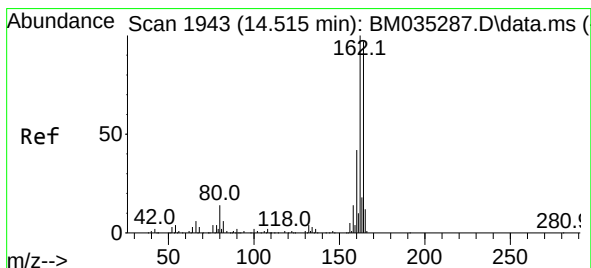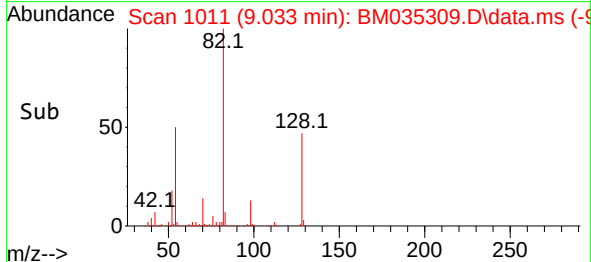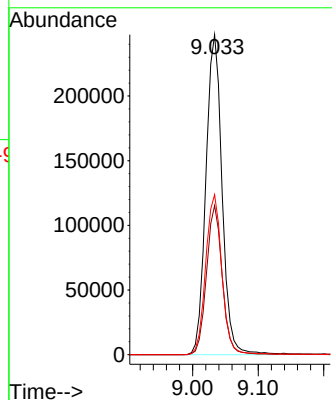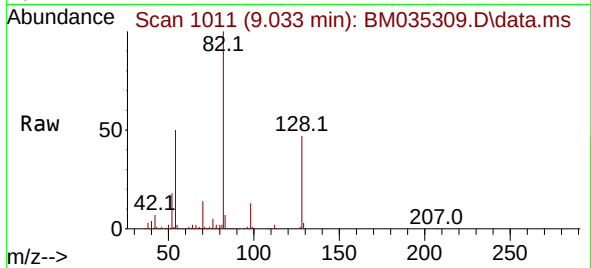

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.510 min Scan# 1942
Delta R.T. -0.005 min
Lab File: BM035309.D
Acq: 28 May 2022 14:47

Tgt Ion: 164 Resp: 217177
Ion Ratio Lower Upper
164 100
162 104.8 83.0 124.6
160 46.1 37.0 55.4

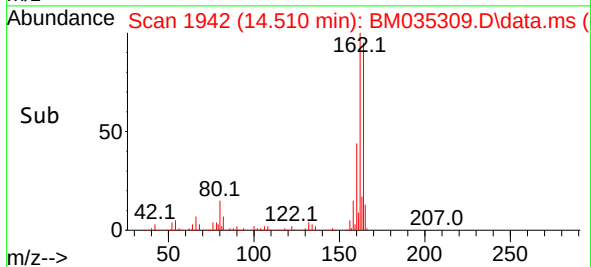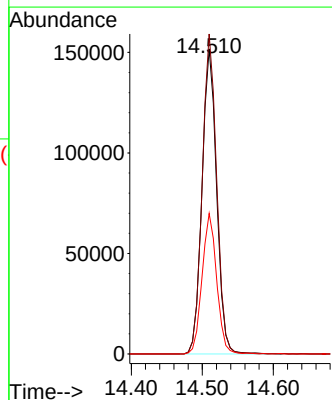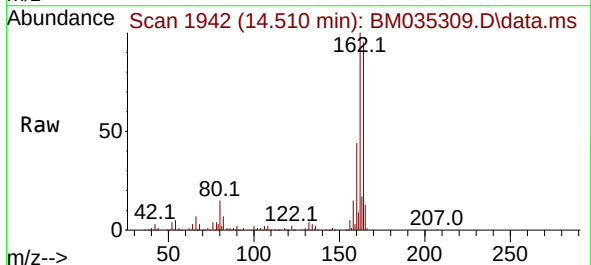

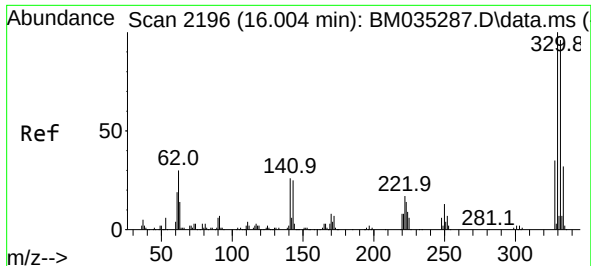

#42

2,4,6-Tribromophenol

Concen: 95.206 ng

RT: 15.998 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM035309.D


Acq: 28 May 2022 14:47

Instrument :

BNA_M

ClientSampleId :

P009-SS003-0006-01

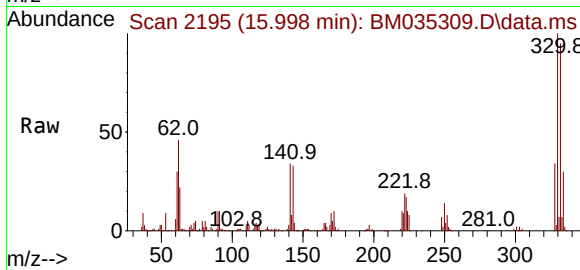




Tgt Ion:330 Resp: 268236

Ion Ratio Lower Upper

330 100

332 97.1 77.0 115.4

141 34.5 35.3 52.9#

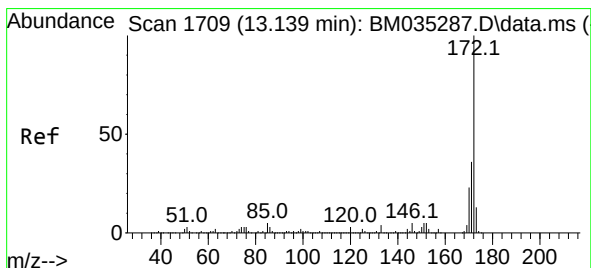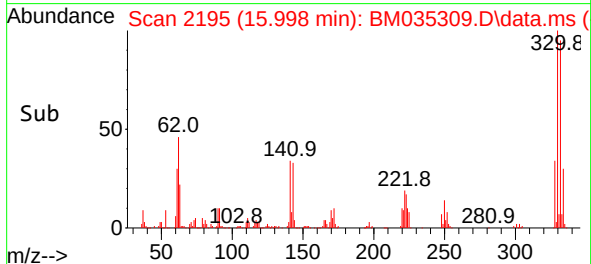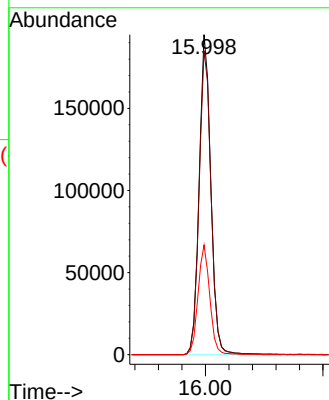

#45

2-Fluorobiphenyl

Concen: 64.605 ng

RT: 13.133 min Scan# 1708

Delta R.T. -0.006 min

Lab File: BM035309.D

Acq: 28 May 2022 14:47




Tgt Ion:172 Resp: 1011773


Ion Ratio Lower Upper

172 100

171 35.8 28.5 42.7

170 23.2 18.7 28.1

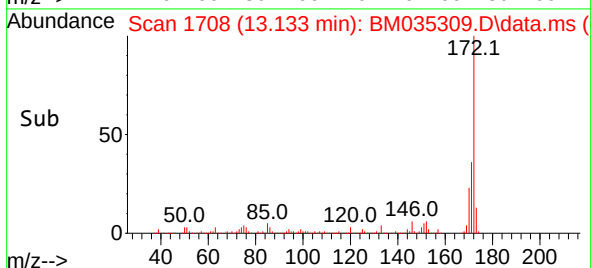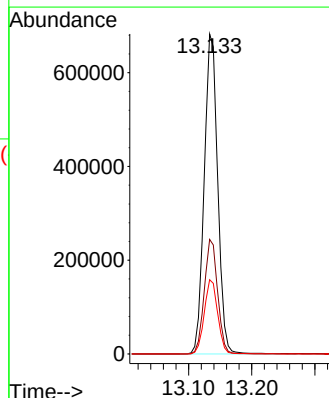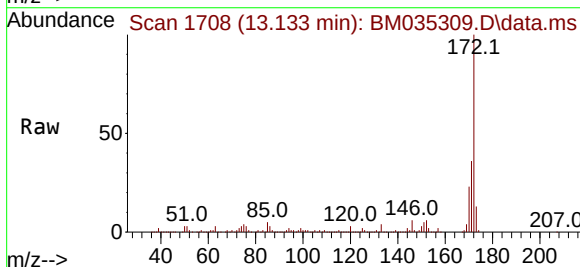

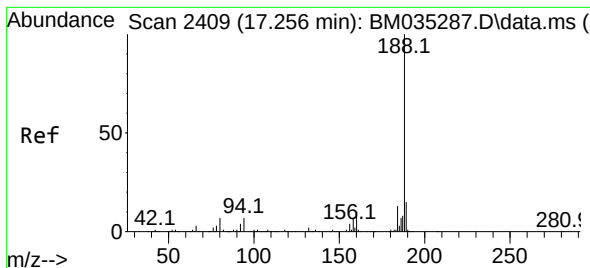

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.251 min Scan# 2408

Delta R.T. -0.006 min

Lab File: BM035309.D

Acq: 28 May 2022 14:47

Instrument :

BNA_M

ClientSampleId :

P009-SS003-0006-01





Tgt Ion:188 Resp: 483947

Ion Ratio Lower Upper

188 100

94 6.8 7.0 10.4#

80 7.9 7.6 11.4

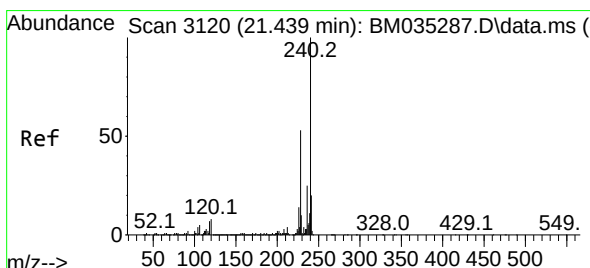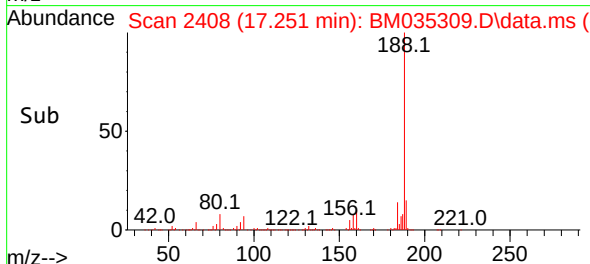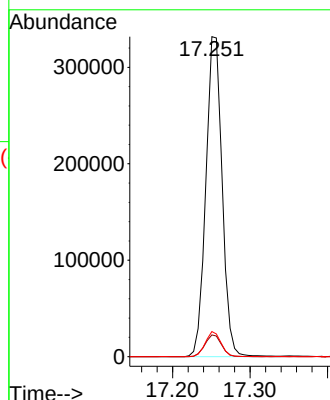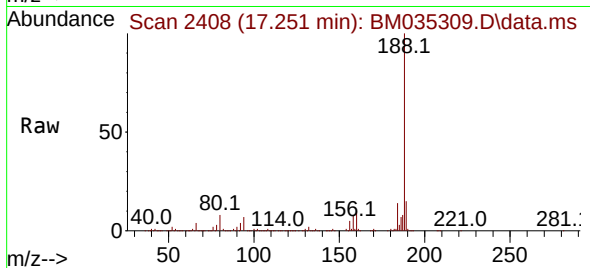

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.433 min Scan# 3119

Delta R.T. -0.006 min

Lab File: BM035309.D

Acq: 28 May 2022 14:47




Tgt Ion:240 Resp: 635887


Ion Ratio Lower Upper

240 100

120 8.6 9.4 14.0#

236 25.9 20.6 30.8


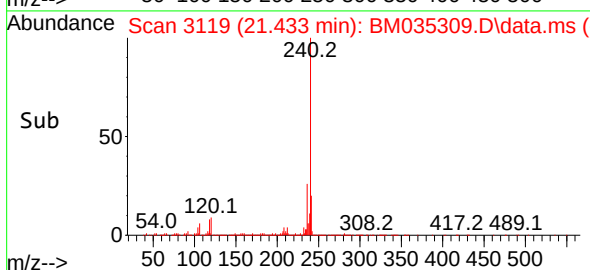
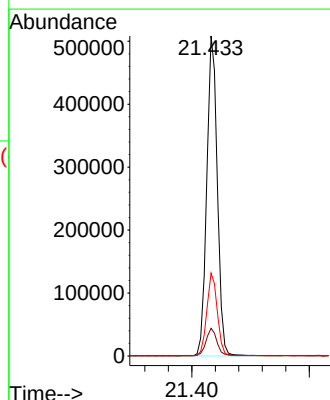
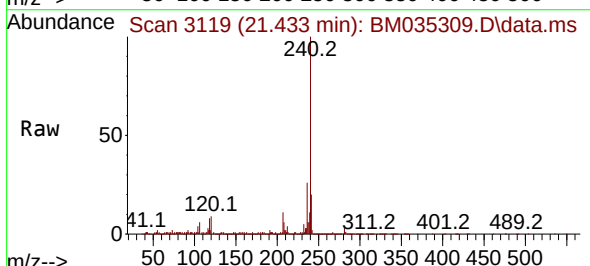


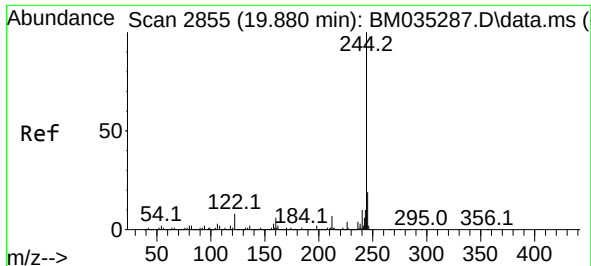

#79
 Terphenyl-d14
 Concen: 52.267 ng
 RT: 19.880 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM035309.D
 Acq: 28 May 2022 14:47




Instrument :
 BNA_M
 ClientSampleId :
 P009-SS003-0006-01


Tgt Ion:244 Resp: 1875623
 Ion Ratio Lower Upper
 244 100
 212 6.9 6.2 9.4
 122 7.9 8.3 12.5#

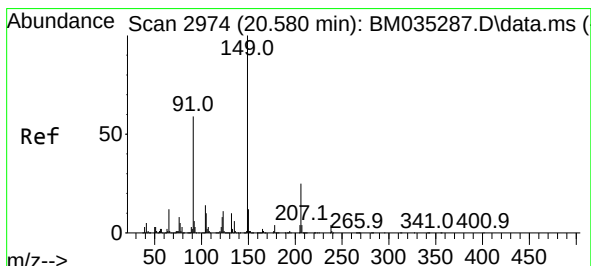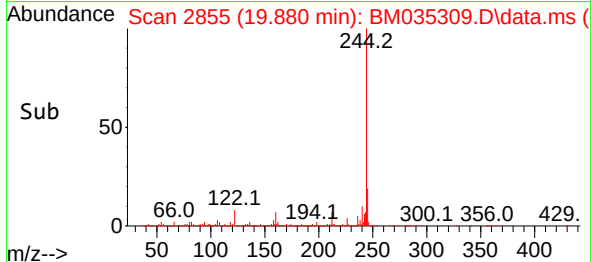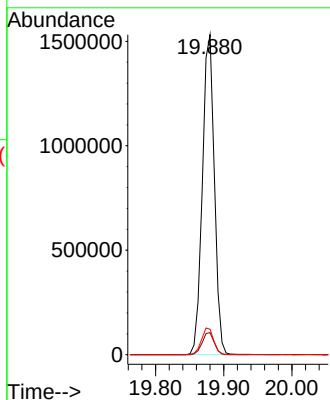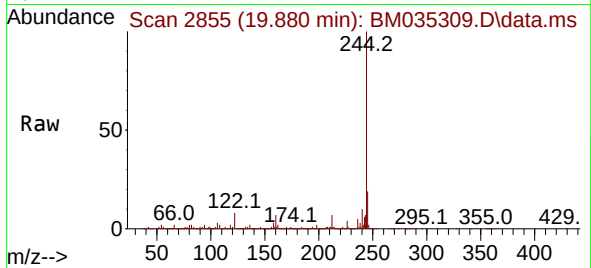

#80
 Butylbenzylphthalate
 Concen: 3.988 ng
 RT: 20.574 min Scan# 2973
 Delta R.T. -0.006 min
 Lab File: BM035309.D
 Acq: 28 May 2022 14:47

Tgt Ion:149 Resp: 63637
 Ion Ratio Lower Upper
 149 100
 91 63.5 56.6 85.0
 206 22.7 15.4 23.0


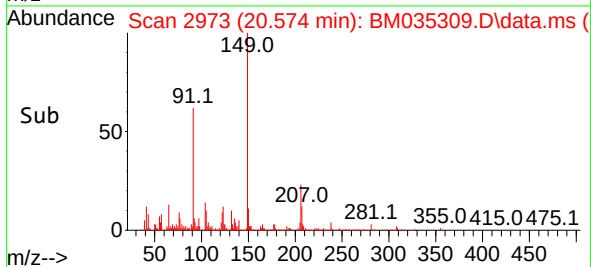
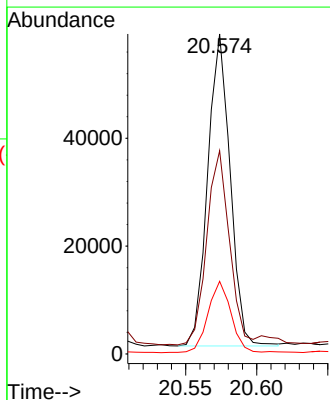
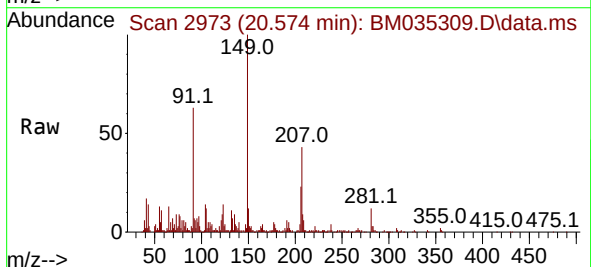


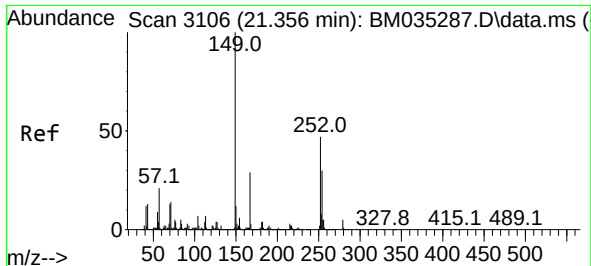

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.540 ng
 RT: 21.350 min Scan# 3106
 Delta R.T. -0.006 min
 Lab File: BM035309.D
 Acq: 28 May 2022 14:47

Instrument :
 BNA_M
 ClientSampleId :
 P009-SS003-0006-01

Tgt Ion:149 Resp: 57311
 Ion Ratio Lower Upper
 149 100
 167 27.4 21.1 31.7
 279 4.6 2.8 4.2#

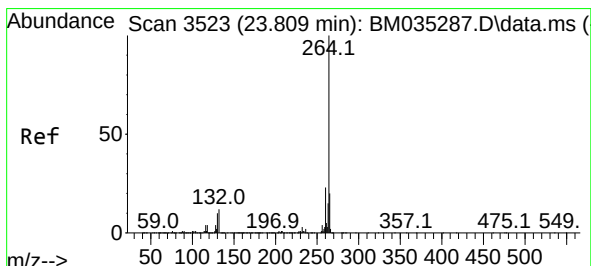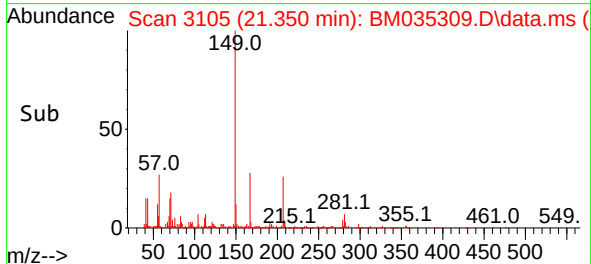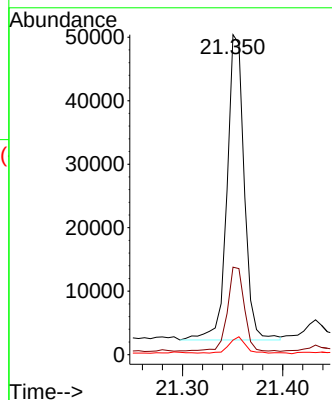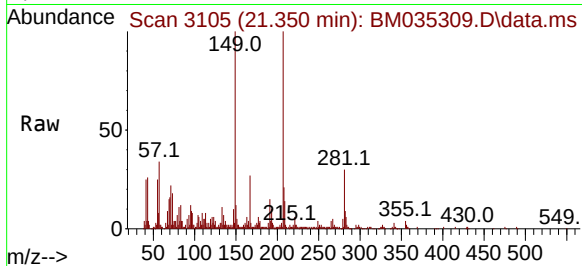

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.803 min Scan# 3522
 Delta R.T. -0.006 min
 Lab File: BM035309.D
 Acq: 28 May 2022 14:47

Tgt Ion:264 Resp: 708802
 Ion Ratio Lower Upper
 264 100
 260 23.7 18.9 28.3
 265 21.8 17.5 26.3

