

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035317.D
 Acq On : 28 May 2022 19:41
 Operator : CG/JU
 Sample : N2930-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P002-SS003-1218-01

Quant Time: May 29 00:34:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 16:44:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	135888	20.000	ng	0.00
21) Naphthalene-d8	10.675	136	492158	20.000	ng	# 0.00
39) Acenaphthene-d10	14.510	164	312057	20.000	ng	0.00
64) Phenanthrene-d10	17.257	188	691461	20.000	ng	0.00
76) Chrysene-d12	21.439	240	682710	20.000	ng	# 0.00
86) Perylene-d12	23.809	264	711968	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	600326	81.569	ng	0.00
7) Phenol-d6	7.051	99	728878	76.484	ng	0.00
23) Nitrobenzene-d5	9.034	82	451247	50.472	ng	0.00
42) 2,4,6-Tribromophenol	16.004	330	333304	82.332	ng	0.00
45) 2-Fluorobiphenyl	13.139	172	1150616	51.132	ng	0.00
79) Terphenyl-d14	19.880	244	1903263	49.400	ng	0.00
Target Compounds						
32) Benzoic acid	10.028	122	63	2.916	ng	# 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035317.D
Acq On : 28 May 2022 19:41
Operator : CG/JU
Sample : N2930-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01

Quant Time: May 29 00:34:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 16:44:39 2022
Response via : Initial Calibration




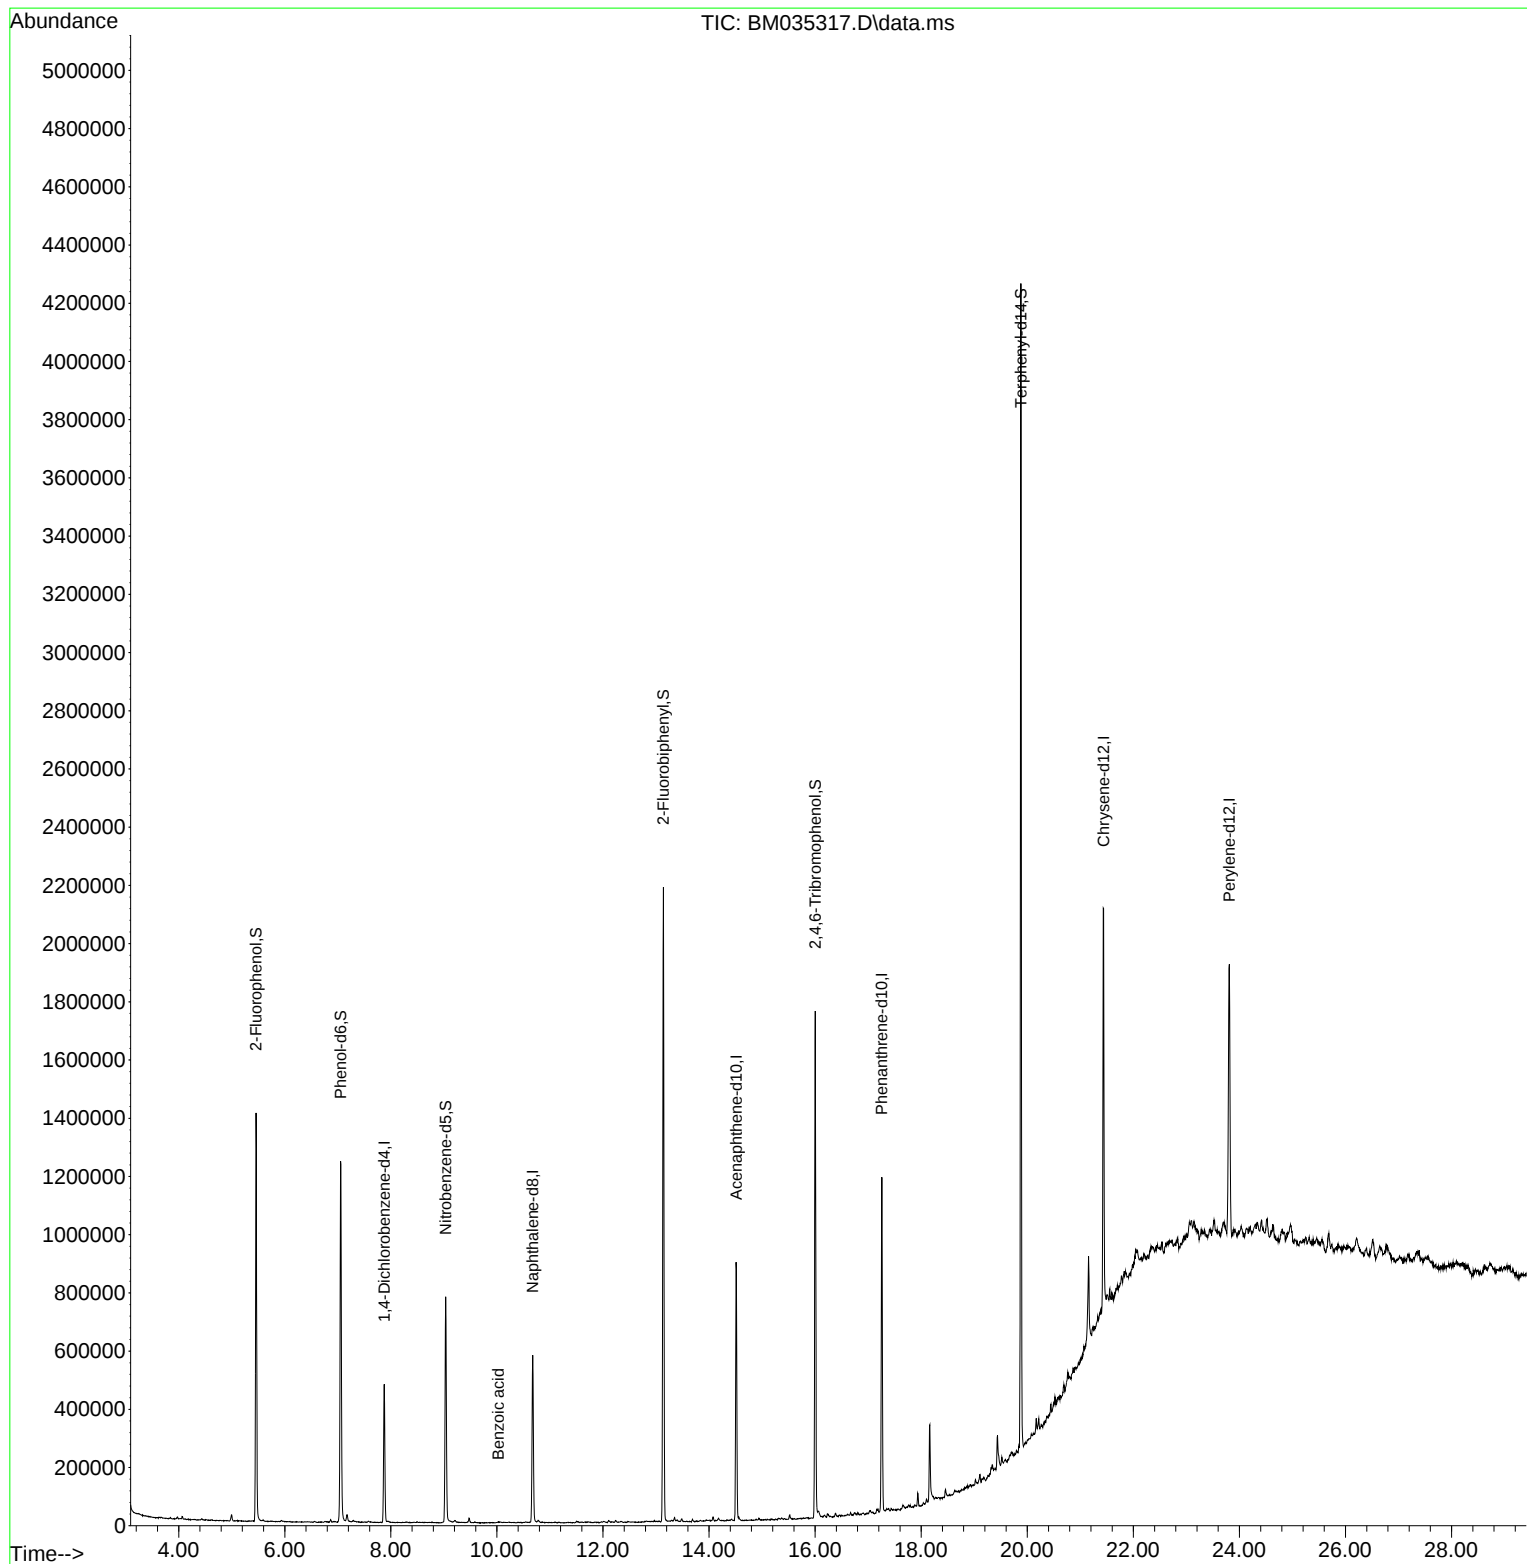


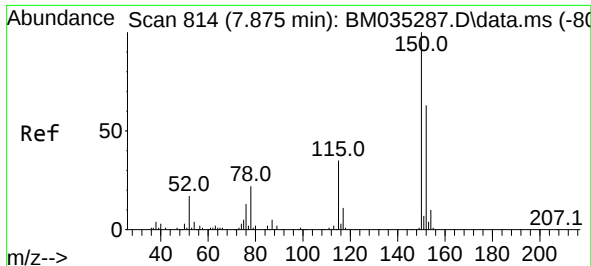

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.875 min Scan# 814
Delta R.T. -0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41




Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01


Tgt Ion:152 Resp: 135888
Ion Ratio Lower Upper
152 100
150 158.3 124.9 187.3
115 57.7 47.9 71.9

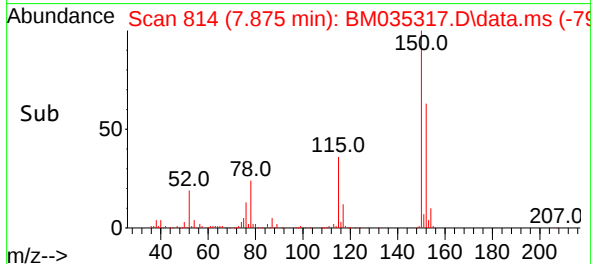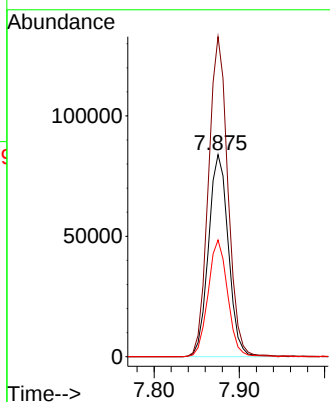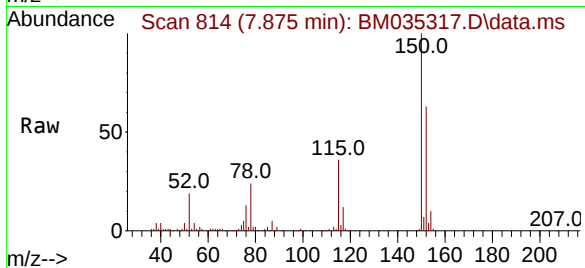

#5
2-Fluorophenol
Concen: 81.569 ng
RT: 5.457 min Scan# 403
Delta R.T. 0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41

Tgt Ion:112 Resp: 600326
Ion Ratio Lower Upper
112 100
64 56.4 47.8 71.6
63 29.8 26.6 40.0


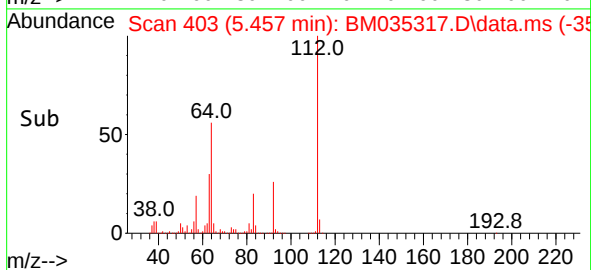
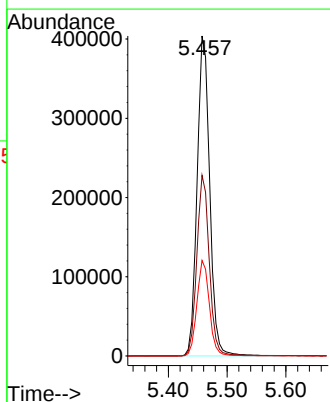
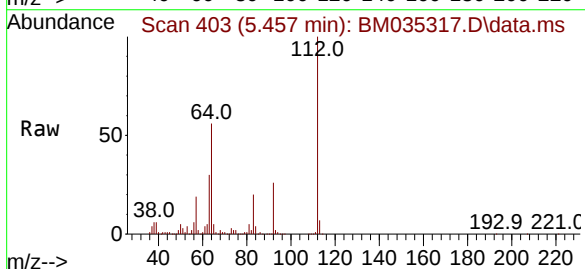


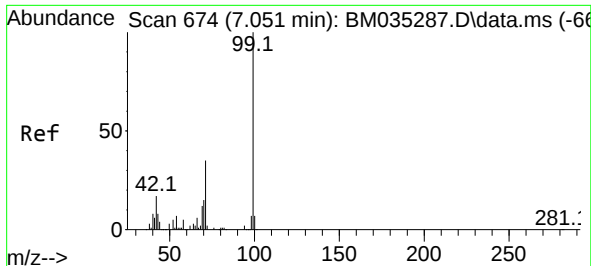

#7
Phenol-d6
Concen: 76.484 ng
RT: 7.051 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41




Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01


Tgt Ion: 99 Resp: 728878
Ion Ratio Lower Upper
99 100
42 19.0 18.8 28.2
71 35.9 30.2 45.2

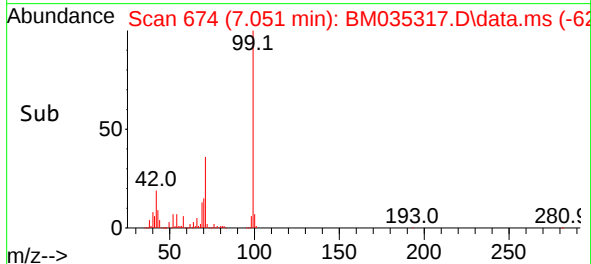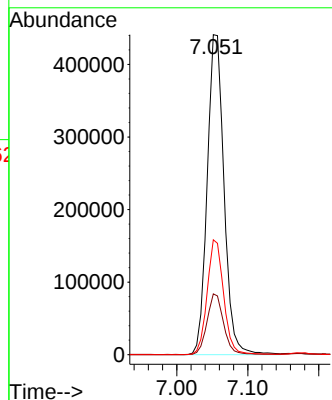

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.675 min Scan# 1290
Delta R.T. -0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41

Tgt Ion: 136 Resp: 492158
Ion Ratio Lower Upper
136 100
137 11.2 8.9 13.3
54 6.7 7.0 10.4#
68 5.0 4.3 6.5

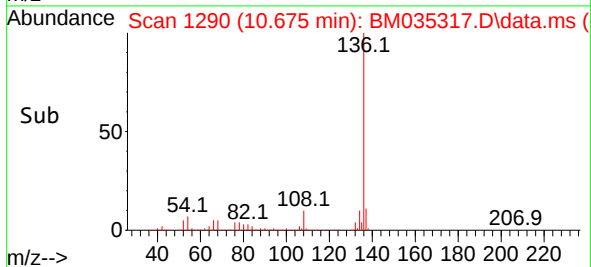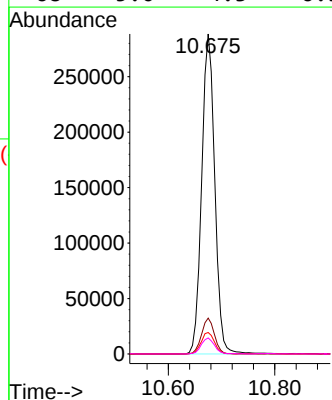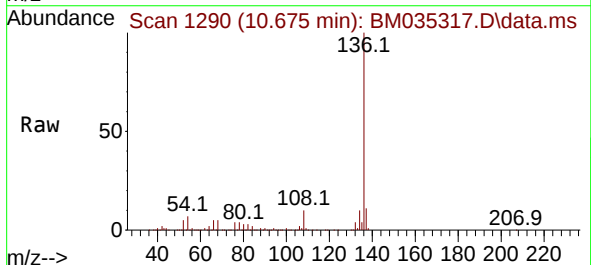



#23

Nitrobenzene-d5

Concen: 50.472 ng

RT: 9.034 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM035317.D


Acq: 28 May 2022 19:41

Instrument :

BNA_M

ClientSampleId :

P002-SS003-1218-01






Tgt Ion: 82 Resp: 451247

Ion Ratio Lower Upper

82 100

128 45.2 33.7 50.5

54 49.8 43.2 64.8

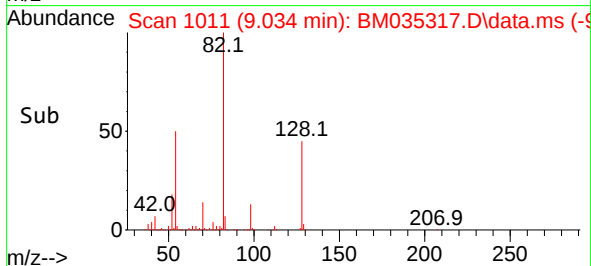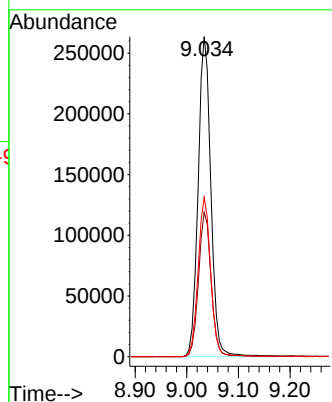

#32

Benzoic acid

Concen: 2.916 ng

RT: 10.028 min Scan# 1180

Delta R.T. 0.018 min

Lab File: BM035317.D

Acq: 28 May 2022 19:41




Tgt Ion:122 Resp: 63


Ion Ratio Lower Upper

122 100

105 110.6 105.7 145.7

77 233.5 80.0 120.0#


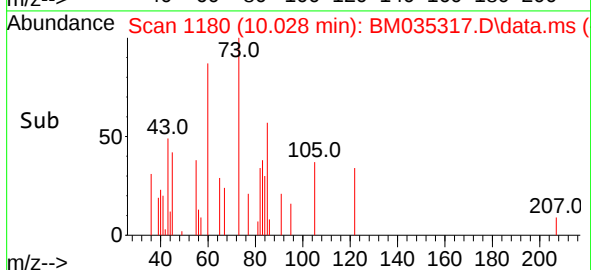
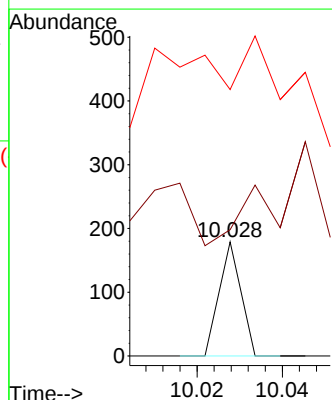
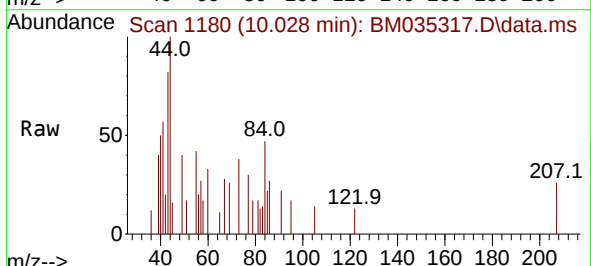


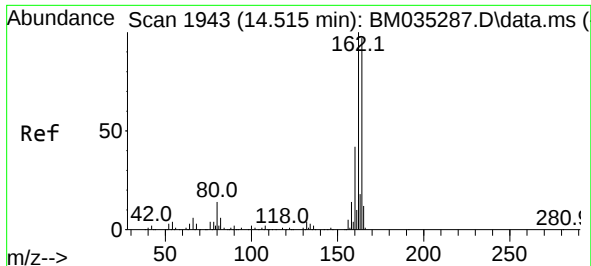

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.510 min Scan# 1942
Delta R.T. -0.005 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41




Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01


Tgt Ion:164 Resp: 312057
Ion Ratio Lower Upper
164 100
162 102.9 83.0 124.6
160 45.6 37.0 55.4

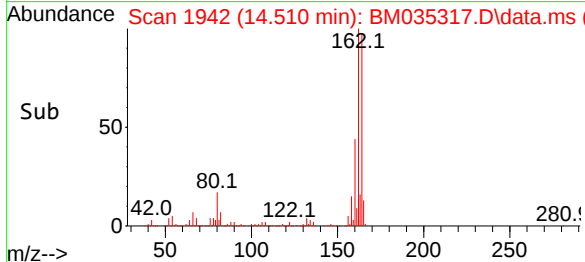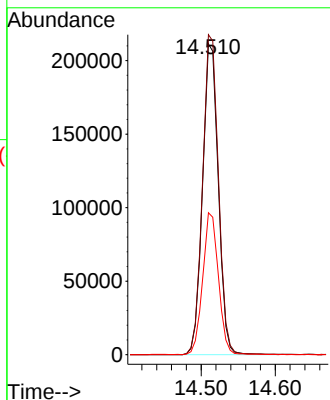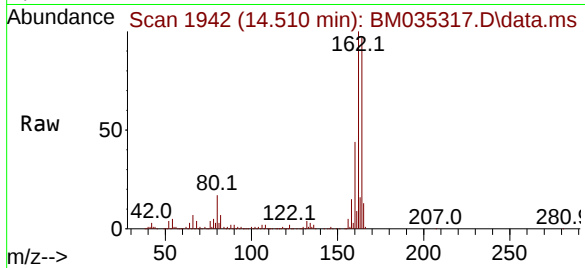

#42
2,4,6-Tribromophenol
Concen: 82.332 ng
RT: 16.004 min Scan# 2196
Delta R.T. -0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41

Tgt Ion:330 Resp: 333304
Ion Ratio Lower Upper
330 100
332 96.2 77.0 115.4
141 33.9 35.3 52.9#


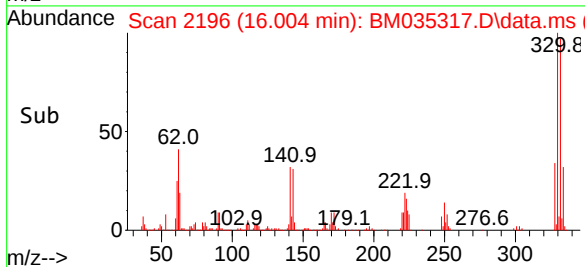
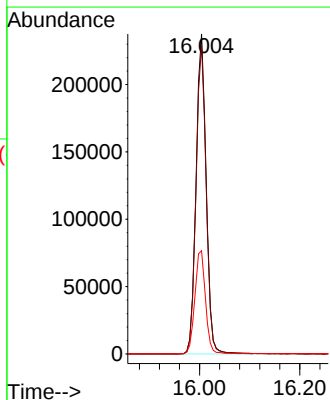
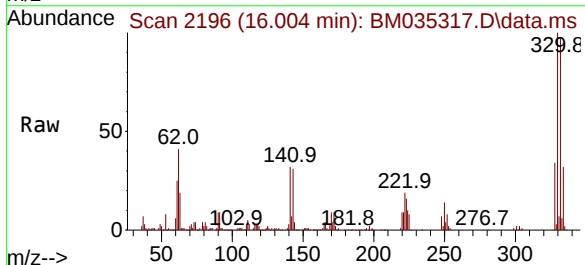


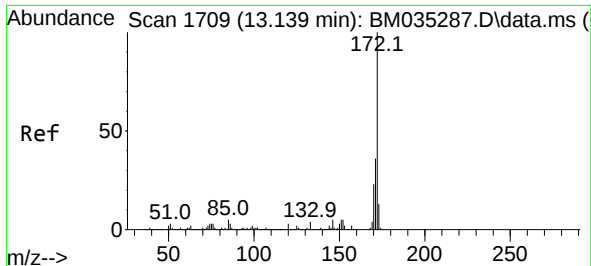

#45
2-Fluorobiphenyl
Concen: 51.132 ng
RT: 13.139 min Scan# 1709
Delta R.T. 0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41




Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01


Tgt Ion:172 Resp: 1150616
Ion Ratio Lower Upper
172 100
171 34.7 28.5 42.7
170 23.1 18.7 28.1

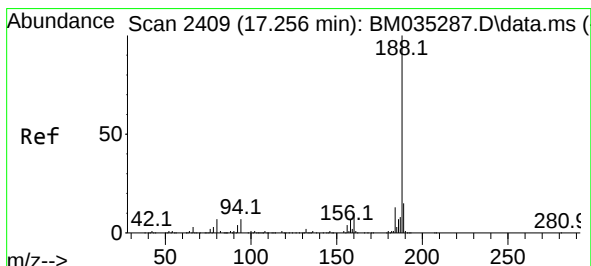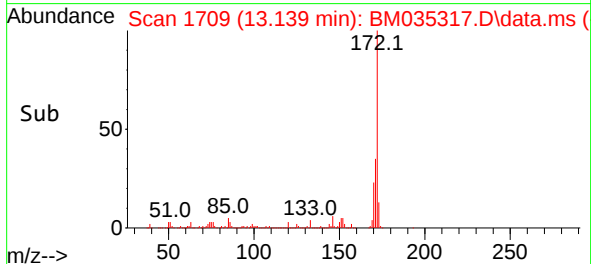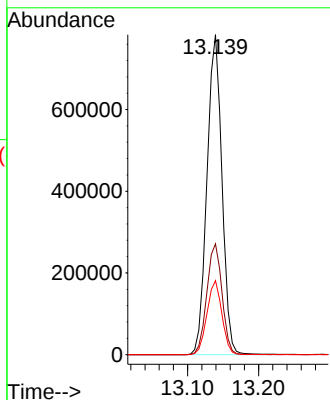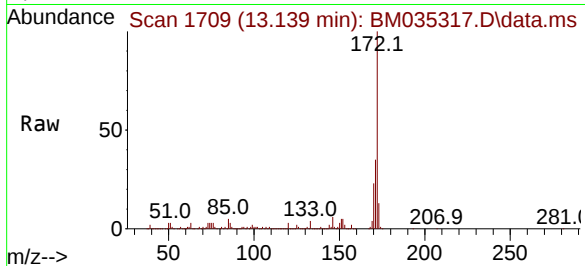

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.257 min Scan# 2409
Delta R.T. 0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41

Tgt Ion:188 Resp: 691461
Ion Ratio Lower Upper
188 100
94 7.0 7.0 10.4
80 7.7 7.6 11.4


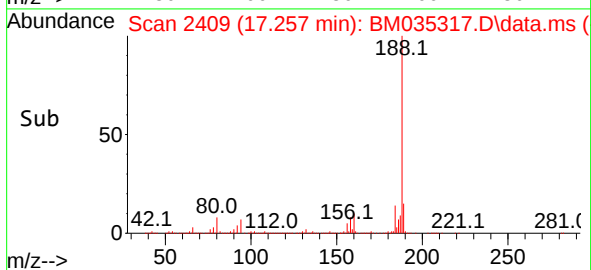
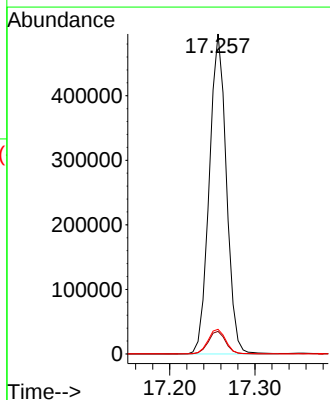
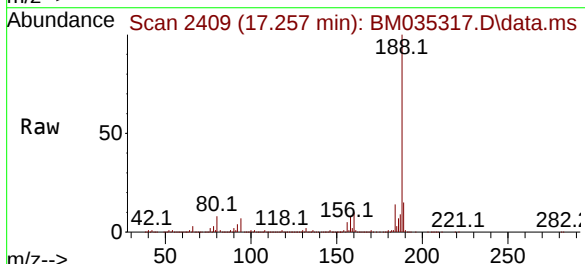


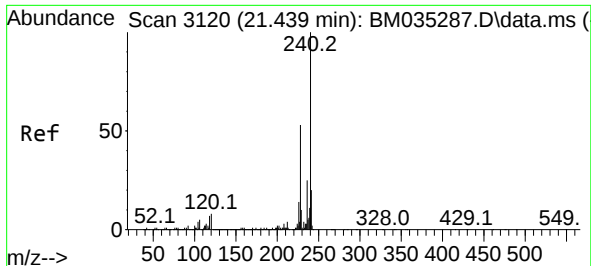

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.439 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41




Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01


Tgt Ion:240 Resp: 682710
Ion Ratio Lower Upper
240 100
120 8.2 9.4 14.0#
236 25.9 20.6 30.8

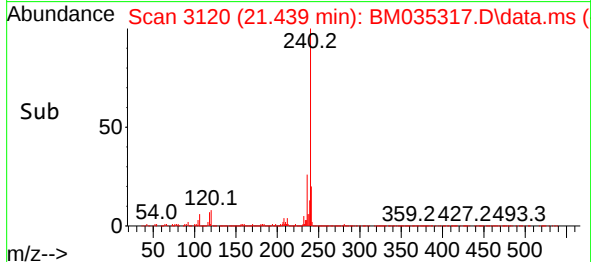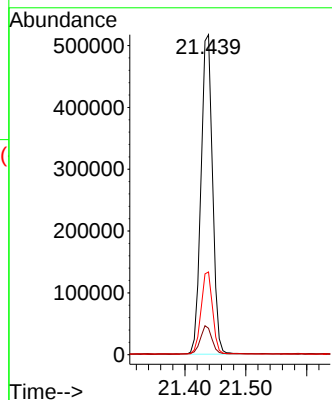

#79
Terphenyl-d14
Concen: 49.400 ng
RT: 19.880 min Scan# 2855
Delta R.T. 0.000 min
Lab File: BM035317.D
Acq: 28 May 2022 19:41

Tgt Ion:244 Resp: 1903263
Ion Ratio Lower Upper
244 100
212 7.1 6.2 9.4
122 8.8 8.3 12.5

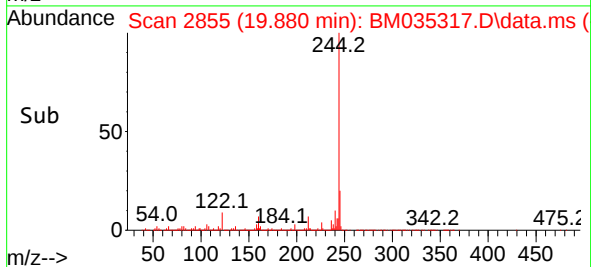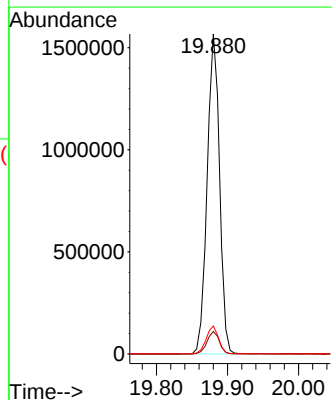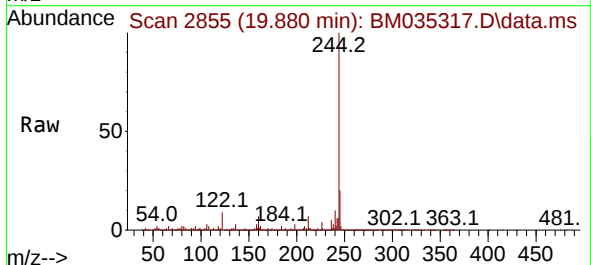



#86

Perylene-d12

Concen: 20.000 ng

RT: 23.809 min Scan# 3

Delta R.T. 0.000 min

Lab File: BM035317.D


Acq: 28 May 2022 19:41

Instrument :

BNA_M

ClientSampleId :

P002-SS003-1218-01

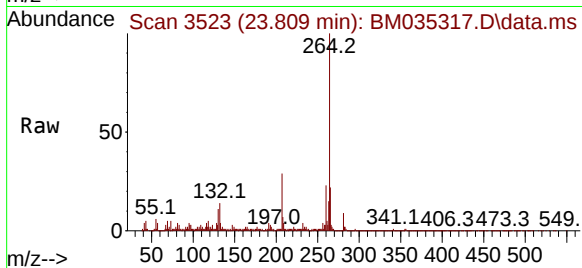

Tgt Ion:264 Resp: 711968

Ion Ratio Lower Upper

264 100

260 23.1 18.9 28.3

265 21.6 17.5 26.3

