
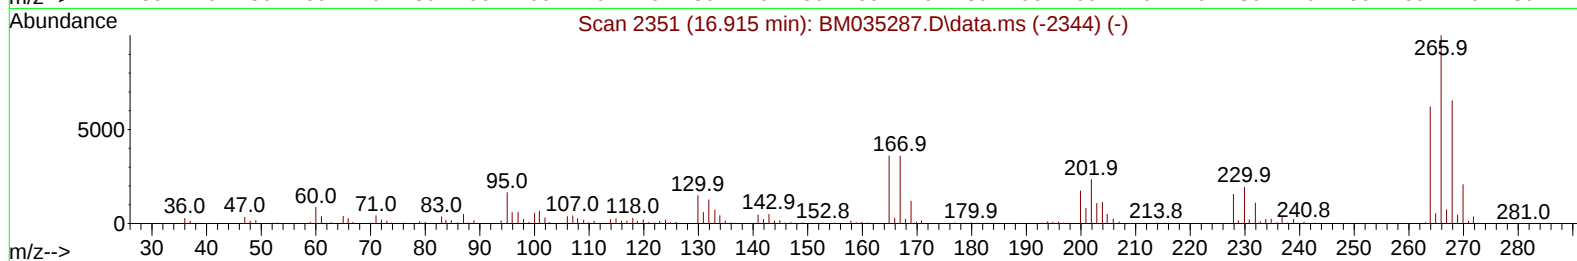
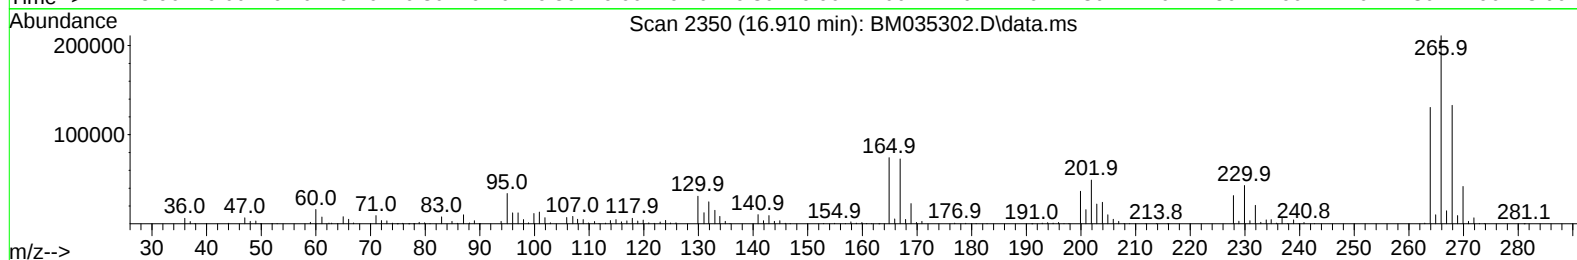


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035302.D
 Acq On : 28 May 2022 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 04:26:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 16:44:39 2022
 Response via : Initial Calibration

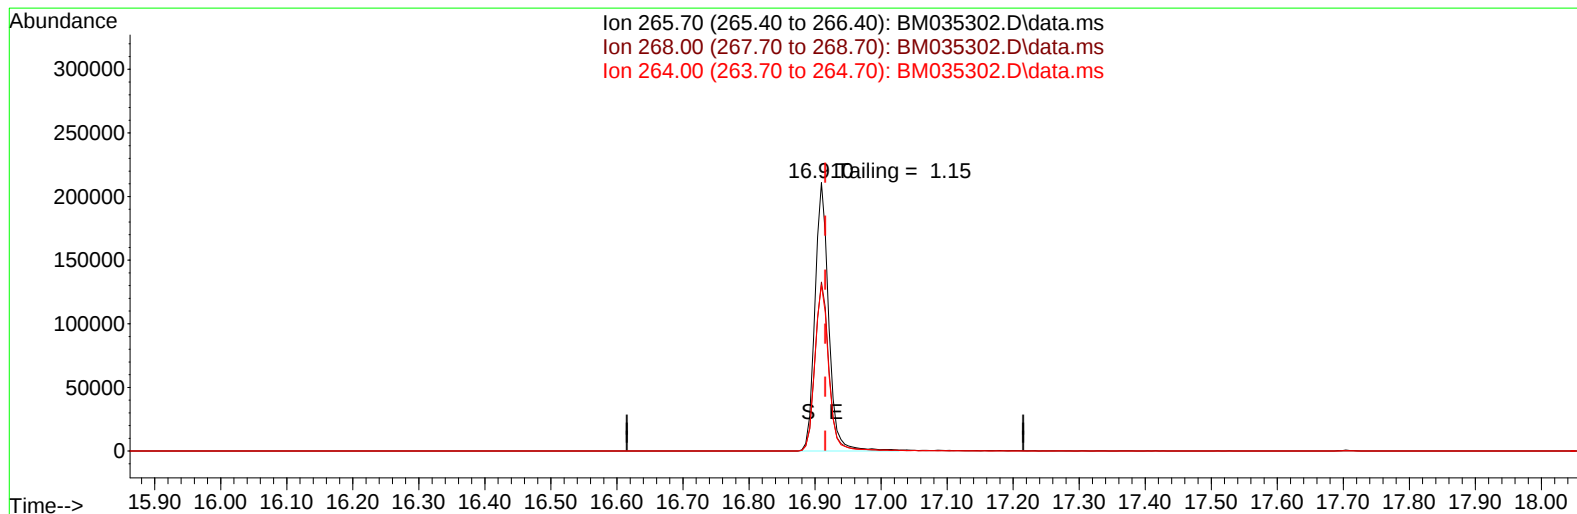

TIC: BM035302.D\data.ms




(70) Pentachlorophenol (C)

16.910min (-0.006) 0.00 ng

response 306966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.99
264.00	63.30	61.92
0.00	0.00	0.00

Quant Time: May 29 04:26:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 16:44:39 2022
Response via : Initial Calibration

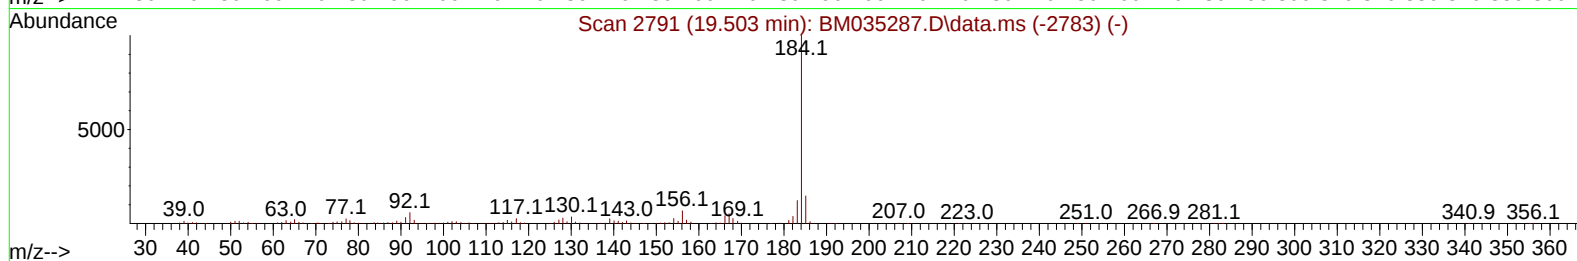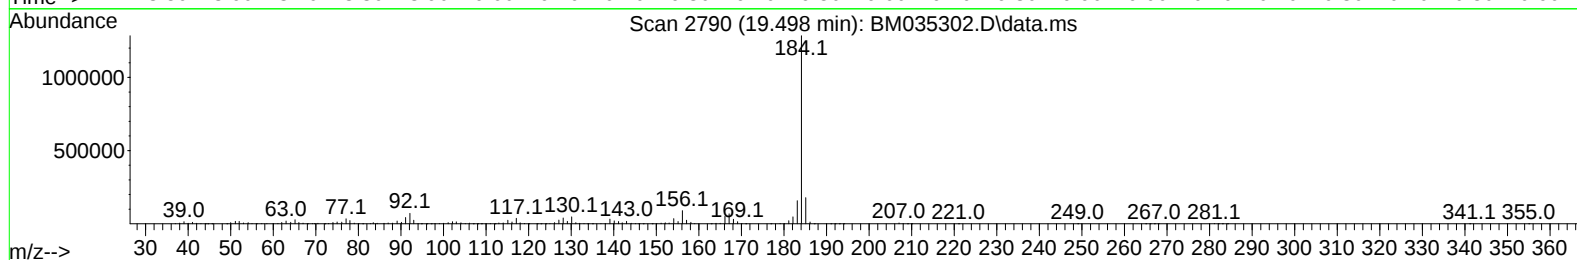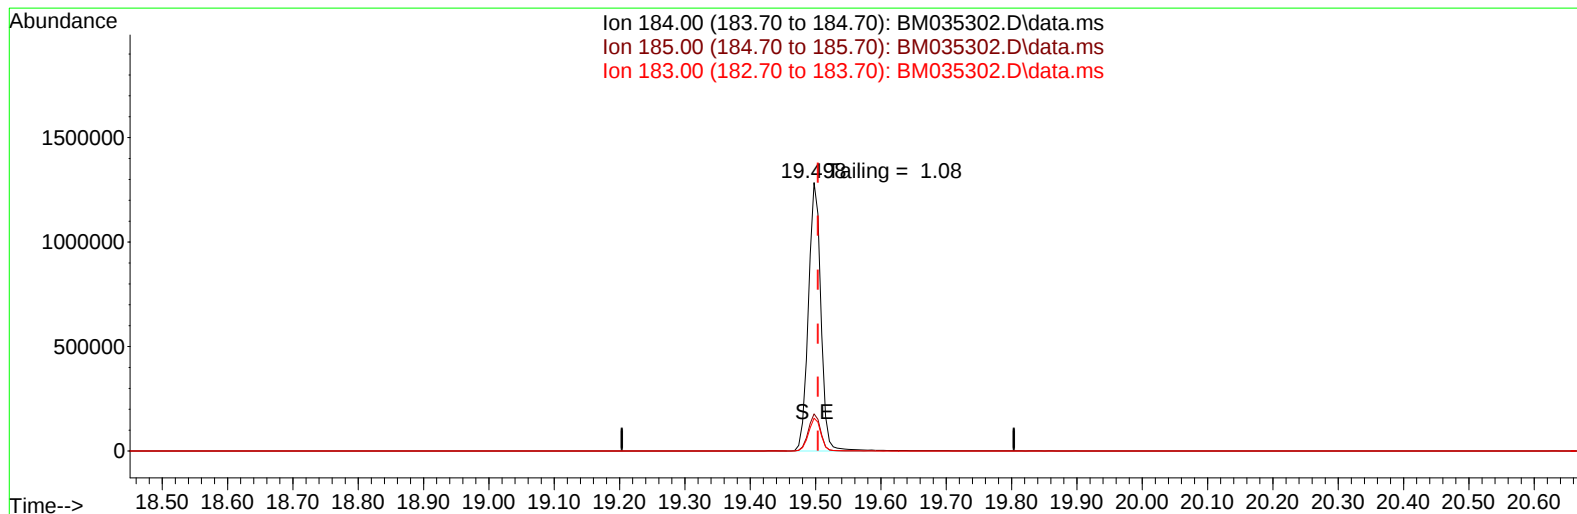

TIC: BM035302.D\data.ms

(77) Benzidine

19.498min (-0.006) 165261.52 ng

response **1717362**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.10	13.87
--------	-------	-------

183.00	11.90	12.24
--------	-------	-------

0.00 0.00 0.00