

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035304.D
 Acq On : 28 May 2022 11:39
 Operator : CG/JU
 Sample : PB145147BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145147BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	420	rBV	2463571	3585027	36.88%	9.329%
2	7.051	666	674	695	rBV	2317332	3694277	38.00%	9.613%
3	7.875	806	814	821	rBV	425110	683361	7.03%	1.778%
4	9.034	1003	1011	1026	rBV	1423473	2357504	24.25%	6.135%
5	10.675	1282	1290	1304	rBV	525811	933176	9.60%	2.428%
6	13.139	1701	1709	1721	rBV	4076504	6047978	62.22%	15.738%
7	14.510	1935	1942	1952	rBV	906474	1319457	13.57%	3.434%
8	15.998	2188	2195	2217	rBV	3345675	4683138	48.18%	12.187%
9	17.251	2402	2408	2421	rBV	1086877	1609011	16.55%	4.187%
10	19.880	2849	2855	2860	rBV	8189560	9721068	100.00%	25.297%
11	21.433	3114	3119	3128	rBV	1441346	1903067	19.58%	4.952%
12	23.803	3515	3522	3534	rVB	944142	1891119	19.45%	4.921%




Sum of corrected areas: 38428183

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035304.D
Acq On : 28 May 2022 11:39
Operator : CG/JU
Sample : PB145147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

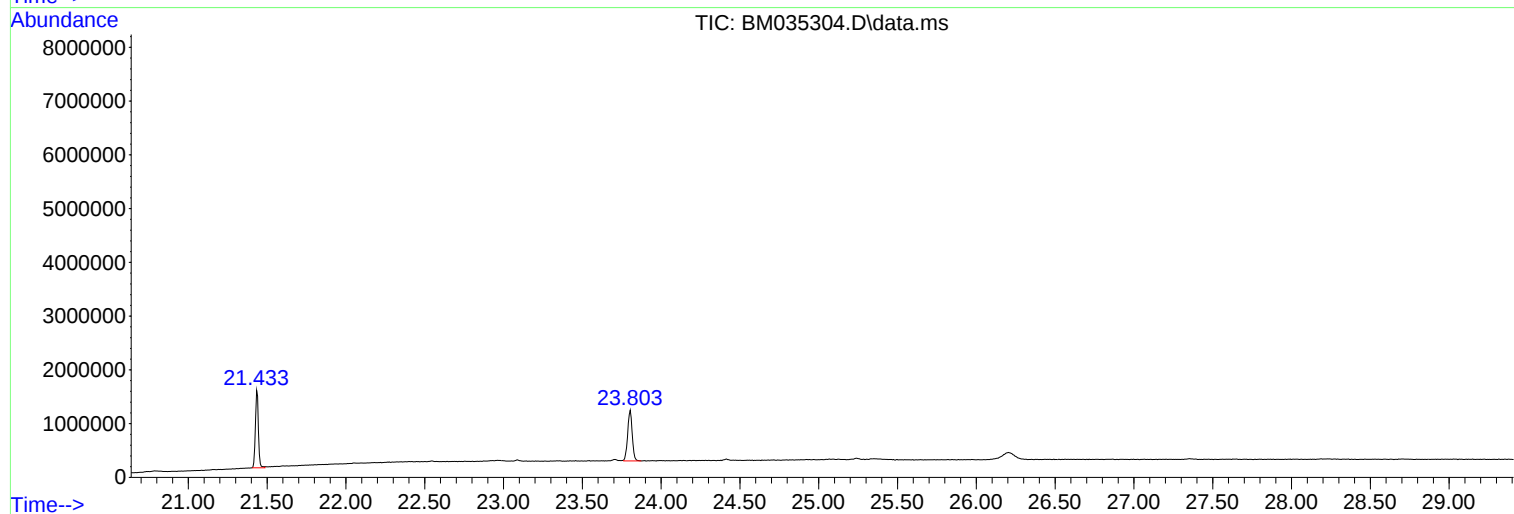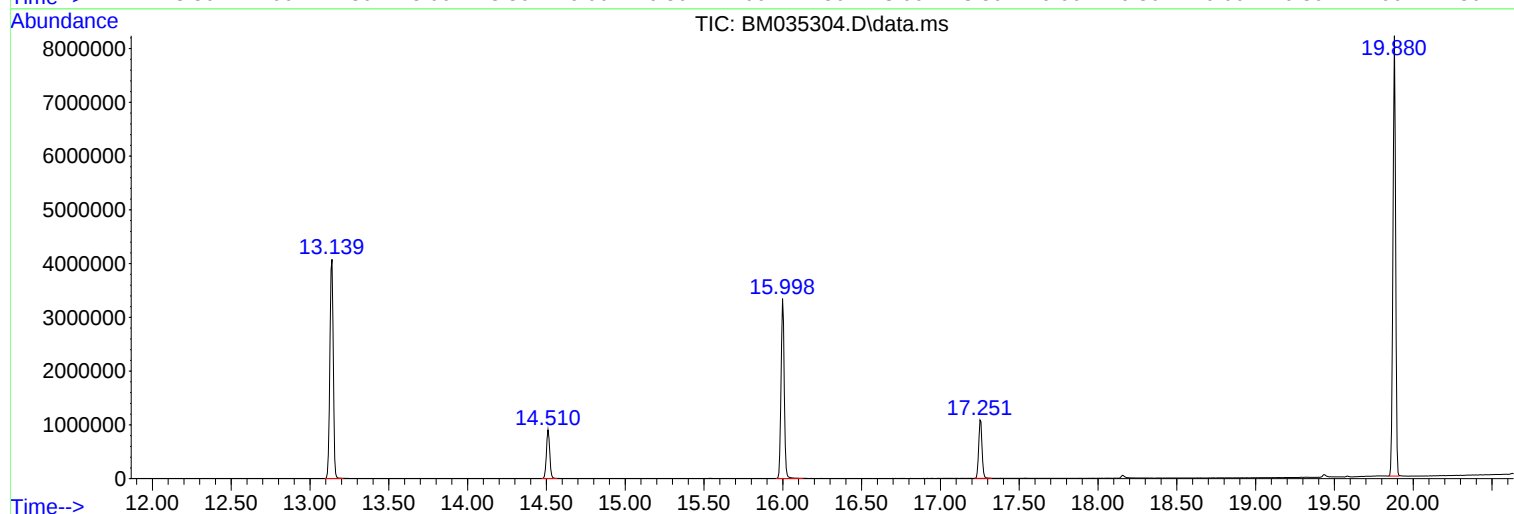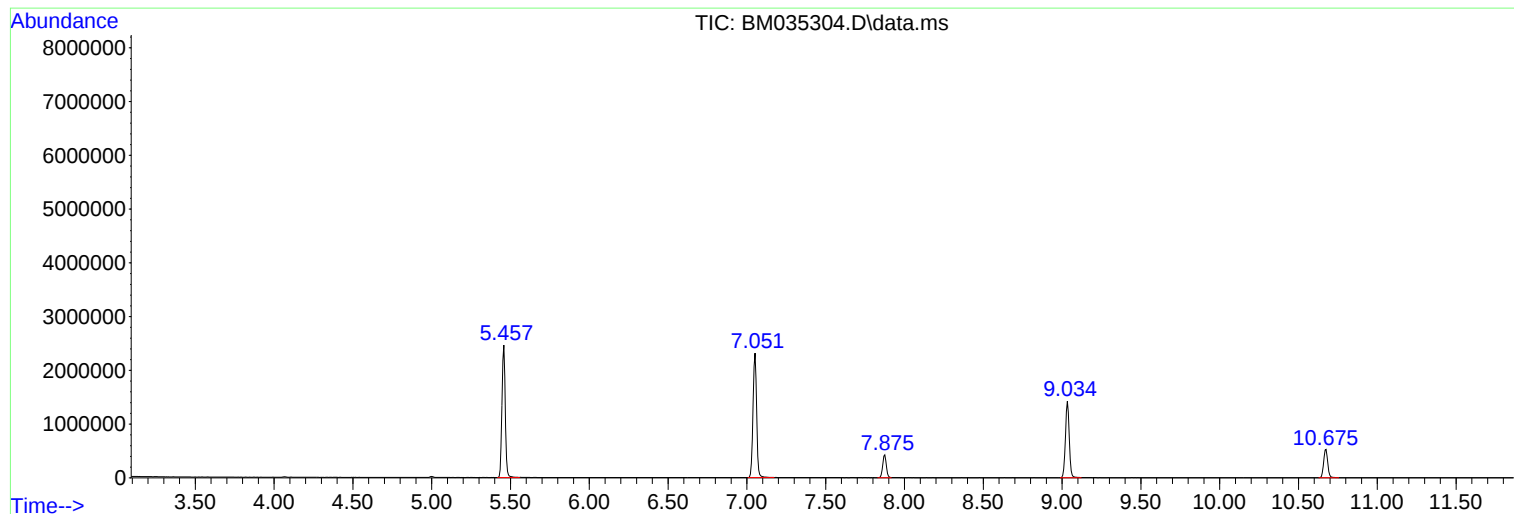

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035304.D
Acq On : 28 May 2022 11:39
Operator : CG/JU
Sample : PB145147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035304.D
Acq On : 28 May 2022 11:39
Operator : CG/JU
Sample : PB145147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------