

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035309.D
 Acq On : 28 May 2022 14:47
 Operator : CG/JU
 Sample : N2931-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P009-SS003-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	318	324	329	rBV	50158	74358	1.53%	0.273%
2	5.457	396	403	418	rBV	1252910	1889796	38.95%	6.947%
3	7.045	666	673	687	rBV	1127498	1913006	39.43%	7.032%
4	7.875	807	814	822	rBV	353135	578853	11.93%	2.128%
5	9.033	1002	1011	1023	rBV	737205	1262009	26.01%	4.639%
6	10.675	1282	1290	1305	rBV	423906	751237	15.49%	2.761%
7	13.133	1701	1708	1721	rBV	1943381	2862621	59.01%	10.523%
8	14.510	1935	1942	1948	rBV	642019	924546	19.06%	3.399%
9	14.563	1948	1951	1959	rVB	36454	51129	1.05%	0.188%
10	15.515	2107	2113	2120	rBV	310038	398574	8.22%	1.465%
11	15.998	2188	2195	2203	rBV	1492258	2075070	42.77%	7.628%
12	16.233	2228	2235	2241	rBV	40145	57351	1.18%	0.211%
13	16.662	2302	2308	2315	rBV2	52664	80993	1.67%	0.298%
14	17.033	2366	2371	2377	rBV5	33269	48755	1.00%	0.179%
15	17.251	2401	2408	2415	rBV	771871	1127839	23.25%	4.146%
16	17.733	2485	2490	2494	rBV	33512	50119	1.03%	0.184%
17	18.156	2557	2562	2570	rBV	286760	419454	8.65%	1.542%
18	18.227	2570	2574	2578	rVB	48282	66871	1.38%	0.246%
19	18.456	2608	2613	2622	rBV3	56286	111012	2.29%	0.408%
20	18.827	2672	2676	2681	rBV	58989	79025	1.63%	0.290%
21	19.098	2718	2722	2727	rVB	54131	65275	1.35%	0.240%
22	19.180	2730	2736	2742	rVV3	61629	135700	2.80%	0.499%
23	19.315	2754	2759	2769	rVB	293325	378378	7.80%	1.391%
24	19.433	2775	2779	2790	rBV2	122007	226879	4.68%	0.834%
25	19.527	2791	2795	2802	rVB4	101407	145708	3.00%	0.536%
26	19.880	2849	2855	2861	rBV	3867114	4851252	100.00%	17.833%
27	20.168	2900	2904	2911	rBV5	80215	124758	2.57%	0.459%
28	20.415	2943	2946	2948	rBV	78928	97545	2.01%	0.359%
29	20.445	2948	2951	2955	rVB2	120523	144070	2.97%	0.530%
30	20.497	2956	2960	2968	rBV	321640	394264	8.13%	1.449%
31	20.574	2969	2973	2976	rBV	257000	334685	6.90%	1.230%
32	20.609	2976	2979	2984	rVB4	90282	122976	2.53%	0.452%
33	20.909	3026	3030	3034	rBV	158234	203489	4.19%	0.748%
34	20.956	3034	3038	3044	rVB	275663	381900	7.87%	1.404%
35	21.156	3068	3072	3081	rVB2	387861	635627	13.10%	2.336%
36	21.350	3103	3105	3109	rVB	143355	151736	3.13%	0.558%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035309.D
Acq On : 28 May 2022 14:47
Operator : CG/JU
Sample : N2931-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.433	3115	3119	3123	rBV	1323671	1728498	35.63%	6.354%
38	22.680	3327	3331	3337	rVB	288979	410128	8.45%	1.508%
39	23.803	3516	3522	3530	rVB2	926641	1848929	38.11%	6.796%




Sum of corrected areas: 27204415

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035309.D
Acq On : 28 May 2022 14:47
Operator : CG/JU
Sample : N2931-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

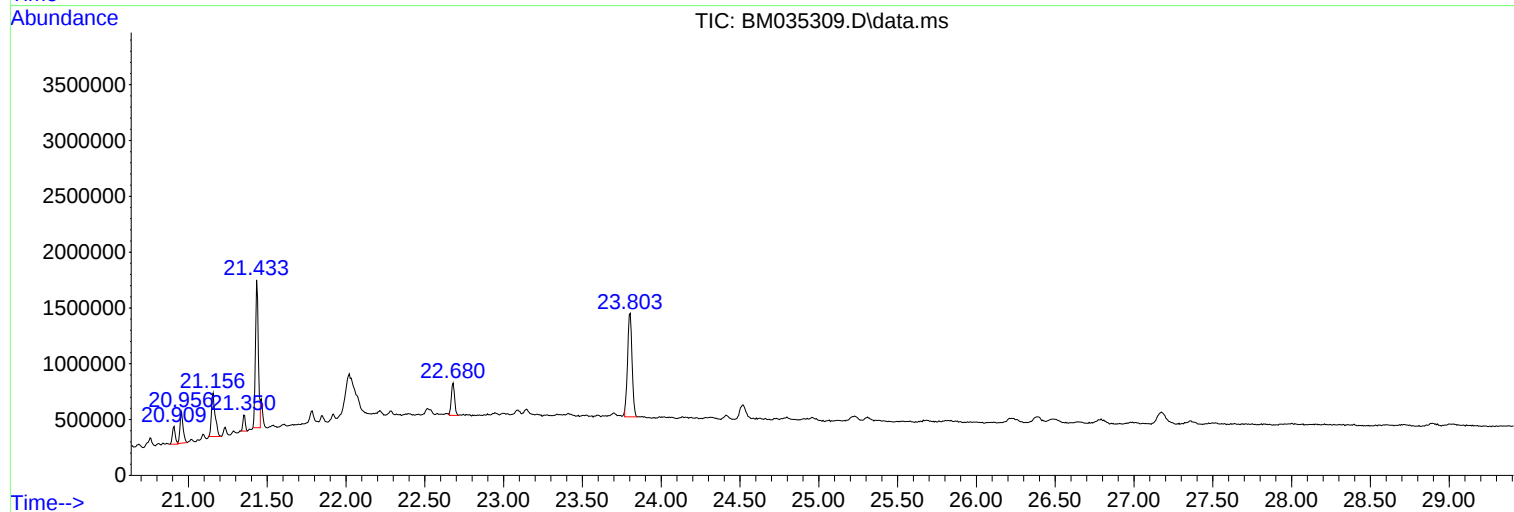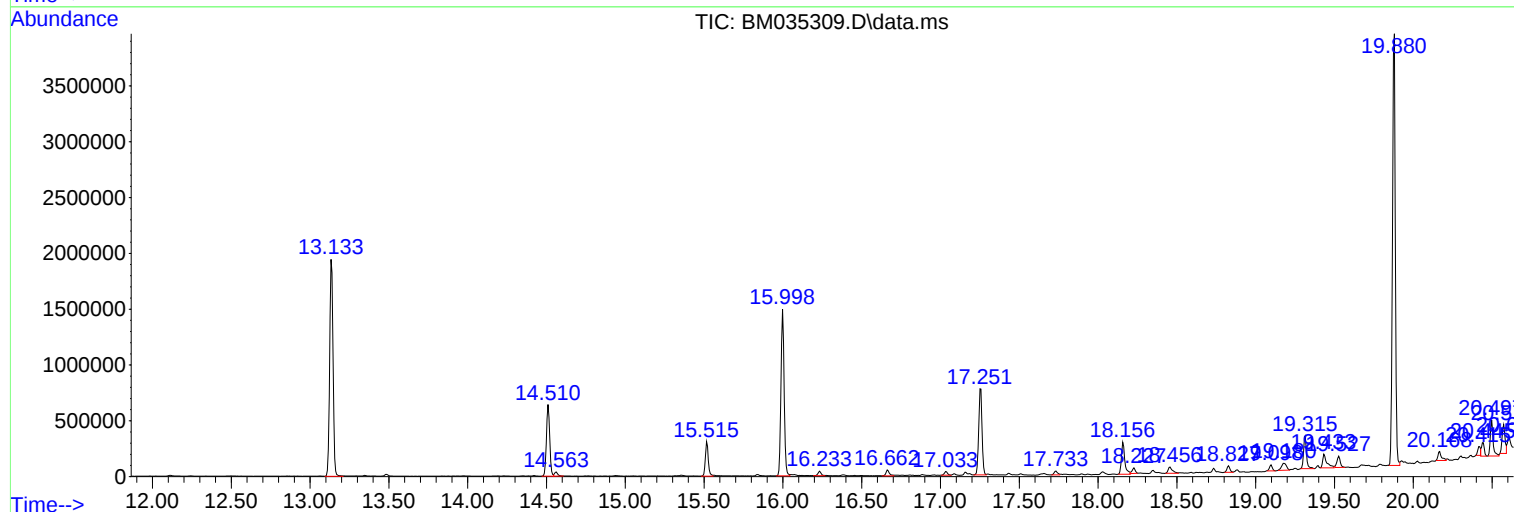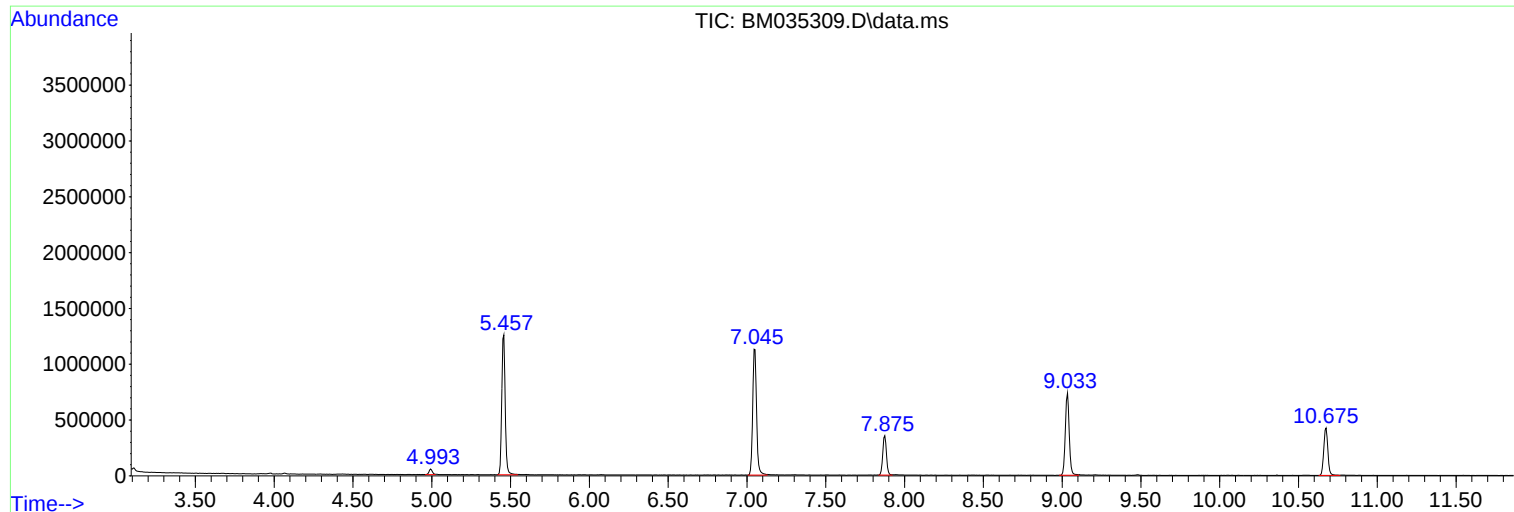

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035309.D
Acq On : 28 May 2022 14:47
Operator : CG/JU
Sample : N2931-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035309.D
Acq On : 28 May 2022 14:47
Operator : CG/JU
Sample : N2931-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P009-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------