

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035311.D
 Acq On : 28 May 2022 16:01
 Operator : CG/JU
 Sample : N2921-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P013-SS002-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	418	rBV	1451194	2154509	35.97%	6.698%
2	7.051	665	674	686	rBV	1371934	2222649	37.11%	6.910%
3	7.875	807	814	820	rBV	383310	607308	10.14%	1.888%
4	9.033	1002	1011	1027	rBV	856539	1446078	24.15%	4.495%
5	10.675	1282	1290	1301	rBV	455541	781354	13.05%	2.429%
6	13.139	1701	1709	1724	rBV	2339804	3511691	58.64%	10.917%
7	14.510	1934	1942	1949	rBV	714022	1043327	17.42%	3.243%
8	15.998	2189	2195	2203	rBV	1923779	2737754	45.71%	8.511%
9	17.256	2401	2409	2415	rBV	917952	1321875	22.07%	4.109%
10	17.933	2520	2524	2531	rBV	50150	65058	1.09%	0.202%
11	18.162	2557	2563	2578	rBV	1030506	1474654	24.62%	4.584%
12	18.456	2609	2613	2618	rBV	47333	66549	1.11%	0.207%
13	19.109	2720	2724	2727	rVB2	106973	131326	2.19%	0.408%
14	19.321	2756	2760	2772	rVB	849934	1133723	18.93%	3.524%
15	19.439	2775	2780	2792	rBV	1594651	2129915	35.56%	6.621%
16	19.692	2820	2823	2838	rVB2	404478	546530	9.13%	1.699%
17	19.880	2850	2855	2860	rBV	5013669	5988943	100.00%	18.618%
18	21.156	3068	3072	3080	rVB	671873	895812	14.96%	2.785%
19	21.433	3115	3119	3129	rBV	1334650	2079669	34.73%	6.465%
20	23.803	3517	3522	3530	rVB2	918614	1828703	30.53%	5.685%




Sum of corrected areas: 32167427

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035311.D
Acq On : 28 May 2022 16:01
Operator : CG/JU
Sample : N2921-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS002-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

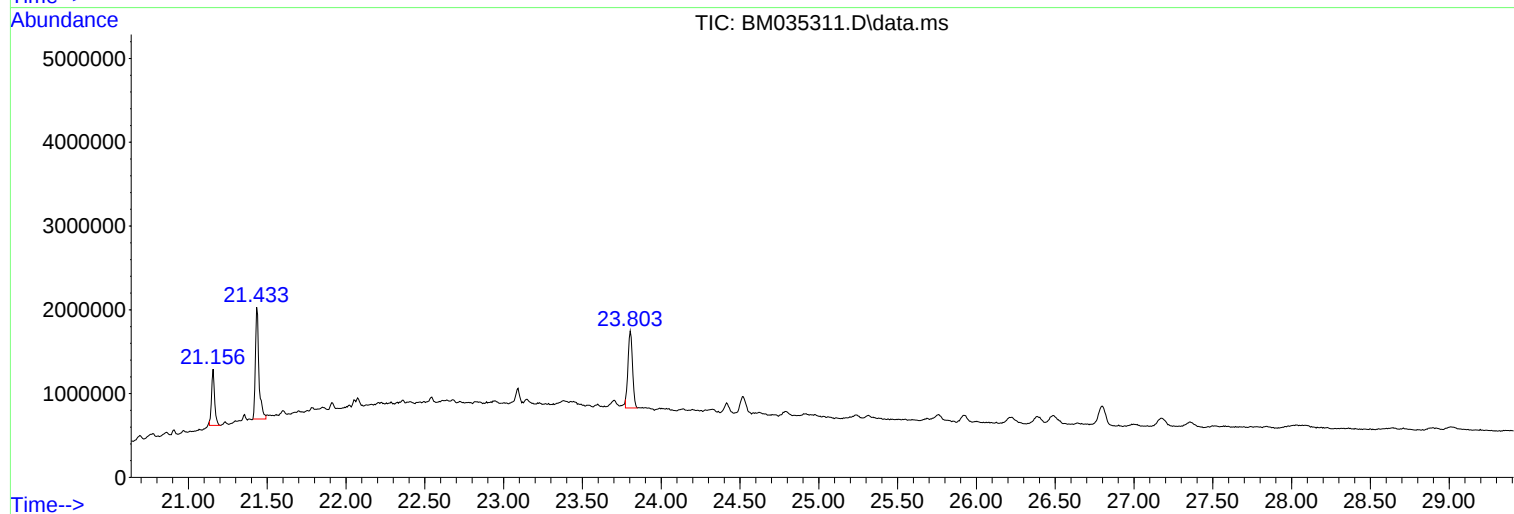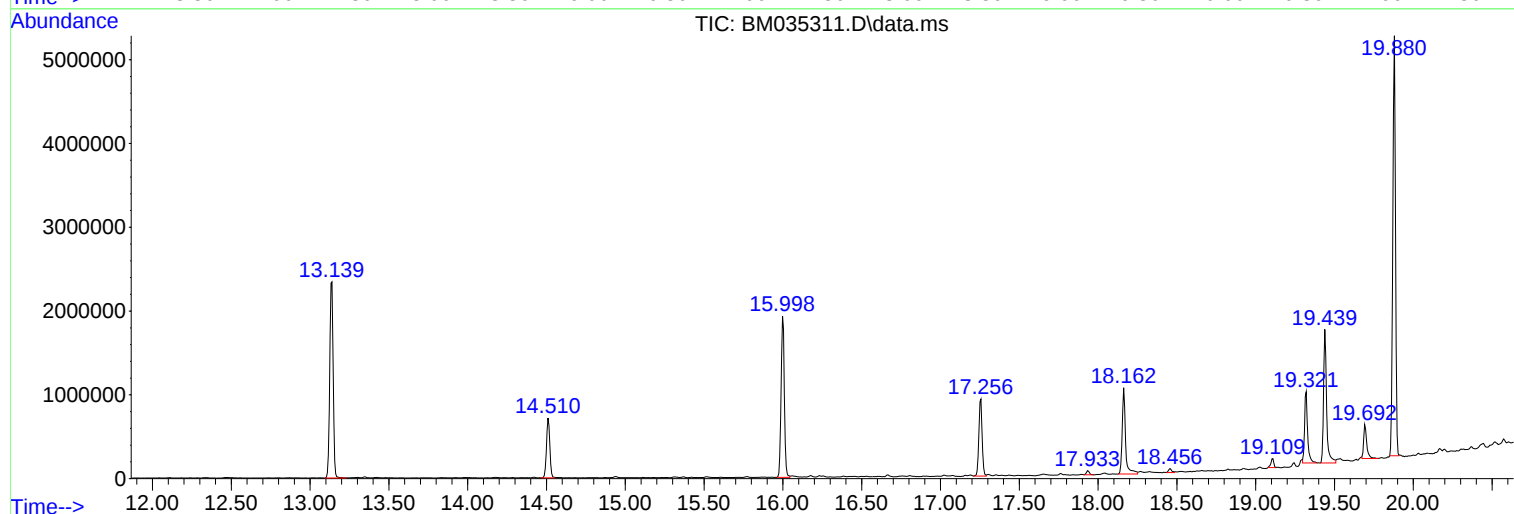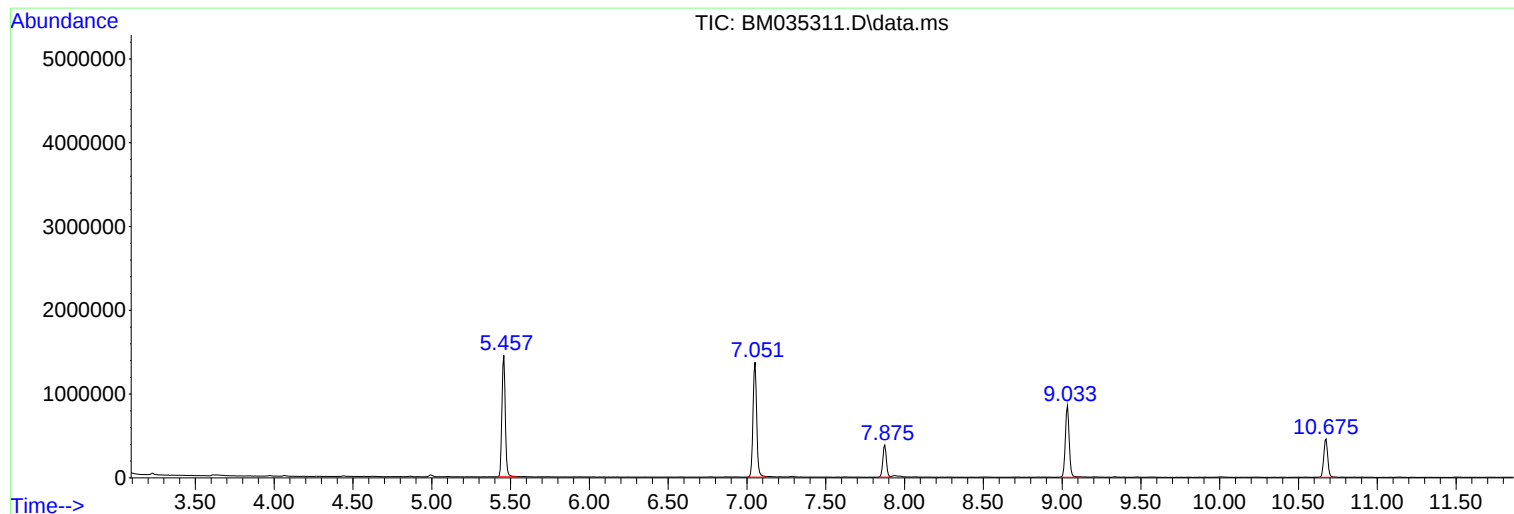

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035311.D
Acq On : 28 May 2022 16:01
Operator : CG/JU
Sample : N2921-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS002-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035311.D
Acq On : 28 May 2022 16:01
Operator : CG/JU
Sample : N2921-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS002-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------