

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035312.D
 Acq On : 28 May 2022 16:38
 Operator : CG/JU
 Sample : N2934-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P025-SS001-0612-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	421	rBV	928130	1392717	27.82%	5.195%
2	7.051	665	674	688	rBV	827394	1410814	28.18%	5.262%
3	7.875	807	814	822	rBV	375919	592437	11.83%	2.210%
4	9.034	1004	1011	1023	rBV	507439	879832	17.58%	3.282%
5	10.675	1282	1290	1303	rBV	443890	772965	15.44%	2.883%
6	13.133	1702	1708	1724	rBV	1470373	2210785	44.16%	8.246%
7	14.510	1935	1942	1957	rBV	711827	1036906	20.71%	3.868%
8	15.998	2189	2195	2203	rBV	1135247	1688692	33.73%	6.299%
9	17.251	2402	2408	2415	rBV	869856	1279696	25.56%	4.773%
10	18.156	2557	2562	2571	rBV	363367	544884	10.88%	2.032%
11	19.315	2756	2759	2768	rVB2	54550	93710	1.87%	0.350%
12	19.433	2775	2779	2789	rBV	372512	576305	11.51%	2.150%
13	19.698	2822	2824	2830	rVB	44214	50425	1.01%	0.188%
14	19.880	2849	2855	2863	rBV	2997926	3647903	72.87%	13.606%
15	20.168	2900	2904	2907	rBV3	65505	86476	1.73%	0.323%
16	20.445	2947	2951	2955	rBV	138009	162713	3.25%	0.607%
17	20.574	2969	2973	2976	rBV	205017	228043	4.56%	0.851%
18	20.756	3002	3004	3010	rVB2	104092	131379	2.62%	0.490%
19	20.909	3027	3030	3034	rVB	112452	132262	2.64%	0.493%
20	21.156	3066	3072	3080	rVB2	261250	564987	11.29%	2.107%
21	21.356	3102	3106	3109	rBV	589765	648358	12.95%	2.418%
22	21.433	3115	3119	3129	rBV	1256291	1903030	38.01%	7.098%
23	23.803	3516	3522	3531	rVB2	903401	1768789	35.33%	6.597%
24	26.797	4022	4031	4045	rVB2	1611504	5006081	100.00%	18.672%




Sum of corrected areas: 26810189

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035312.D
Acq On : 28 May 2022 16:38
Operator : CG/JU
Sample : N2934-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P025-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

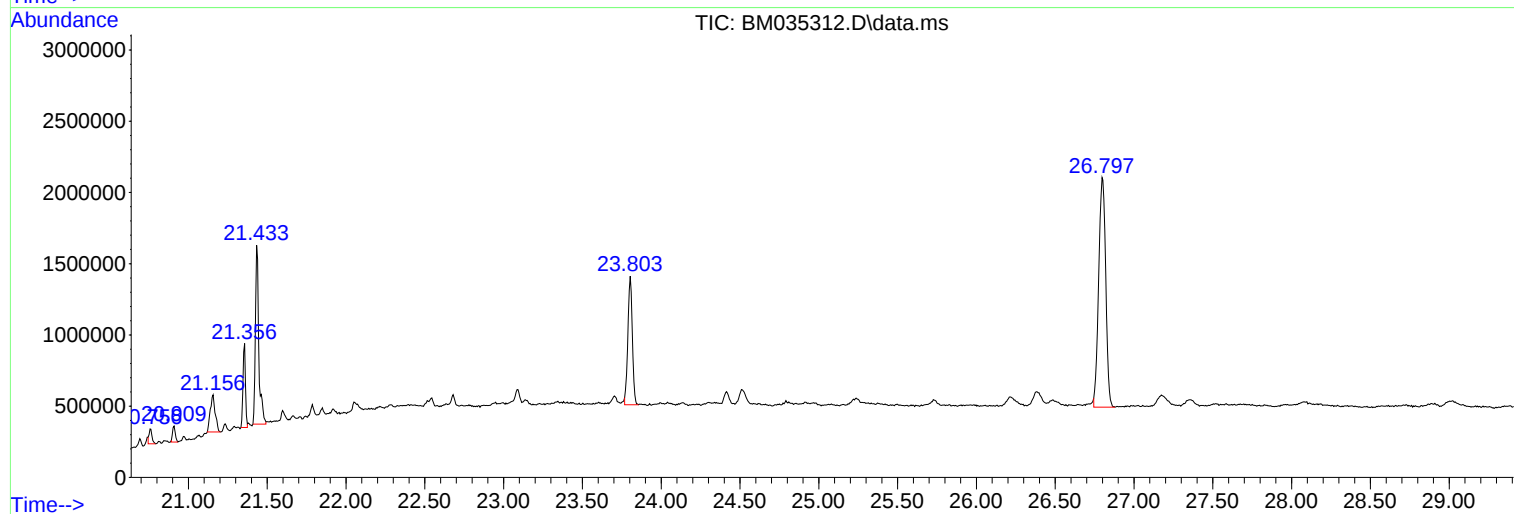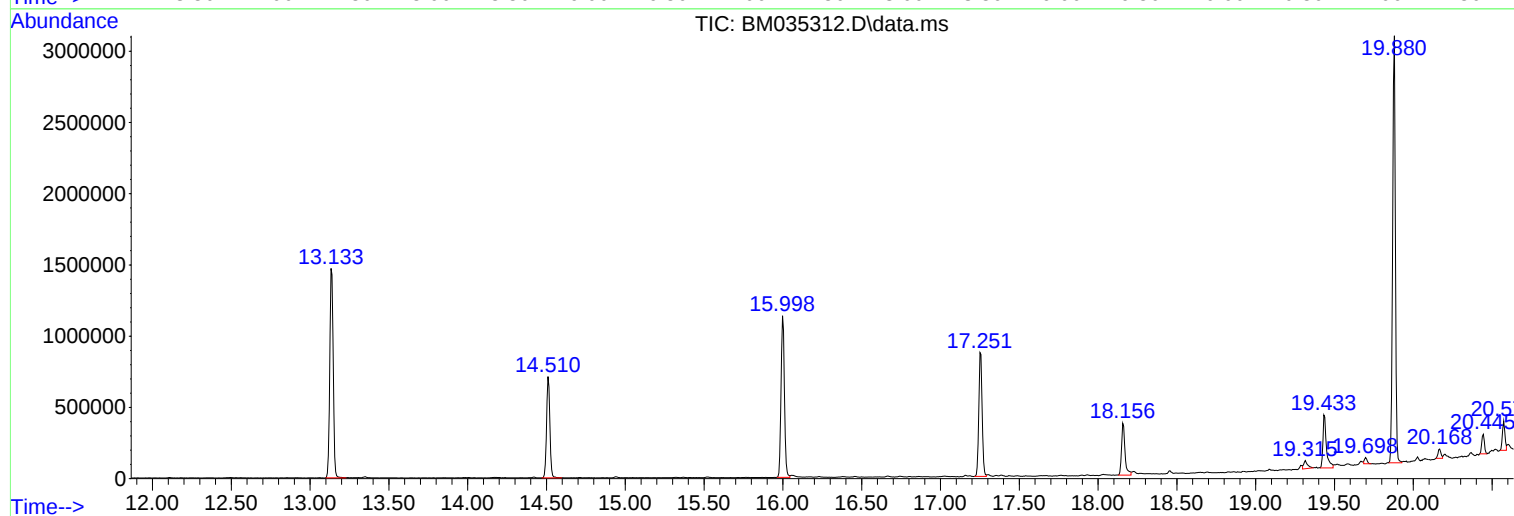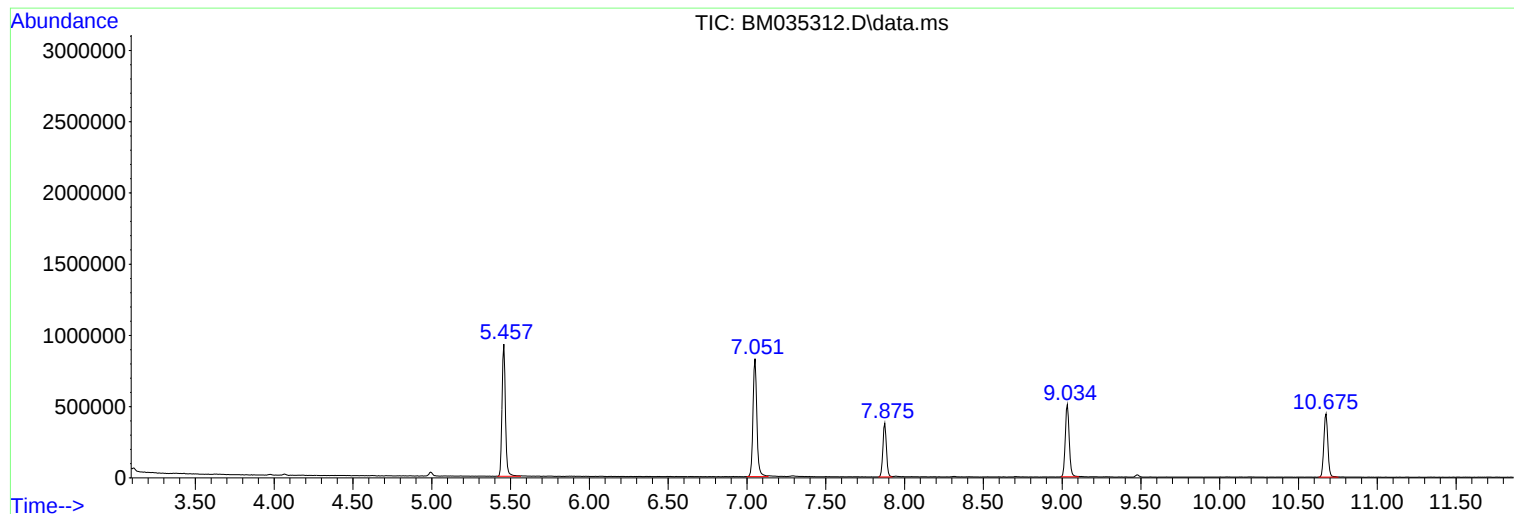

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035312.D
Acq On : 28 May 2022 16:38
Operator : CG/JU
Sample : N2934-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P025-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035312.D
Acq On : 28 May 2022 16:38
Operator : CG/JU
Sample : N2934-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P025-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------