

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035315.D
 Acq On : 28 May 2022 18:28
 Operator : CG/JU
 Sample : N2928-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P026-SS001-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.999	317	325	332	rVB	57542	90947	1.23%	0.266%
2	5.457	397	403	422	rBV	2067056	3047105	41.23%	8.925%
3	7.057	665	675	687	rBV	1853188	3060289	41.41%	8.963%
4	7.875	806	814	820	rBV	427339	680913	9.21%	1.994%
5	9.034	1003	1011	1019	rBV	1199784	1974600	26.72%	5.783%
6	10.675	1282	1290	1303	rBV	497558	852935	11.54%	2.498%
7	12.463	1587	1594	1606	rBV	28852	93365	1.26%	0.273%
8	13.139	1702	1709	1722	rVB	3109404	4541731	61.45%	13.302%
9	14.510	1936	1942	1948	rBV	691850	1024254	13.86%	3.000%
10	15.998	2189	2195	2203	rBV	2237452	3320116	44.92%	9.724%
11	16.068	2203	2207	2217	rVB7	35803	82942	1.12%	0.243%
12	16.804	2328	2332	2339	rVB2	54642	77440	1.05%	0.227%
13	17.257	2403	2409	2414	rBV	870055	1219022	16.49%	3.570%
14	18.162	2558	2563	2577	rBV	363434	569465	7.71%	1.668%
15	19.027	2707	2710	2713	rBV2	59562	83353	1.13%	0.244%
16	19.439	2776	2780	2790	rBV	324749	562253	7.61%	1.647%
17	19.880	2850	2855	2865	rVB	5969065	7390598	100.00%	21.646%
18	20.168	2901	2904	2907	rVB2	144041	154433	2.09%	0.452%
19	20.445	2948	2951	2955	rVB	267875	291600	3.95%	0.854%
20	20.909	3027	3030	3034	rVB2	368719	377275	5.10%	1.105%
21	21.356	3103	3106	3110	rBV	453745	456023	6.17%	1.336%
22	21.439	3116	3120	3122	rBV	1285894	1611799	21.81%	4.721%
23	21.462	3122	3124	3129	rVB2	719995	860897	11.65%	2.521%
24	23.809	3520	3523	3531	rVB2	897054	1719532	23.27%	5.036%




Sum of corrected areas: 34142887

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035315.D
Acq On : 28 May 2022 18:28
Operator : CG/JU
Sample : N2928-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P026-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

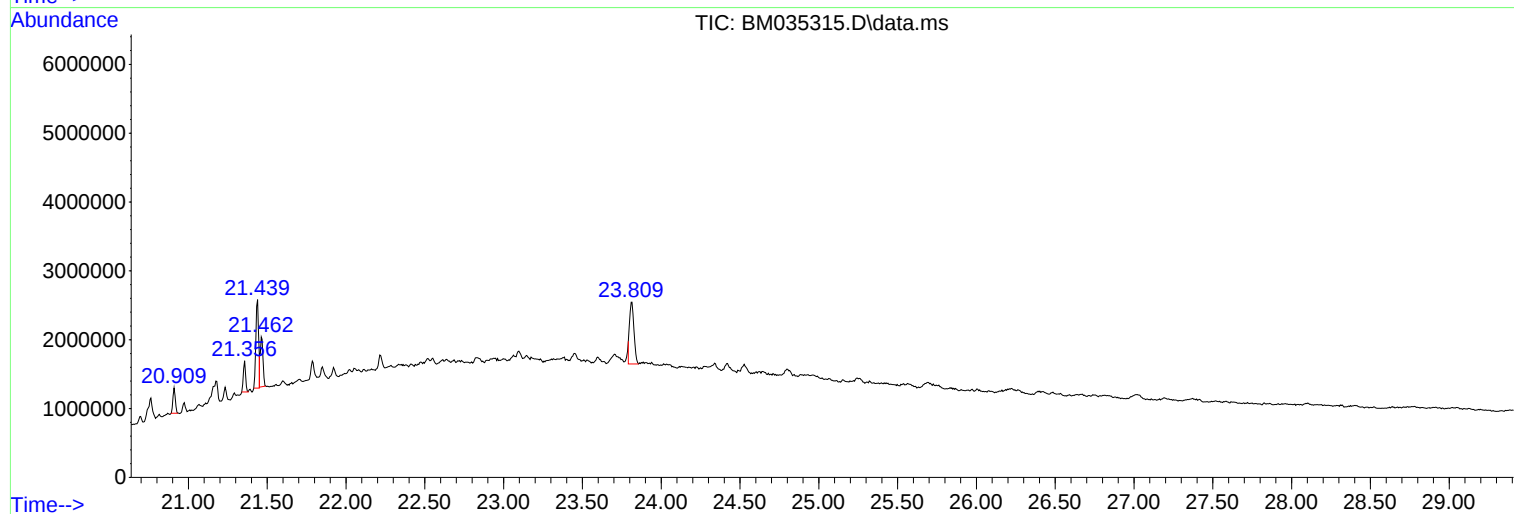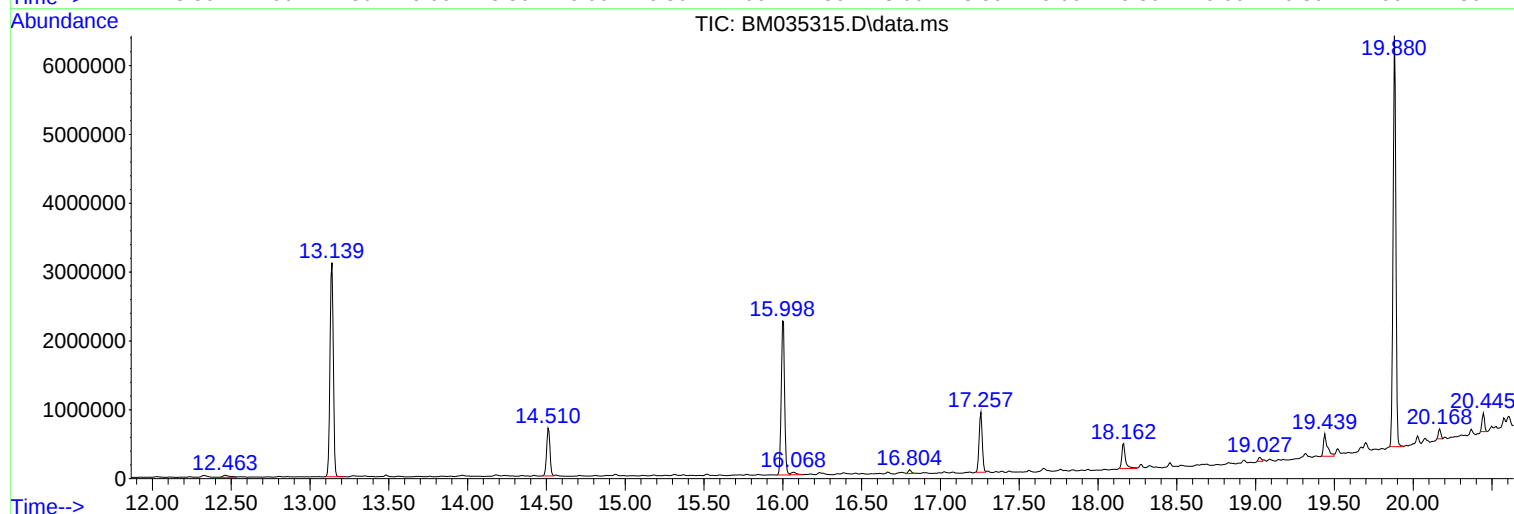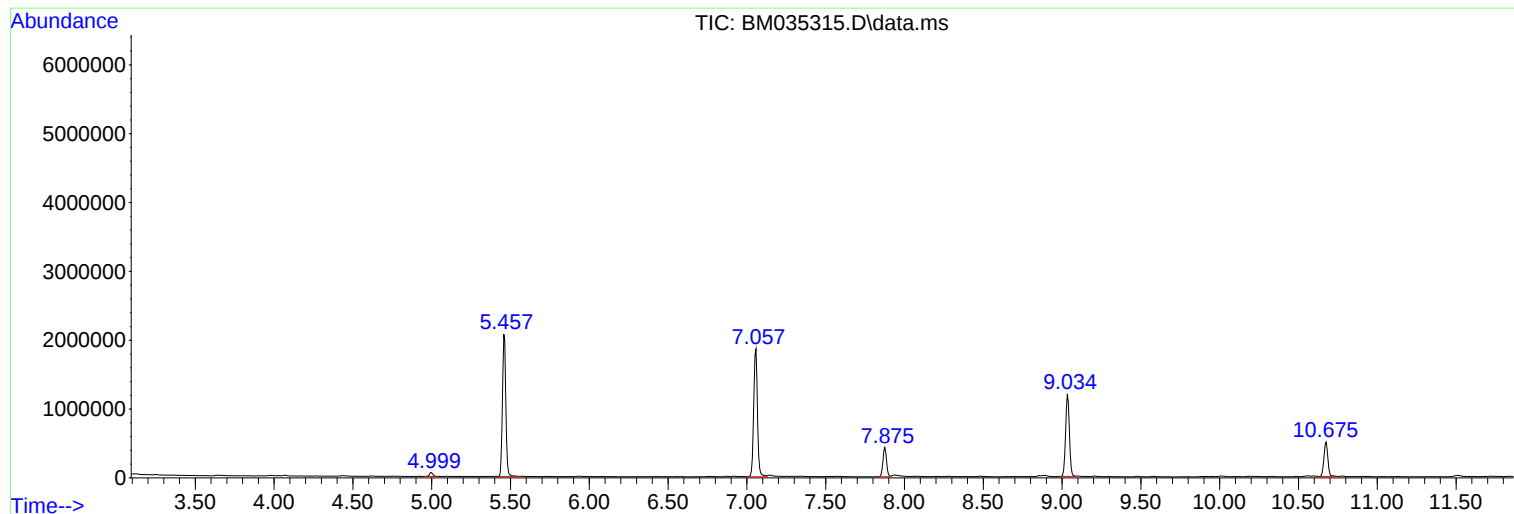

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035315.D
Acq On : 28 May 2022 18:28
Operator : CG/JU
Sample : N2928-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P026-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035315.D
Acq On : 28 May 2022 18:28
Operator : CG/JU
Sample : N2928-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P026-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------