

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035316.D
 Acq On : 28 May 2022 19:05
 Operator : CG/JU
 Sample : N2954-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P044-SS004-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	397	403	417	rBV	1297171	1921609	38.27%	6.905%
2	7.057	667	675	687	rBV	1133824	1894466	37.73%	6.808%
3	7.875	805	814	822	rBV	382681	602452	12.00%	2.165%
4	9.034	1004	1011	1026	rBV	713836	1196984	23.84%	4.301%
5	10.675	1282	1290	1302	rBV	450081	760776	15.15%	2.734%
6	13.139	1702	1709	1718	rBV	1905817	2827240	56.31%	10.160%
7	14.510	1936	1942	1948	rBV	676878	1012921	20.17%	3.640%
8	16.004	2189	2196	2204	rBV	1653375	2415961	48.12%	8.682%
9	17.163	2389	2393	2401	rBV2	90384	152496	3.04%	0.548%
10	17.257	2401	2409	2414	rVV	955126	1374500	27.37%	4.939%
11	17.310	2414	2418	2422	rVB4	41544	61275	1.22%	0.220%
12	17.657	2470	2477	2485	rBV4	17927	52598	1.05%	0.189%
13	18.045	2539	2543	2548	rBV3	41891	58588	1.17%	0.211%
14	18.104	2548	2553	2558	rBV	336607	481743	9.59%	1.731%
15	18.162	2558	2563	2578	rVV	1151933	1634344	32.55%	5.873%
16	18.462	2609	2614	2624	rBV3	95354	186484	3.71%	0.670%
17	19.292	2752	2755	2756	rBV2	71673	75958	1.51%	0.273%
18	19.321	2756	2760	2761	rVV	256030	308164	6.14%	1.107%
19	19.345	2761	2764	2776	rVV	585905	850721	16.94%	3.057%
20	19.439	2776	2780	2788	rVV	449229	642948	12.80%	2.310%
21	19.880	2850	2855	2862	rVB	4275709	5021104	100.00%	18.043%
22	20.168	2901	2904	2907	rBV3	100076	123886	2.47%	0.445%
23	20.445	2947	2951	2956	rBV	250478	319285	6.36%	1.147%
24	21.356	3103	3106	3109	rBV	197486	218981	4.36%	0.787%
25	21.439	3115	3120	3123	rBV	1373533	1827463	36.40%	6.567%
26	23.809	3517	3523	3531	rVB2	893549	1805495	35.96%	6.488%


Sum of corrected areas: 27828442

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035316.D
Acq On : 28 May 2022 19:05
Operator : CG/JU
Sample : N2954-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P044-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

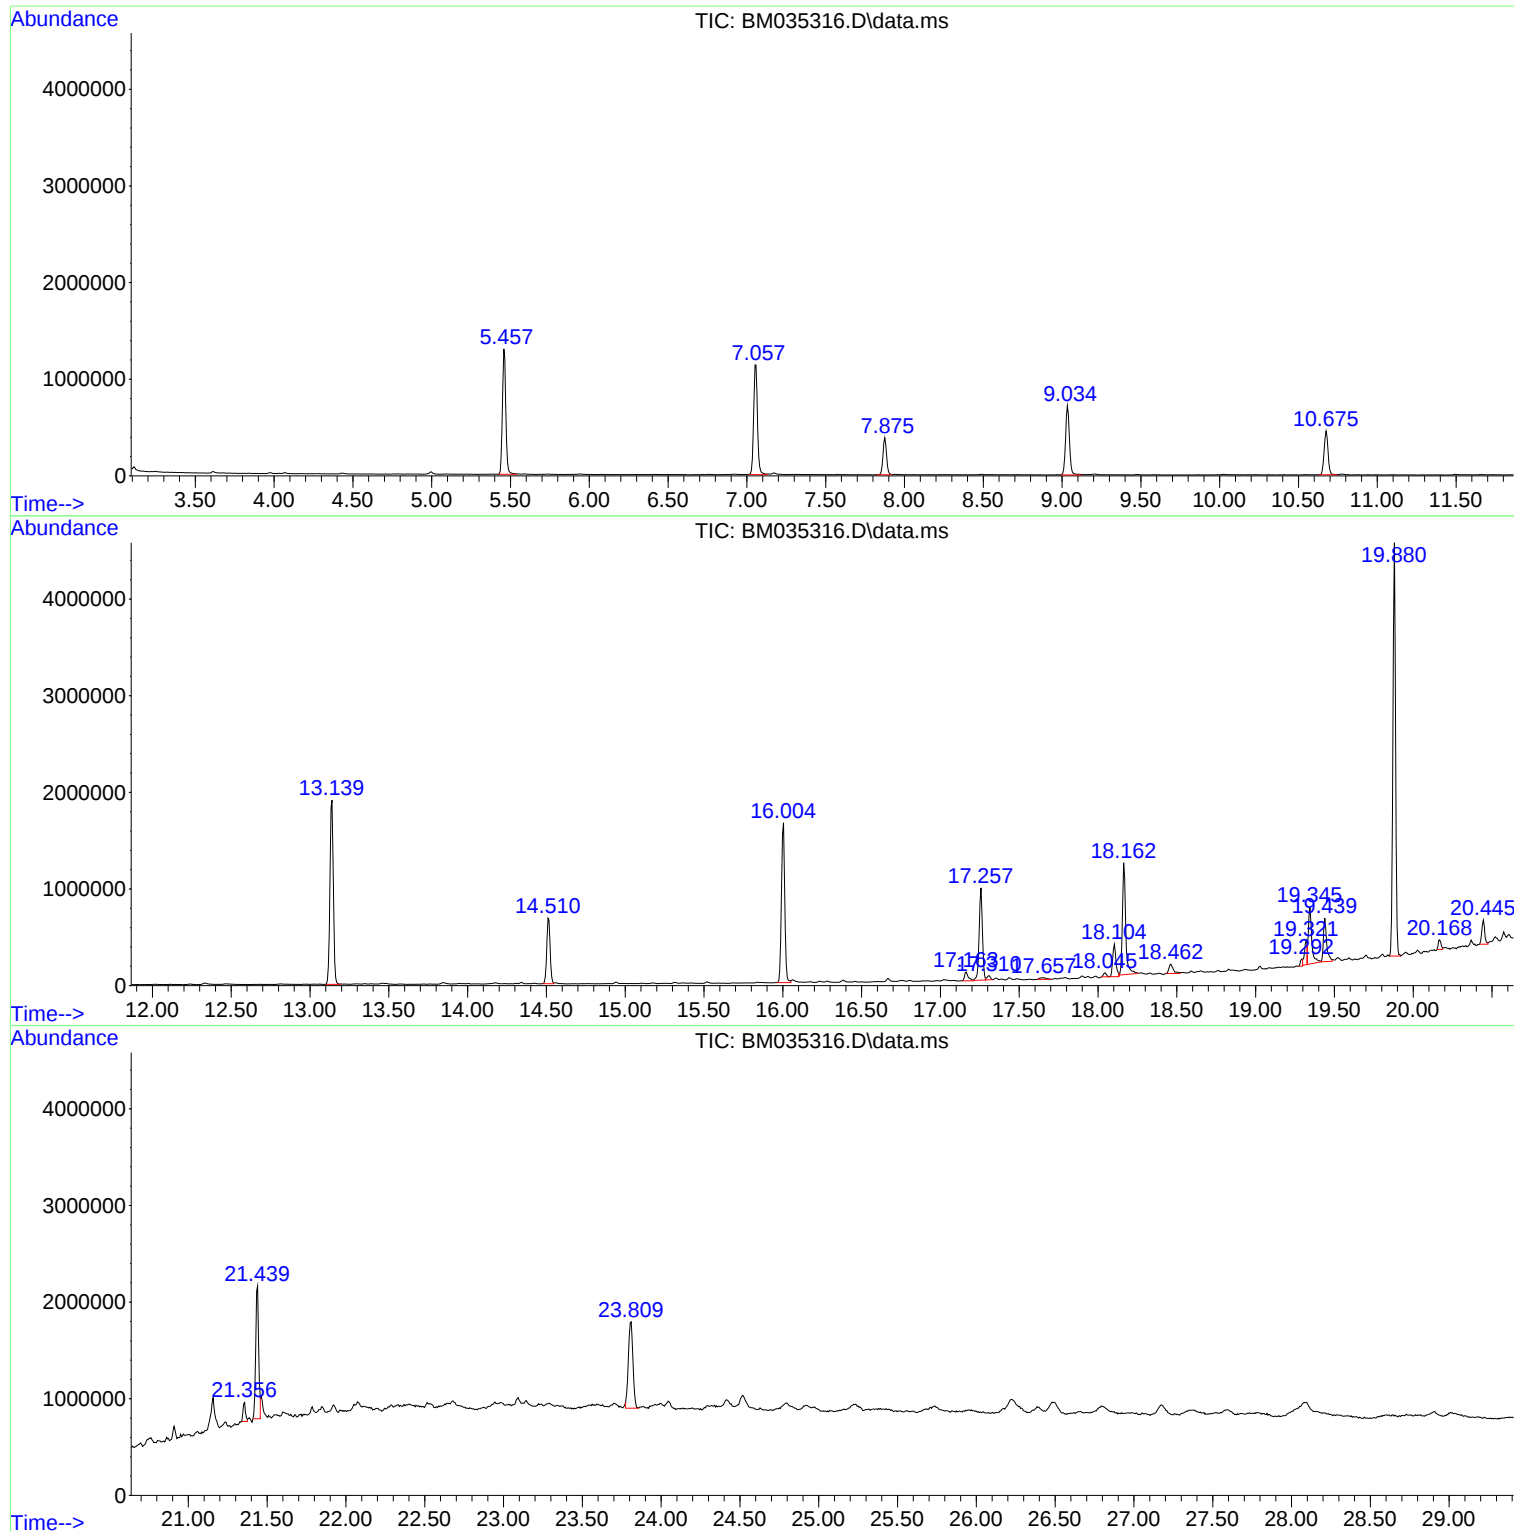

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035316.D
Acq On : 28 May 2022 19:05
Operator : CG/JU
Sample : N2954-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P044-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035316.D
Acq On : 28 May 2022 19:05
Operator : CG/JU
Sample : N2954-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P044-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------