

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035317.D
 Acq On : 28 May 2022 19:41
 Operator : CG/JU
 Sample : N2930-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P002-SS003-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	397	403	418	rBV	1403057	2070871	42.64%	8.177%
2	7.051	665	674	687	rBV	1240282	2083287	42.90%	8.226%
3	7.875	806	814	822	rBV	476046	762963	15.71%	3.013%
4	9.034	1004	1011	1024	rBV	773833	1309042	26.96%	5.169%
5	10.675	1283	1290	1299	rBV	574084	984390	20.27%	3.887%
6	13.139	1701	1709	1720	rBV	2180541	3230364	66.52%	12.755%
7	14.510	1936	1942	1949	rBV	886668	1328974	27.37%	5.247%
8	16.004	2189	2196	2203	rBV	1741813	2538983	52.28%	10.025%
9	17.257	2402	2409	2419	rBV	1149628	1626047	33.48%	6.420%
10	17.933	2521	2524	2530	rVB	45586	55400	1.14%	0.219%
11	18.162	2558	2563	2574	rBV	264679	436986	9.00%	1.725%
12	19.439	2776	2780	2789	rBV2	113179	214522	4.42%	0.847%
13	19.880	2850	2855	2863	rBV	3997831	4856070	100.00%	19.174%
14	21.433	3115	3119	3128	rBV	1366857	1909694	39.33%	7.540%
15	23.809	3517	3523	3531	rVB2	936260	1918435	39.51%	7.575%




Sum of corrected areas: 25326028

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035317.D
Acq On : 28 May 2022 19:41
Operator : CG/JU
Sample : N2930-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

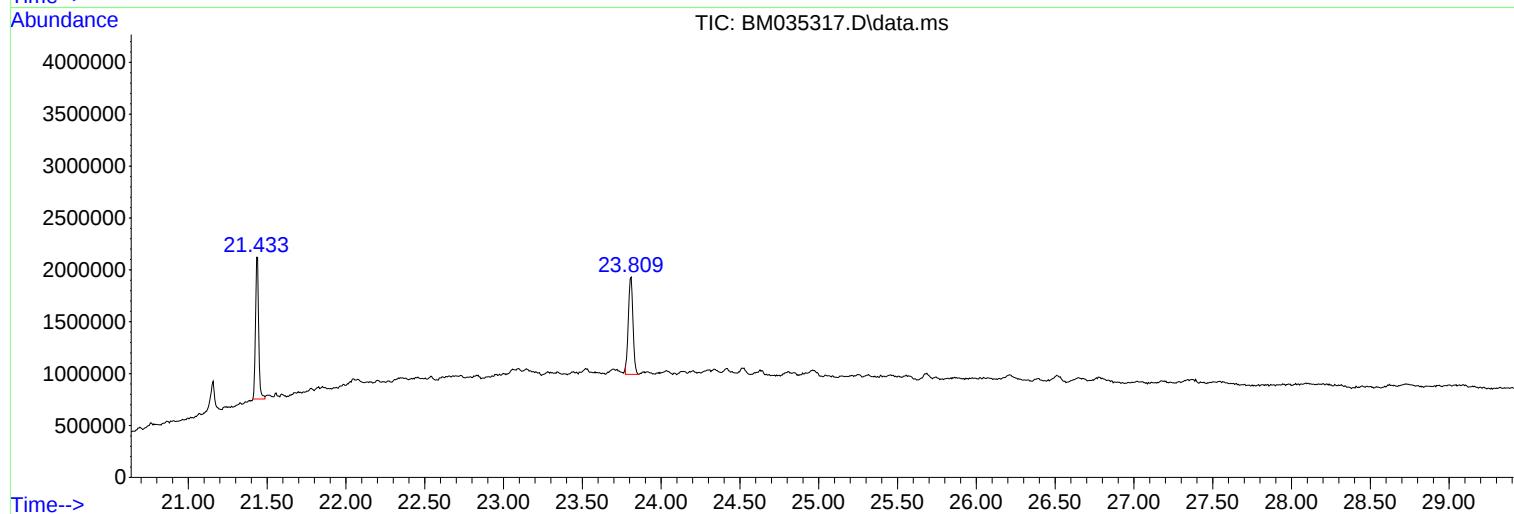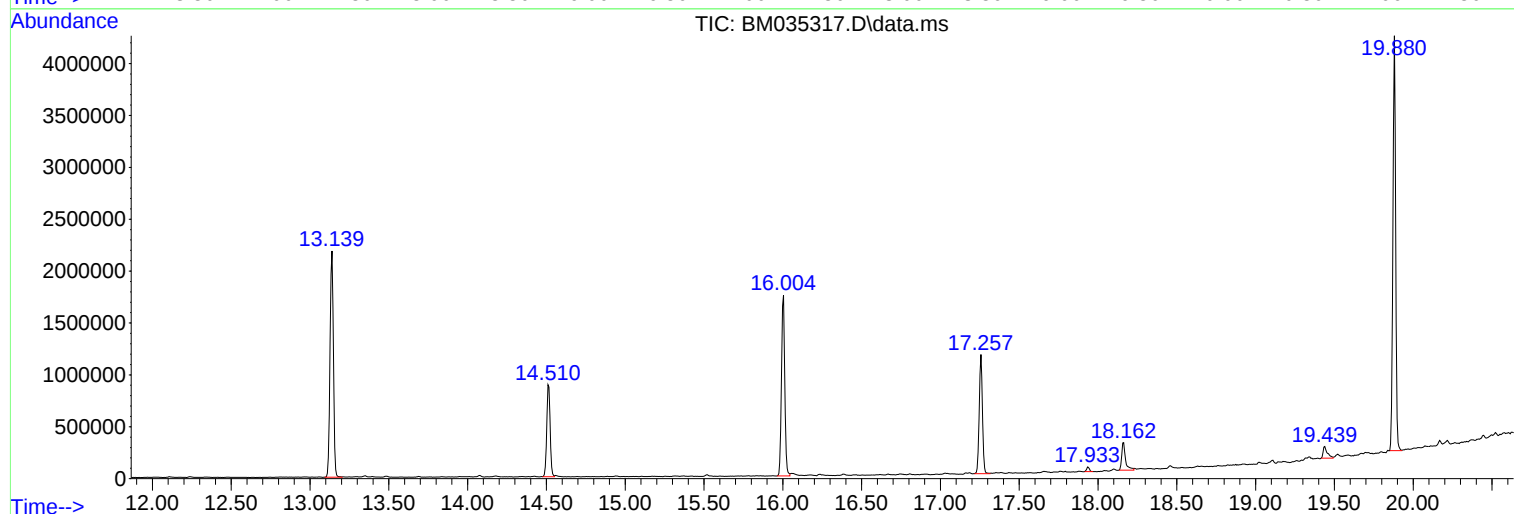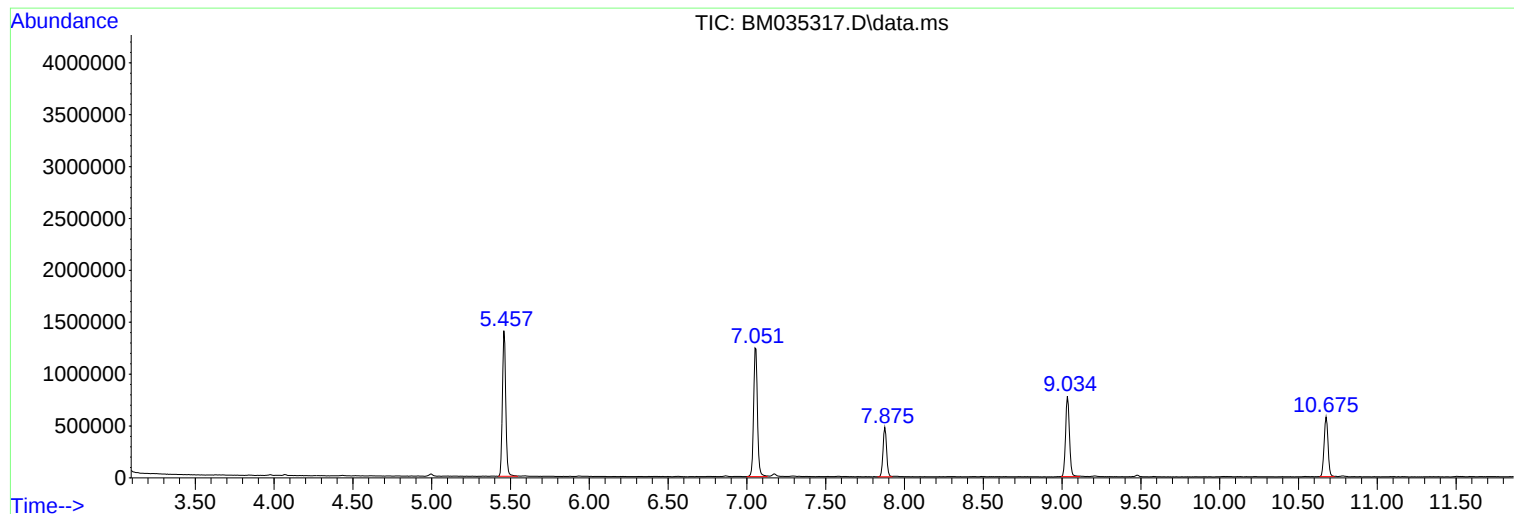

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035317.D
Acq On : 28 May 2022 19:41
Operator : CG/JU
Sample : N2930-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035317.D
Acq On : 28 May 2022 19:41
Operator : CG/JU
Sample : N2930-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P002-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------