

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035321.D
 Acq On : 28 May 2022 22:08
 Operator : CG/JU
 Sample : N2921-24 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P013-SS006-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	415	rBV	512246	800482	36.39%	4.615%
2	7.057	666	675	687	rBV	480656	826485	37.57%	4.765%
3	7.875	806	814	823	rBV	555301	888133	40.38%	5.120%
4	7.951	823	827	841	rVB6	10194	26894	1.22%	0.155%
5	9.034	1005	1011	1025	rBV	297700	523058	23.78%	3.016%
6	9.810	1135	1143	1149	rBV	34566	54081	2.46%	0.312%
7	10.675	1282	1290	1303	rBV	702476	1164776	52.95%	6.715%
8	11.498	1422	1430	1436	rBV10	8542	23379	1.06%	0.135%
9	12.474	1591	1596	1604	rBV7	8624	27265	1.24%	0.157%
10	13.139	1701	1709	1719	rBV	903709	1368926	62.24%	7.892%
11	14.516	1936	1943	1949	rBV	1053764	1536079	69.83%	8.856%
12	16.004	2190	2196	2203	rBV	606037	929311	42.25%	5.358%
13	16.233	2231	2235	2243	rBV4	15056	36335	1.65%	0.209%
14	16.386	2257	2261	2267	rVB8	19915	28965	1.32%	0.167%
15	17.257	2403	2409	2415	rBV	1240107	1757341	79.89%	10.131%
16	17.309	2415	2418	2422	rVV3	42915	57804	2.63%	0.333%
17	17.357	2422	2426	2429	rVB2	32361	42896	1.95%	0.247%
18	18.162	2558	2563	2578	rBV	216419	382710	17.40%	2.206%
19	19.439	2776	2780	2787	rBV	120224	196036	8.91%	1.130%
20	19.880	2850	2855	2861	rBV	1593581	1888972	85.88%	10.890%
21	21.156	3070	3072	3077	rVB	263755	289310	13.15%	1.668%
22	21.356	3103	3106	3110	rVB	362126	360030	16.37%	2.076%
23	21.439	3116	3120	3127	rBV	1511178	1936632	88.04%	11.165%
24	23.815	3518	3524	3532	rVB2	1065525	2199596	100.00%	12.681%




Sum of corrected areas: 17345496

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035321.D
Acq On : 28 May 2022 22:08
Operator : CG/JU
Sample : N2921-24 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS006-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

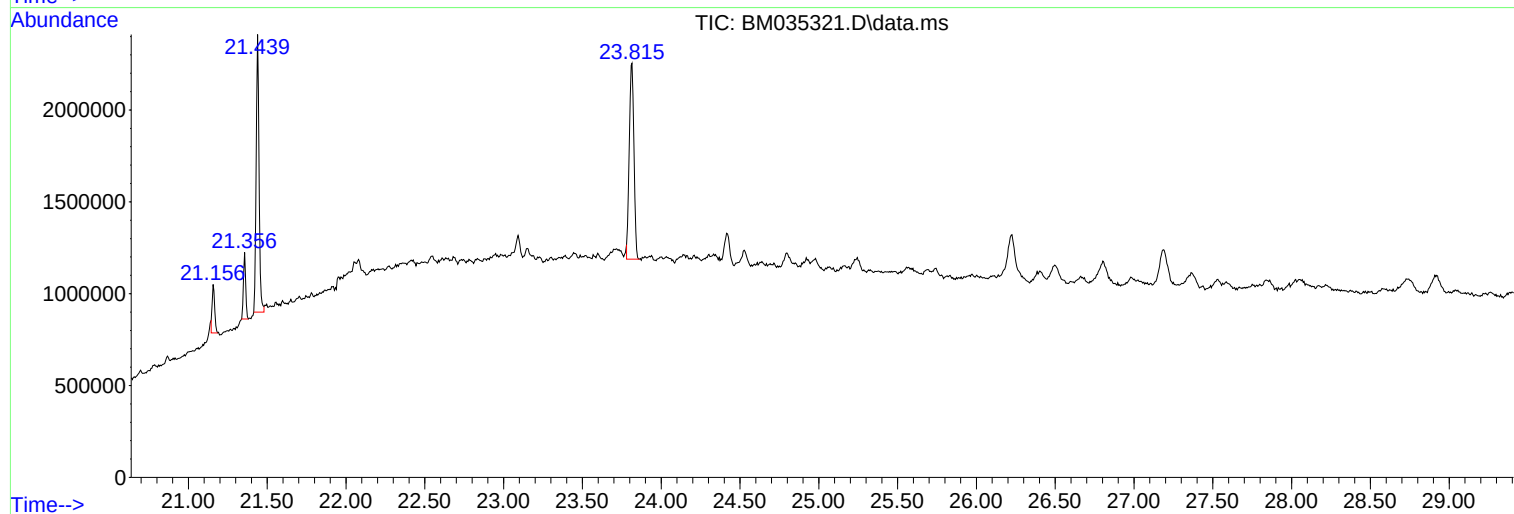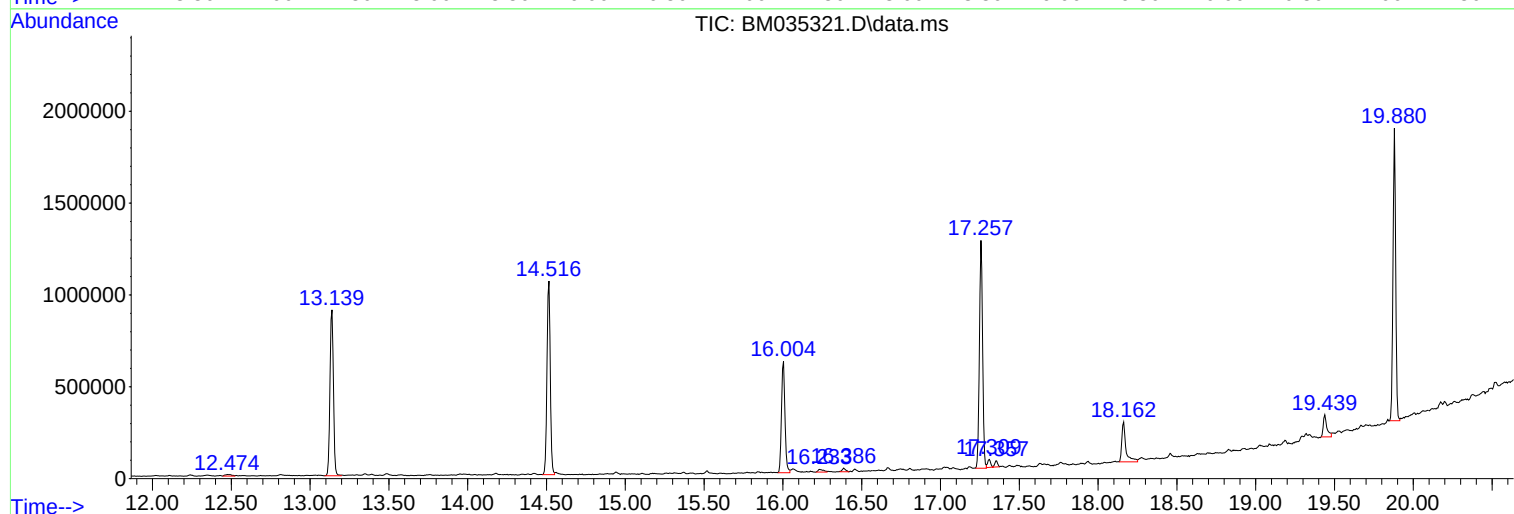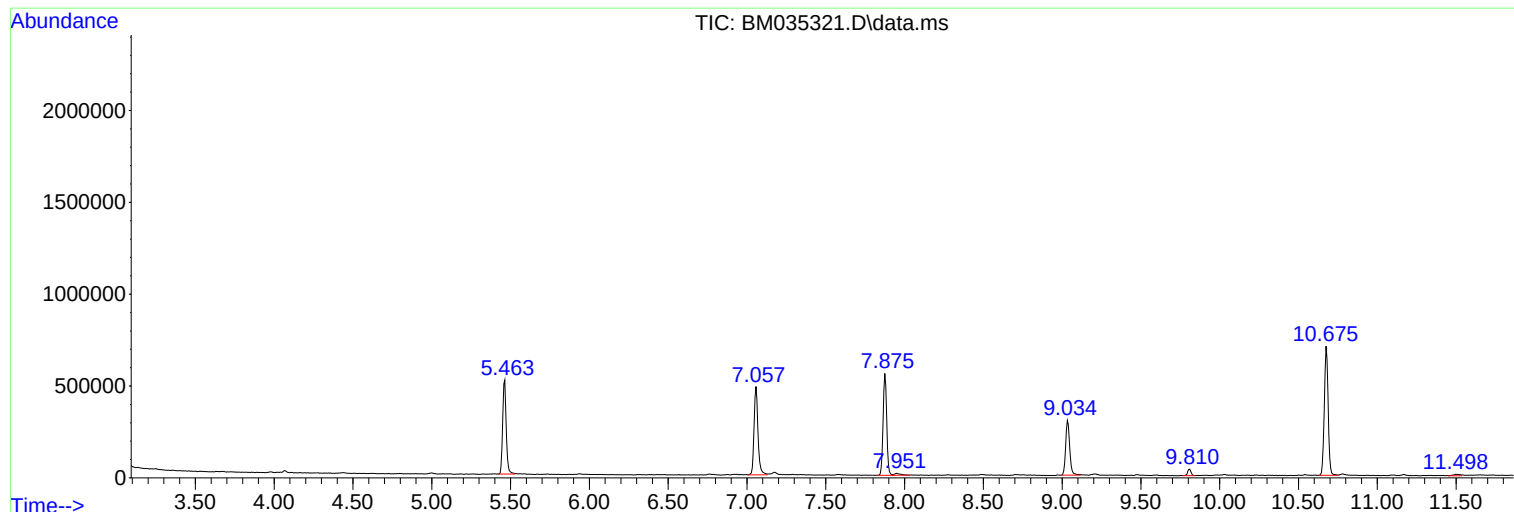

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035321.D
Acq On : 28 May 2022 22:08
Operator : CG/JU
Sample : N2921-24 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS006-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035321.D
Acq On : 28 May 2022 22:08
Operator : CG/JU
Sample : N2921-24 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P013-SS006-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------