
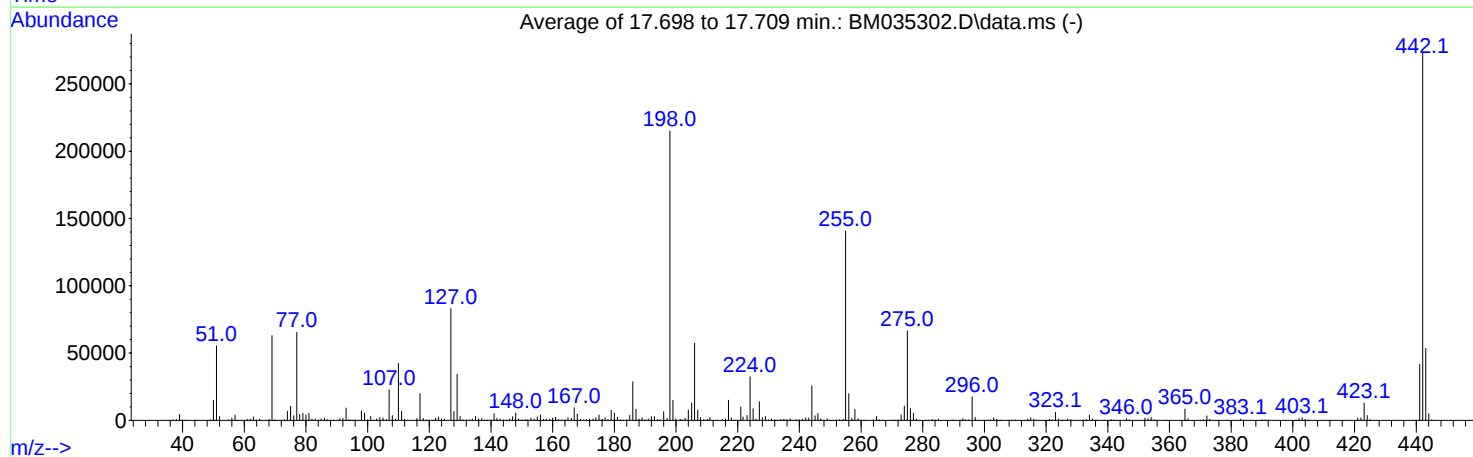


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035302.D
 Acq On : 28 May 2022 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 16:44:39 2022

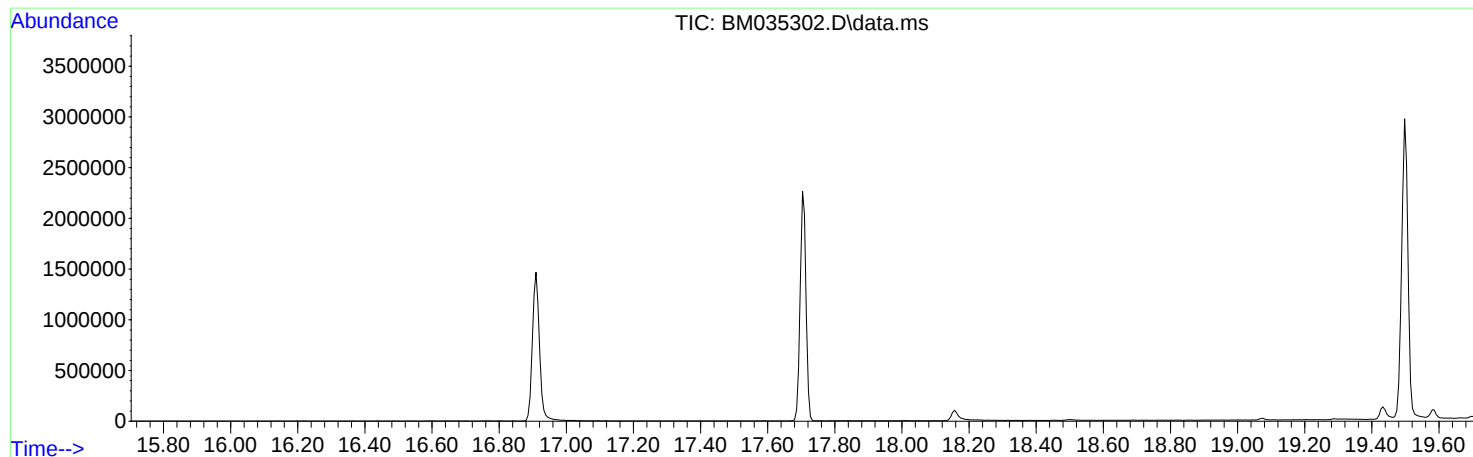




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	55443	PASS
68	69	0.00	2	1.5	949	PASS
69	198	0.00	100	29.3	63000	PASS
70	69	0.00	2	0.5	321	PASS
127	198	10	80	38.6	83005	PASS
197	198	0.00	2	0.7	1474	PASS
198	198	100	100	100.0	214912	PASS
199	198	5	9	6.9	14850	PASS
275	198	10	60	31.0	66597	PASS
365	198	1	100	4.0	8509	PASS
441	198	0.01	100	19.3	41464	PASS
442	442	50	100	100.0	273344	PASS
443	442	15	24	19.6	53576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
Data File : BM035302.D
Acq On : 28 May 2022 10:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 29 04:26:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 16:44:39 2022
Response via : Initial Calibration

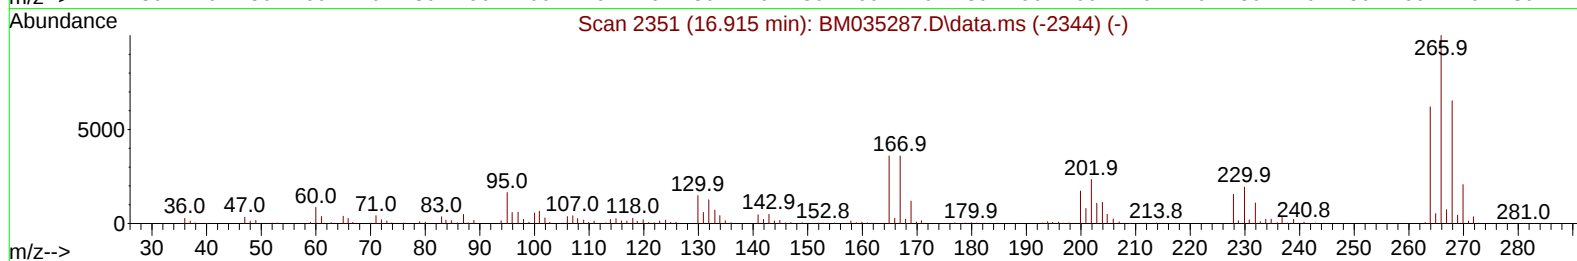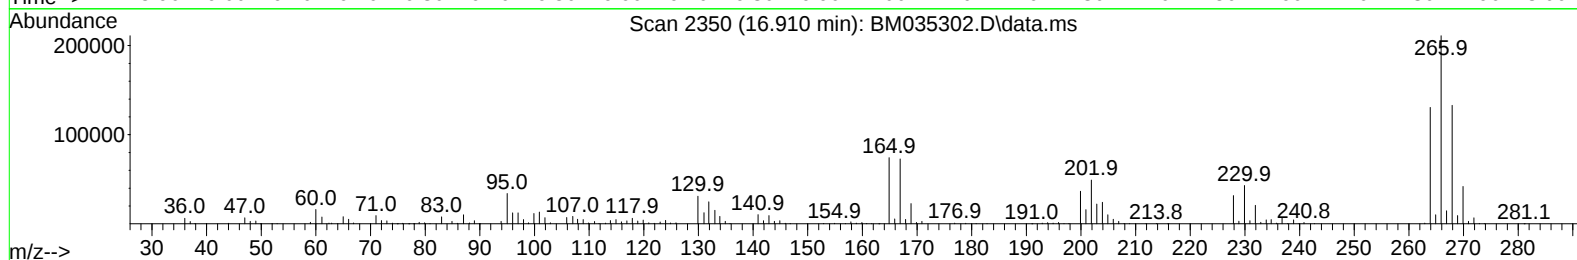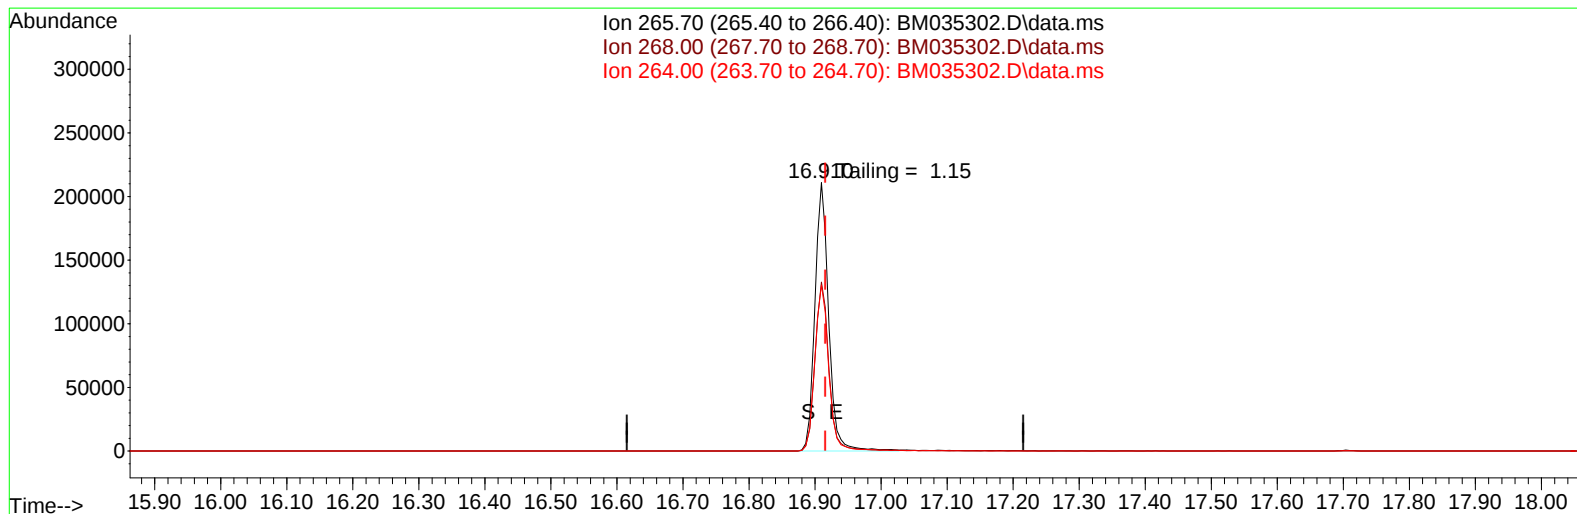

TIC: BM035302.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 0.00 ng




response 306966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.99
264.00	63.30	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052822\
 Data File : BM035302.D
 Acq On : 28 May 2022 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 29 04:26:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 16:44:39 2022
 Response via : Initial Calibration

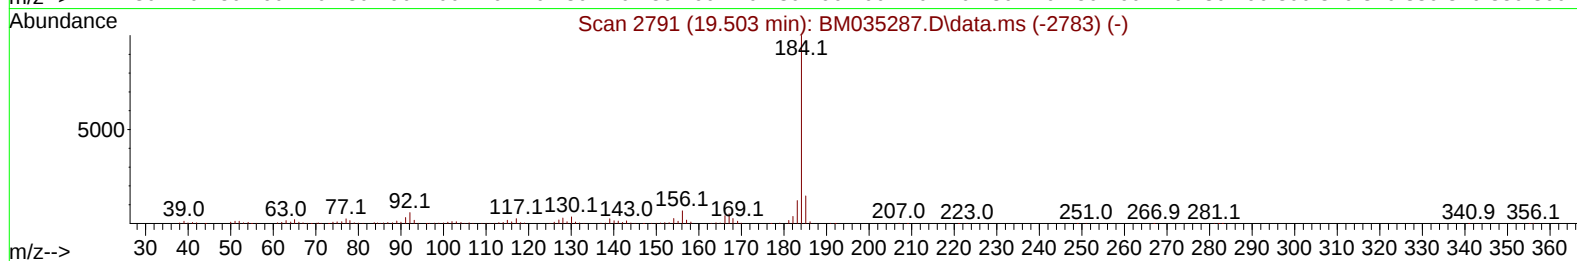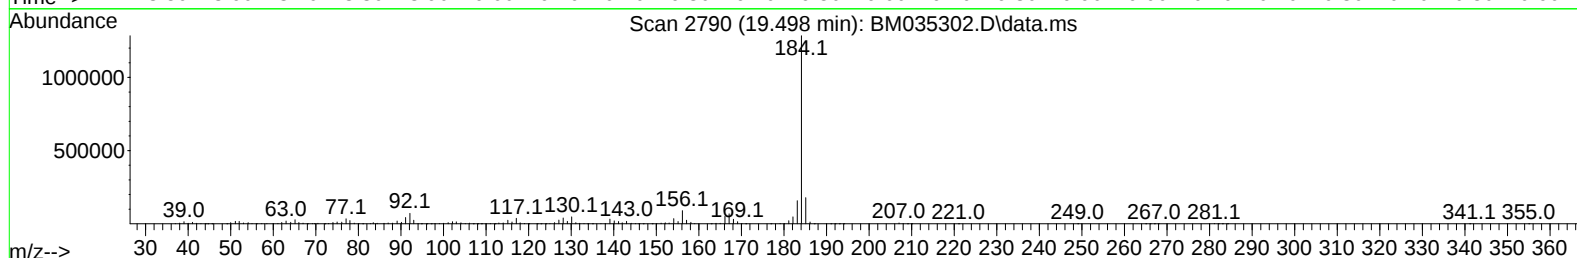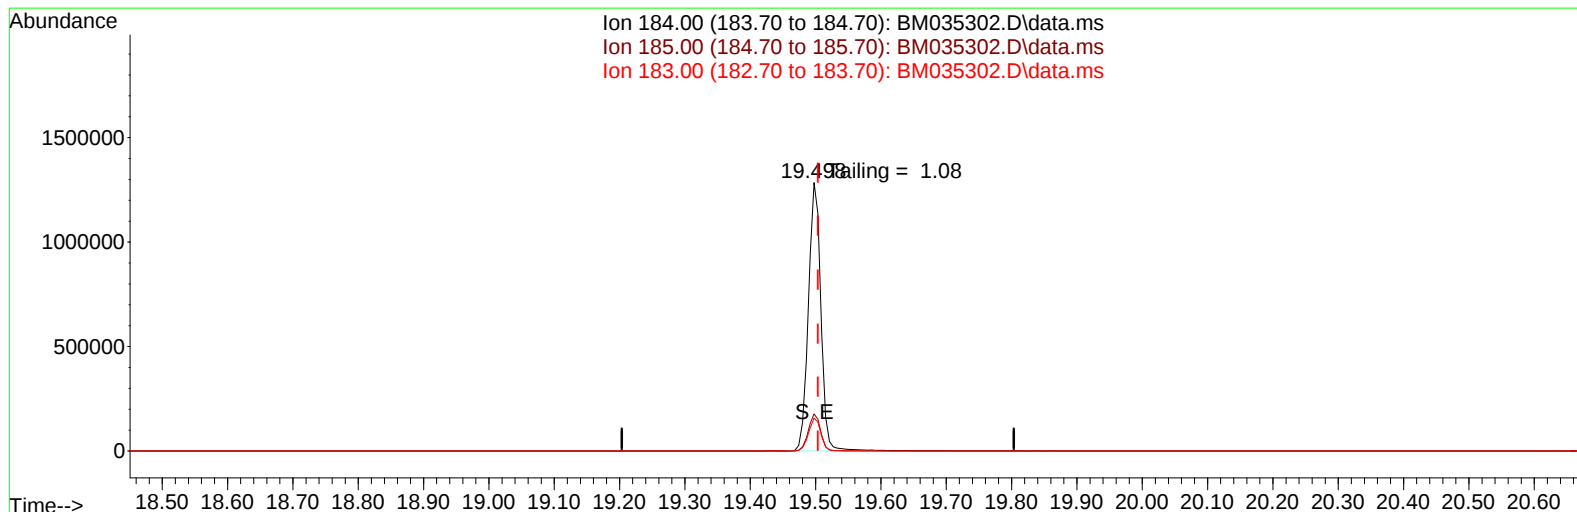

TIC: BM035302.D\data.ms

(77) Benzidine

19.498min (-0.006) 165261.52 ng

response 1717362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.87
183.00	11.90	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2022	BNA_M	<u>BM035302.D</u>
Compound Name	Response	Retention Time
DDT	919141	20.733
DDD	10643	20.292
DDE	641	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11284	930425	1.21

Instrument :
BNA_M
ClientSampleId :
DFTPP