


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052915\
Data File : BM001442.D
Acq On : 29 May 2015 09:59
Operator : TP/IZ
Sample : DFTPP51
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP51

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
Title : SVOA CALIBRATION
Last Update : Thu May 14 05:09:17 2015

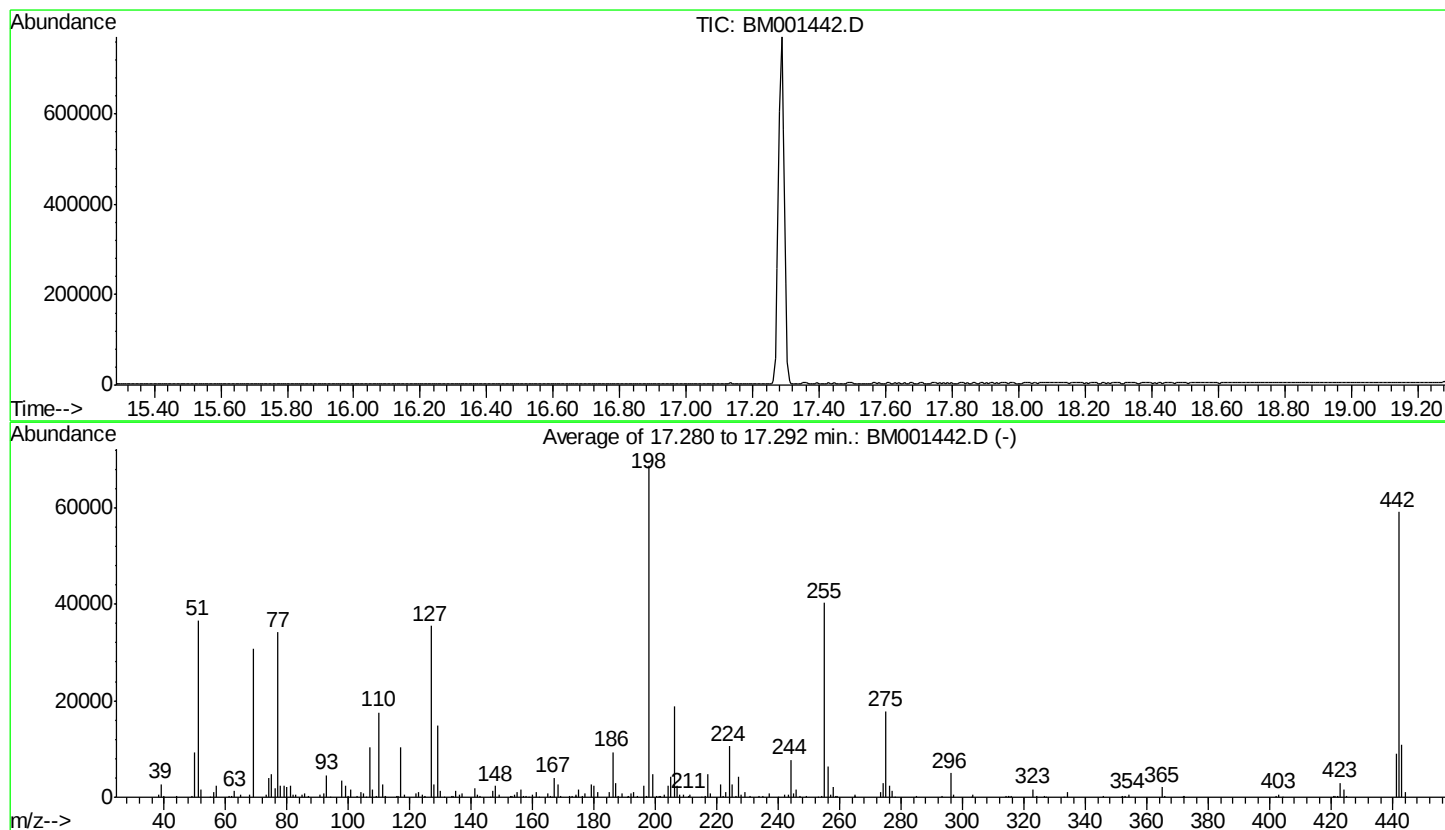

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	36560	PASS
68	69	0.00	2	1.9	581	PASS
69	198	0.00	100	44.6	30664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.6	35450	PASS
197	198	0.00	2	0.3	220	PASS
198	198	100	100	100.0	68714	PASS
199	198	5	9	7.0	4799	PASS
275	198	10	60	25.7	17667	PASS
365	198	1	100	3.0	2042	PASS
441	443	0.01	100	84.0	9083	PASS
442	198	50	100	86.0	59090	PASS
443	442	15	24	18.3	10816	PASS

m/z	Abundance
38.00	599.0
39.10	2961.0
40.10	829.0
44.00	2845.0
50.10	10261.0
51.00	39296.0
52.00	1667.0
56.00	1181.0
57.00	2697.0
61.00	503.0
62.10	395.0
63.00	1187.0
65.10	518.0
68.00	694.0
69.00	33728.0
73.10	439.0
74.00	4383.0
75.00	5323.0
76.00	1831.0
77.00	35072.0
78.00	2869.0
79.00	2548.0
80.00	2328.0
81.00	2418.0
82.00	387.0
82.90	709.0
85.00	495.0
85.90	860.0
87.10	433.0
90.90	548.0
91.90	1137.0
93.00	5593.0
98.00	3339.0
99.00	2643.0
100.10	374.0
101.00	1751.0
103.00	306.0
104.00	958.0
104.90	686.0
105.90	362.0
107.00	11365.0
107.90	1341.0
109.00	483.0
110.00	17776.0
111.00	3126.0
116.00	639.0
117.00	10321.0
118.20	612.0
122.10	375.0
123.00	857.0
124.00	522.0
127.00	35152.0
128.00	3212.0
129.00	14546.0
129.90	1365.0
133.80	502.0
134.90	1148.0
135.90	515.0
137.00	820.0
141.00	1818.0
142.10	334.0
143.00	657.0
146.10	304.0
147.00	1150.0
147.90	2401.0
148.90	509.0
153.10	466.0
153.90	457.0
155.00	1240.0
156.10	1253.0
156.90	338.0
157.90	544.0
159.80	395.0
161.10	668.0
162.00	303.0
165.00	577.0
166.00	512.0
167.00	3705.0
168.00	2677.0
169.00	370.0
171.90	569.0
172.90	362.0
173.90	553.0
175.00	1622.0
176.10	558.0
176.90	714.0
179.00	2658.0
179.90	2410.0
181.10	682.0
185.10	1138.0
186.00	9320.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

187.00	2336.0
188.00	388.0
189.00	596.0
191.20	325.0
191.90	650.0
192.90	1048.0
193.90	305.0
196.00	2374.0
198.00	63416.0
199.00	4416.0
201.70	395.0
203.00	524.0
204.00	2231.0
205.00	3694.0
206.00	17856.0
207.00	2777.0
207.90	505.0
208.90	406.0
211.10	711.0
214.80	398.0
216.00	350.0
216.90	4299.0
217.90	650.0
221.00	3158.0
223.00	1052.0
224.00	9168.0
225.00	2352.0
226.20	340.0
227.00	3847.0
228.10	593.0
229.00	1074.0
230.90	379.0
234.90	402.0
236.90	866.0
242.00	666.0
243.10	432.0
244.00	6445.0
245.10	913.0
245.90	1306.0
249.00	322.0
252.80	326.0
255.00	33168.0
256.00	5244.0
257.00	409.0
258.00	1617.0
258.80	476.0
265.10	758.0
273.00	910.0
274.10	2255.0
275.00	15121.0
276.00	2304.0
277.00	1273.0
277.90	417.0
284.90	312.0
293.10	481.0
296.00	4523.0
297.00	403.0
303.10	554.0
314.80	496.0
323.00	1258.0
324.00	304.0
326.80	306.0
333.90	618.0
351.80	314.0
353.90	315.0
364.90	1532.0
371.80	381.0
403.00	468.0
421.90	375.0
423.00	2129.0
424.00	1614.0
424.90	426.0
441.00	7155.0
442.00	42640.0
443.00	7779.0
444.00	1056.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
38.10	531.0
39.00	3072.0
39.90	852.0
44.00	2598.0
48.90	443.0
50.10	10247.0
51.10	44232.0
52.00	1901.0
56.00	1572.0
57.10	2640.0
61.00	717.0
62.00	740.0
63.00	1575.0
65.10	736.0
67.90	706.0
69.00	35344.0
73.00	706.0
74.10	4544.0
75.10	5595.0
76.10	2240.0
77.00	39600.0
78.00	2715.0
79.00	2729.0
80.10	2404.0
81.00	3044.0
82.00	533.0
83.00	435.0
85.00	790.0
85.90	799.0
86.90	593.0
90.90	518.0
92.00	728.0
93.00	4440.0
94.00	388.0
98.00	4285.0
99.10	2977.0
100.00	462.0
100.90	1753.0
102.80	372.0
104.00	1156.0
105.00	1035.0
107.00	11880.0
108.00	1877.0
110.00	19992.0
111.00	2985.0
112.00	473.0
115.80	574.0
117.00	11911.0
118.00	784.0
122.00	1142.0
123.00	1182.0
123.90	709.0
125.00	549.0
127.00	42808.0
128.00	2867.0
129.00	17232.0
130.00	1546.0
131.20	302.0
134.10	459.0
135.00	1385.0
136.00	558.0
137.00	830.0
141.00	2192.0
141.90	701.0
143.00	548.0
146.90	1531.0
148.00	2604.0
149.00	734.0
152.80	889.0
153.90	470.0
155.10	1181.0
155.90	1973.0
157.00	543.0
157.80	387.0
159.90	742.0
161.00	1218.0
164.90	1230.0
165.80	660.0
167.00	5308.0
168.10	3153.0
168.90	520.0
171.90	335.0
172.90	470.0
174.10	977.0
175.00	1678.0
176.10	637.0
177.00	1131.0
178.90	3067.0
180.00	2828.0
181.00	1372.0
184.90	1175.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

186.10	9821.0
187.00	3641.0
187.90	791.0
188.90	1027.0
190.80	394.0
192.00	1367.0
192.90	1479.0
196.00	2412.0
196.90	661.0
198.00	81472.0
199.00	5727.0
200.10	566.0
201.20	484.0
203.00	836.0
204.00	2581.0
205.10	5820.0
206.10	22024.0
207.00	3655.0
207.90	756.0
208.90	348.0
211.00	908.0
216.00	405.0
217.00	6274.0
217.90	1035.0
221.00	2297.0
221.90	1016.0
223.00	1496.0
224.00	13070.0
225.00	3371.0
226.00	413.0
226.90	5300.0
227.90	757.0
228.90	1066.0
230.90	520.0
233.90	315.0
235.00	420.0
237.00	1079.0
240.10	303.0
242.10	811.0
243.00	1064.0
244.00	9223.0
245.00	956.0
246.00	2263.0
246.90	409.0
249.10	315.0
254.00	515.0
255.00	49552.0
256.00	8363.0
257.00	728.0
258.00	2867.0
259.00	770.0
265.00	1125.0
273.00	1290.0
274.10	3407.0
275.00	21416.0
276.00	2415.0
277.00	1717.0
285.00	304.0
293.10	366.0
296.10	5893.0
296.90	658.0
303.20	789.0
314.10	372.0
315.00	555.0
316.00	336.0
323.00	2073.0
324.00	423.0
327.00	399.0
332.80	364.0
334.00	1383.0
352.00	379.0
352.90	666.0
353.90	599.0
365.00	2451.0
366.00	313.0
372.00	534.0
402.10	565.0
402.90	489.0
404.00	374.0
420.80	618.0
422.10	454.0
423.00	3584.0
423.90	1731.0
425.00	428.0
441.00	10563.0
442.00	68360.0
443.00	12607.0
443.90	1354.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
38.00	377.0
39.10	1956.0
40.00	545.0
44.00	2465.0
50.00	7396.0
51.10	26152.0
52.00	1283.0
54.90	404.0
55.90	750.0
57.10	1456.0
63.00	1158.0
64.90	479.0
68.10	343.0
69.00	22920.0
73.10	525.0
74.10	2803.0
75.00	3471.0
76.00	1426.0
77.10	27712.0
78.00	1814.0
79.00	1873.0
80.00	1696.0
81.00	1938.0
82.10	304.0
82.90	315.0
84.90	450.0
85.90	557.0
90.80	373.0
91.90	683.0
93.00	3627.0
98.00	2704.0
98.90	1975.0
100.90	1005.0
104.00	796.0
104.90	902.0
107.00	8037.0
107.90	1370.0
109.10	505.0
110.00	14929.0
111.10	2124.0
112.20	395.0
116.20	468.0
117.00	8489.0
118.10	416.0
122.00	569.0
123.00	1040.0
124.10	390.0
124.90	440.0
127.00	28392.0
127.90	1680.0
129.00	12945.0
130.10	960.0
134.10	500.0
135.00	1263.0
136.10	309.0
137.00	494.0
141.00	1866.0
142.00	610.0
147.00	1221.0
148.00	2000.0
149.00	547.0
153.00	462.0
154.00	493.0
155.10	451.0
156.00	1212.0
158.80	370.0
160.00	599.0
160.90	938.0
165.10	507.0
166.10	381.0
167.00	3115.0
168.00	1811.0
174.00	681.0
175.00	1226.0
177.10	683.0
179.00	2497.0
180.00	1980.0
181.00	794.0
184.90	1092.0
186.00	8986.0
187.00	2465.0
189.00	467.0
191.00	528.0
191.90	523.0
193.00	1011.0
193.90	309.0
196.00	2466.0
197.10	319.0
198.00	61256.0
198.90	4254.0
200.20	443.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

201.50	472.0
203.00	426.0
204.00	2074.0
205.00	3549.0
206.00	17024.0
207.00	2311.0
208.00	736.0
208.90	549.0
210.80	634.0
216.00	349.0
217.00	4092.0
218.00	822.0
221.00	2703.0
223.10	783.0
224.00	9265.0
225.00	2077.0
226.00	328.0
227.10	3811.0
228.00	653.0
228.90	705.0
233.80	479.0
237.00	416.0
242.10	378.0
243.10	517.0
244.10	7500.0
245.10	782.0
246.00	1223.0
246.70	321.0
248.90	548.0
254.10	345.0
255.00	37952.0
256.00	5157.0
257.10	414.0
257.90	2081.0
264.80	883.0
273.10	1353.0
274.00	3155.0
275.00	16464.0
276.00	2161.0
276.90	1068.0
285.10	343.0
296.10	4384.0
296.90	753.0
302.80	402.0
314.00	399.0
314.90	646.0
315.90	336.0
323.00	1556.0
324.10	304.0
326.70	316.0
333.90	831.0
345.90	535.0
352.00	474.0
352.90	406.0
354.00	692.0
365.00	2143.0
365.90	530.0
372.20	611.0
402.00	391.0
403.00	693.0
421.00	751.0
422.00	432.0
423.00	3186.0
423.90	1438.0
425.00	307.0
441.00	9533.0
442.00	66272.0
443.00	12063.0
444.00	978.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

Scan 2476 (17.251 min): BM001442.D
DFTPP51

m/z	Abundance
39.90	501.0
44.00	2362.0
207.00	466.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51