

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052920\
 Data File : BM026175.D
 Acq On : 29 May 2020 13:30
 Operator : MA/SJ
 Sample : L2781-01RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC1RX

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.675	131	134	138	rVB	15657	21349	0.98%	0.153%
2	4.652	296	300	308	rBV	24933	41708	1.92%	0.298%
3	4.899	339	342	344	rBV3	3886	4834	0.22%	0.035%
4	5.093	373	375	377	rBV3	2306	2514	0.12%	0.018%
5	5.504	439	445	450	rBV7	5103	9073	0.42%	0.065%
6	5.540	450	451	455	rVB4	3850	3400	0.16%	0.024%
7	5.675	471	474	476	rBV4	1975	2371	0.11%	0.017%
8	5.716	479	481	485	rVB4	2964	3086	0.14%	0.022%
9	5.816	496	498	499	rBV2	3113	2266	0.10%	0.016%
10	6.640	632	638	640	rBV	36242	59806	2.75%	0.427%
11	6.675	640	644	655	rVB2	71199	156690	7.21%	1.119%
12	6.828	664	670	682	rVV	61398	105975	4.88%	0.757%
13	7.016	696	702	713	rVV	69406	119739	5.51%	0.855%
14	7.122	716	720	726	rVB7	4561	5494	0.25%	0.039%
15	7.310	750	752	755	rBV3	2265	2885	0.13%	0.021%
16	7.475	774	780	791	rVV	531370	841160	38.70%	6.009%
17	7.563	793	795	803	rVB8	3989	6653	0.31%	0.048%
18	7.728	819	823	824	rBV4	2075	2209	0.10%	0.016%
19	7.928	855	857	860	rBV3	2860	4185	0.19%	0.030%
20	8.063	877	880	883	rBV4	2897	3965	0.18%	0.028%
21	8.193	897	902	909	rBV	77093	129155	5.94%	0.923%
22	8.298	914	920	929	rVV	64728	114878	5.29%	0.821%
23	8.363	929	931	935	rVV5	1996	2502	0.12%	0.018%
24	8.416	935	940	948	rVV4	6315	13695	0.63%	0.098%
25	8.475	948	950	952	rVB3	2415	2460	0.11%	0.018%
26	8.493	952	953	957	rBV3	1849	2511	0.12%	0.018%
27	8.622	969	975	985	rBV	71934	123968	5.70%	0.886%
28	8.716	989	991	993	rVV3	3153	2972	0.14%	0.021%
29	8.740	993	995	998	rVV4	5333	6011	0.28%	0.043%
30	8.969	1031	1034	1037	rVB4	2299	2959	0.14%	0.021%
31	9.081	1050	1053	1054	rBV2	2178	2239	0.10%	0.016%
32	9.234	1076	1079	1082	rBV5	1918	2951	0.14%	0.021%
33	9.340	1091	1097	1104	rBV	46756	78646	3.62%	0.562%
34	9.528	1126	1129	1130	rBV3	4018	3765	0.17%	0.027%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052920\
 Data File : BM026175.D
 Acq On : 29 May 2020 13:30
 Operator : MA/SJ
 Sample : L2781-01RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC1RX

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	9.540	1130	1131	1135	rVV3	3399	4529	0.21%	0.032%
36	9.575	1135	1137	1139	rVB3	2665	2243	0.10%	0.016%
37	9.698	1154	1158	1165	rBV3	13507	25111	1.16%	0.179%
38	9.875	1181	1188	1200	rBV2	68793	126845	5.84%	0.906%
39	10.239	1242	1250	1261	rVB	709574	1188229	54.67%	8.489%
40	10.387	1269	1275	1285	rBV	64026	130294	6.00%	0.931%
41	10.804	1339	1346	1352	rBV7	6069	12545	0.58%	0.090%
42	11.063	1384	1390	1392	rBV5	4691	8477	0.39%	0.061%
43	11.134	1399	1402	1407	rVB6	1768	2805	0.13%	0.020%
44	11.463	1455	1458	1464	rVB4	1566	2544	0.12%	0.018%
45	11.634	1481	1487	1492	rBV2	5372	11743	0.54%	0.084%
46	11.786	1510	1513	1515	rBV4	2736	2963	0.14%	0.021%
47	11.833	1519	1521	1525	rBV5	2022	2236	0.10%	0.016%
48	12.469	1625	1629	1633	rBV5	2788	4145	0.19%	0.030%
49	12.739	1671	1675	1678	rBV5	2956	4906	0.23%	0.035%
50	13.045	1721	1727	1735	rBV6	8689	18591	0.86%	0.133%
51	13.286	1766	1768	1771	rBV3	2154	2268	0.10%	0.016%
52	13.428	1789	1792	1794	rBV3	1817	2482	0.11%	0.018%
53	13.545	1806	1812	1816	rBV	168652	231090	10.63%	1.651%
54	13.592	1816	1820	1826	rVB	108006	152094	7.00%	1.087%
55	13.710	1837	1840	1845	rVB5	2208	3971	0.18%	0.028%
56	13.810	1848	1857	1863	rBV	132166	200614	9.23%	1.433%
57	13.922	1874	1876	1880	rVB4	3254	3761	0.17%	0.027%
58	14.122	1903	1910	1918	rBV	1027420	1448859	66.66%	10.351%
59	14.210	1922	1925	1926	rBV3	2683	2775	0.13%	0.020%
60	14.357	1945	1950	1959	rBV	30029	69327	3.19%	0.495%
61	14.516	1976	1977	1982	rVB4	2790	2749	0.13%	0.020%
62	14.580	1984	1988	1997	rBV2	43456	67040	3.08%	0.479%
63	14.716	2010	2011	2015	rBV4	2302	2245	0.10%	0.016%
64	14.769	2017	2020	2022	rVV3	4417	4524	0.21%	0.032%
65	14.922	2044	2046	2048	rBV3	3279	2975	0.14%	0.021%
66	15.121	2073	2080	2090	rBV	216387	309081	14.22%	2.208%
67	15.210	2093	2095	2098	rBV4	3106	3349	0.15%	0.024%
68	15.257	2098	2103	2109	rBV3	40122	63673	2.93%	0.455%
69	15.363	2120	2121	2124	rVB3	4296	3350	0.15%	0.024%
70	15.416	2127	2130	2131	rBV3	2981	2410	0.11%	0.017%
71	15.510	2144	2146	2152	rVB7	3368	5118	0.24%	0.037%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052920\
 Data File : BM026175.D
 Acq On : 29 May 2020 13:30
 Operator : MA/SJ
 Sample : L2781-01RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC1RX

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.716	2178	2181	2184	rBV4	2641	3475	0.16%	0.025%
73	15.904	2212	2213	2216	rBV3	3340	2543	0.12%	0.018%
74	16.533	2315	2320	2326	rBV	85879	133138	6.13%	0.951%
75	16.663	2337	2342	2348	rBV6	7826	14905	0.69%	0.106%
76	16.733	2352	2354	2357	rVB4	3612	3061	0.14%	0.022%
77	16.868	2371	2377	2388	rVV	1221468	1739493	80.04%	12.427%
78	16.968	2388	2394	2407	rVV2	205874	315625	14.52%	2.255%
79	17.263	2443	2444	2445	rBV	4364	2439	0.11%	0.017%
80	17.298	2446	2450	2454	rVB	17057	25449	1.17%	0.182%
81	17.374	2462	2463	2464	rBV	5588	3493	0.16%	0.025%
82	17.663	2507	2512	2515	rBV4	7820	13751	0.63%	0.098%
83	17.798	2532	2535	2539	rBV6	10093	16150	0.74%	0.115%
84	17.845	2540	2543	2545	rVB2	12121	13718	0.63%	0.098%
85	18.586	2666	2669	2673	rVV	15414	22118	1.02%	0.158%
86	18.633	2675	2677	2681	rVB4	14158	14954	0.69%	0.107%
87	18.827	2703	2710	2721	rBV5	39099	118108	5.43%	0.844%
88	19.268	2780	2785	2793	rBV	287407	401938	18.49%	2.871%
89	19.362	2799	2801	2804	rVB4	13236	14073	0.65%	0.101%
90	21.074	3086	3092	3101	rBV	1675272	2173363	100.00%	15.526%
91	21.680	3193	3195	3199	rBV3	77181	82900	3.81%	0.592%
92	22.121	3267	3270	3275	rVB2	115613	142225	6.54%	1.016%
93	22.592	3348	3350	3355	rVB	137462	166590	7.67%	1.190%
94	23.050	3424	3428	3435	rVB	240161	396578	18.25%	2.833%
95	23.186	3445	3451	3459	rVB2	1252944	2157672	99.28%	15.414%


Sum of corrected areas: 13997794

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052920\
Data File : BM026175.D
Acq On : 29 May 2020 13:30
Operator : MA/SJ
Sample : L2781-01RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC1RX

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

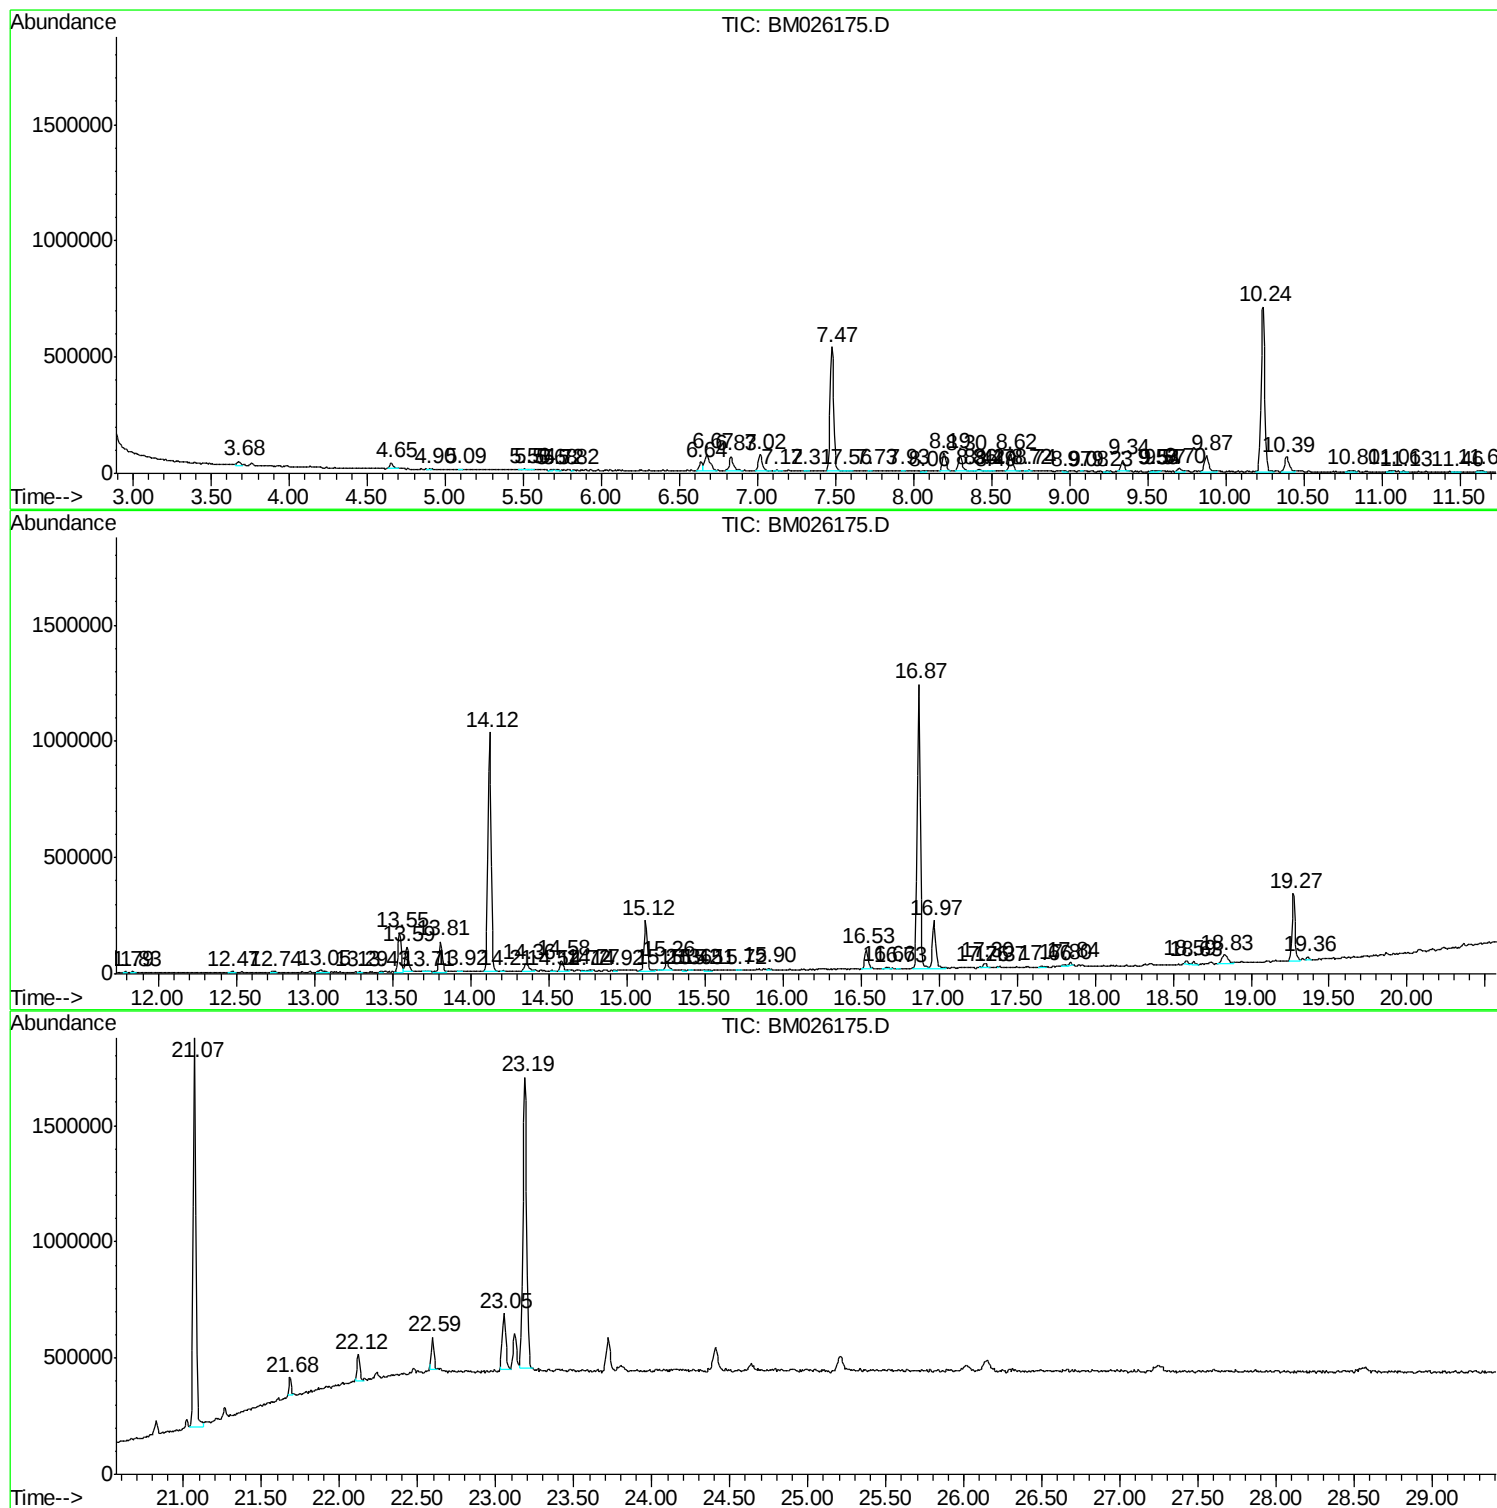

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052920\
Data File : BM026175.D
Acq On : 29 May 2020 13:30
Operator : MA/SJ
Sample : L2781-01RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC1RX

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052920\
Data File : BM026175.D
Acq On : 29 May 2020 13:30
Operator : MA/SJ
Sample : L2781-01RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC1RX

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc