

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053015\
 Data File : BM001475.D
 Acq On : 30 May 2015 15:10
 Operator : TP/IZ
 Sample : G2411-04RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BCRB7RE

Quant Time: May 31 02:20:01 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 31 02:16:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	174061	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	712174	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.06	164	404002	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.82	188	805989	20.00	ng/ul	0.00
75) Chrysene-d12	21.02	240	773495	20.00	ng/ul	0.00
83) Perylene-d12	23.11	264	705871	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.80	96	9388	2.69	ng/uL	0.00
5) Phenol-d5	6.58	99	205814	15.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	130716	16.28	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	175970	16.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.11	113	147018	13.53	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	80781	17.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.25	143	94979	17.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	173694	16.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.31	131	97421	7.83	ng/ul	0.00
43) Dimethylphthalate-d6	13.48	166	478330	16.88	ng/ul	0.00
46) Acenaphthylene-d8	13.75	160	662158	17.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	71695	12.41	ng/ul	0.00
57) Fluorene-d10	15.06	176	454277	16.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.20	200	46937	9.46	ng/ul	0.00
70) Anthracene-d10	16.91	188	620700	16.71	ng/ul	0.00
76) Pyrene-d10	19.22	212	652378	19.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	22.98	264	543484	17.41	ng/ul	0.00

Target Compounds


						Qvalue
14) Acetophenone	8.20	105	53470	3.01	ng/ul	99
44) Dimethylphthalate	13.53	163	321675	10.06	ng/ul	99
69) Phenanthrene	16.86	178	340336	7.58	ng/ul	99
71) Anthracene	16.94	178	94255	2.04	ng/ul	98
73) Di-n-butylphthalate	17.80	149	72044	1.45	ng/ul#	96
74) Fluoranthene	18.89	202	663862	12.21	ng/ul	98
77) Pyrene	19.25	202	555118	12.01	ng/ul	99
80) Benzo(a)anthracene	21.01	228	304219	6.73	ng/ul	97
81) Bis(2-ethylhexyl)phthalate	20.96	149	38830	1.35	ng/ul	97
82) Chrysene	21.06	228	290449	6.83	ng/ul	97
85) Benzo(b)fluoranthene	22.50	252	355412	8.22	ng/ul	97
86) Benzo(k)fluoranthene	22.50	252	102993	2.49	ng/ul	96
88) Benzo(a)pyrene	23.02	252	253258	6.25	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.16	276	167178	3.92	ng/ul	98
90) Dibenzo(a,h)anthracene	25.17	278	47870	1.34	ng/ul#	85
91) Benzo(g,h,i)perylene	25.79	276	155615	4.42	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053015\
Data File : BM001475.D
Acq On : 30 May 2015 15:10
Operator : TP/IZ
Sample : G2411-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BCRB7RE

Quant Time: May 31 02:20:01 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 31 02:16:14 2015
Response via : Initial Calibration

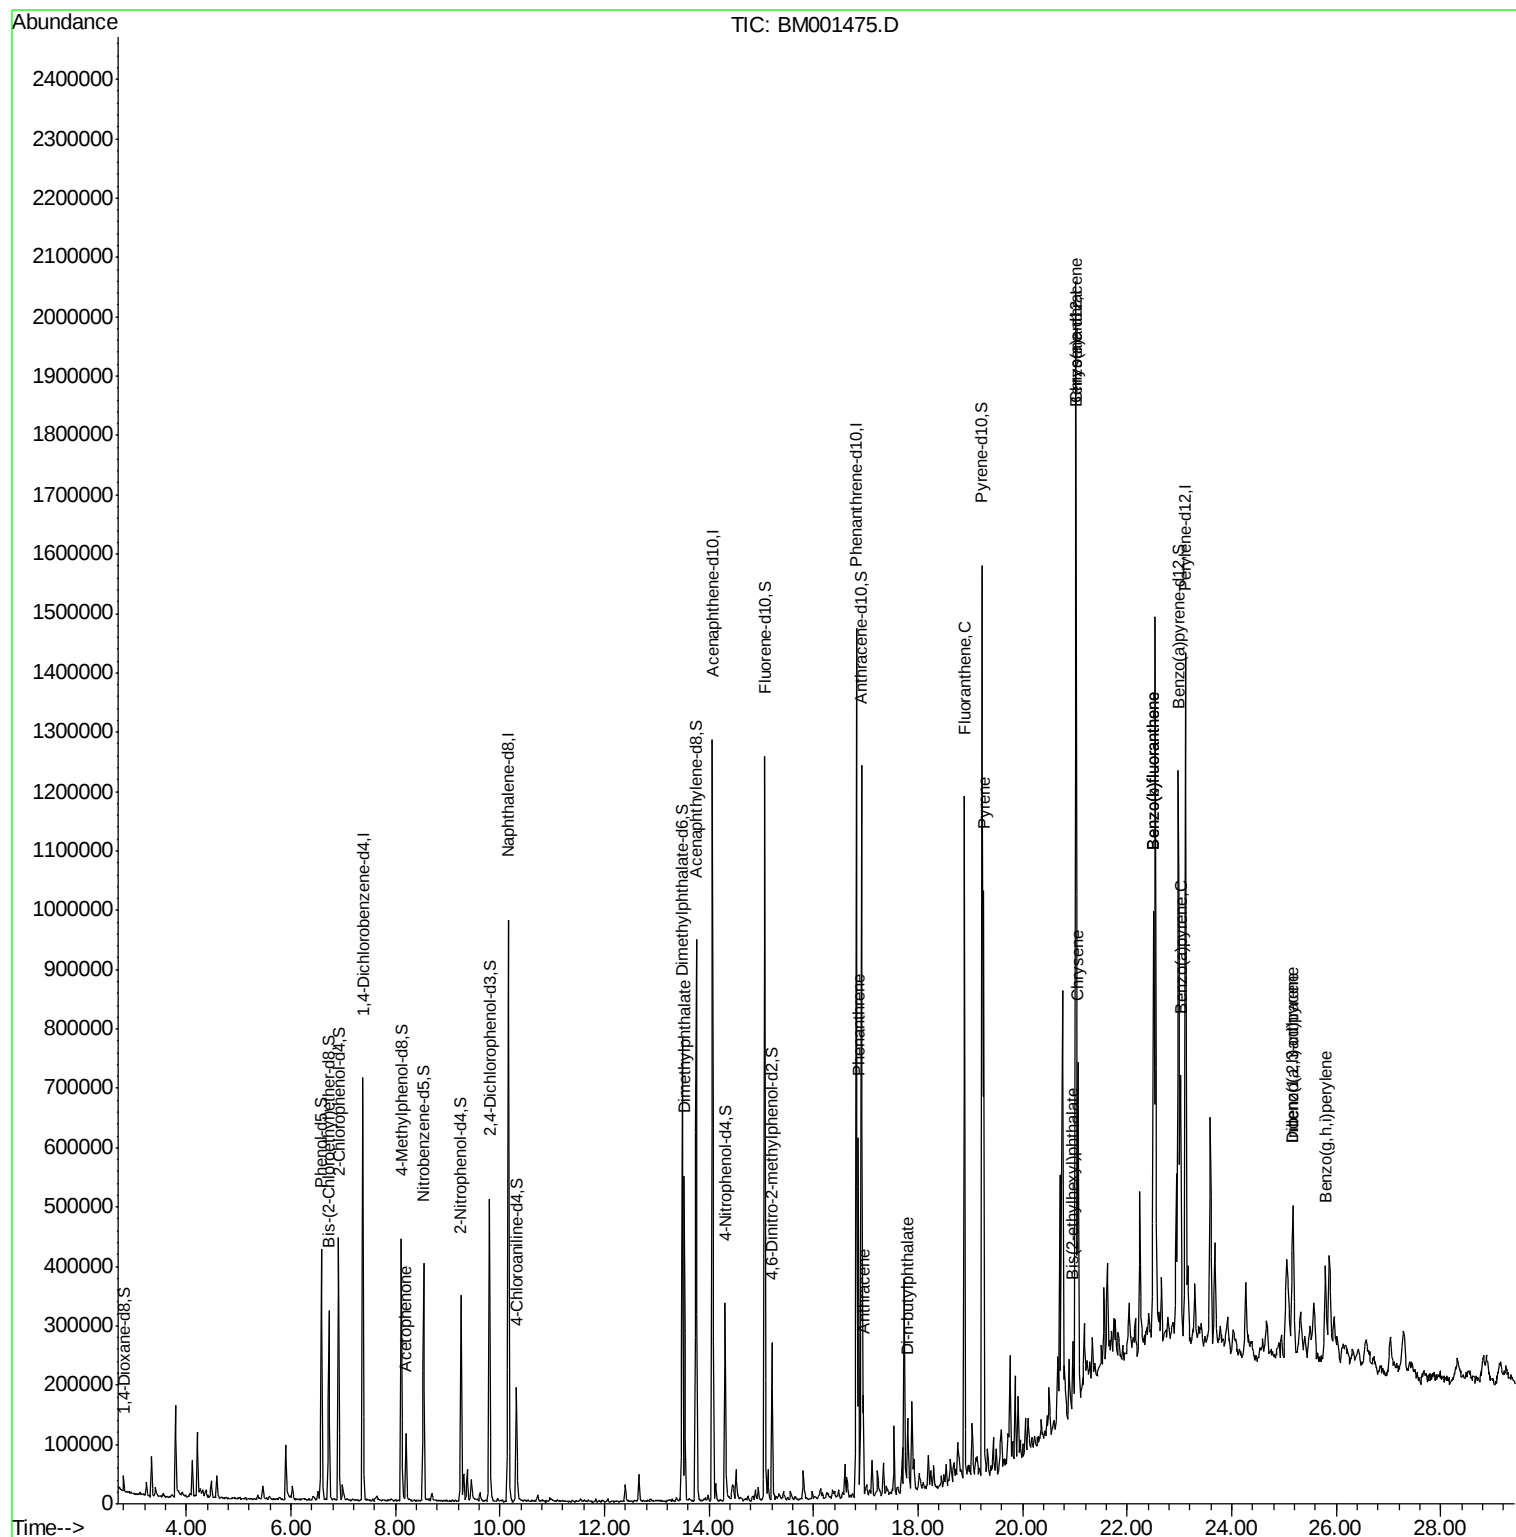

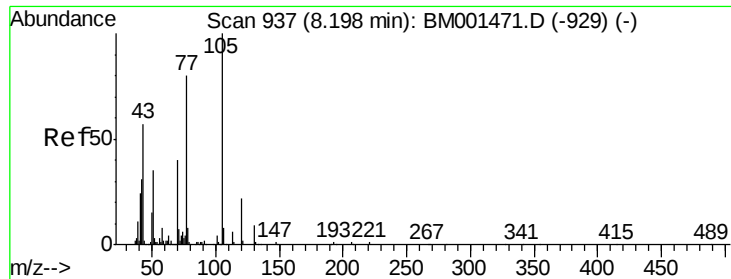

#14

Acetophenone

Concen: 3.01 ng/ul

RT: 8.20 min Scan# 937

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampleId :

BCRB7RE


Tgt Ion:105 Resp: 53470

Ion Ratio Lower Upper

105 100

77 77.0 61.6 92.4




51 35.7 27.5 41.3

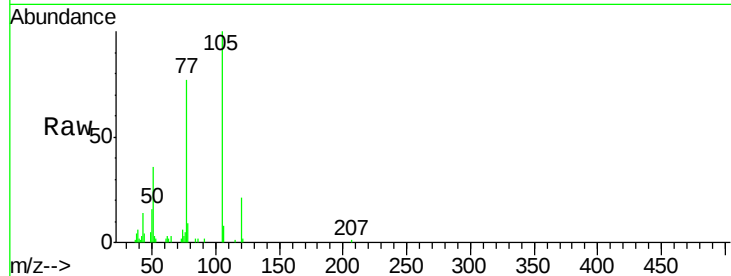

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

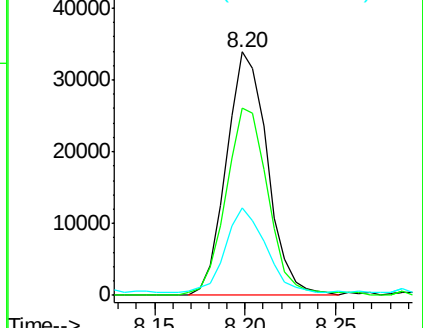

#44

Dimethylphthalate

Concen: 10.06 ng/ul

RT: 13.53 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:163 Resp: 321675

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6



164 10.9 8.2 12.4




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

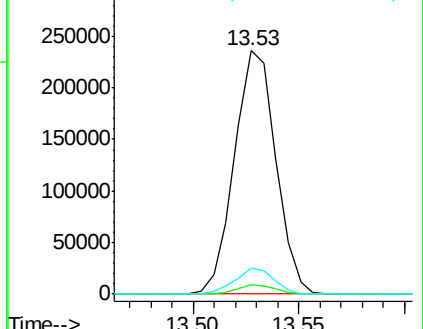

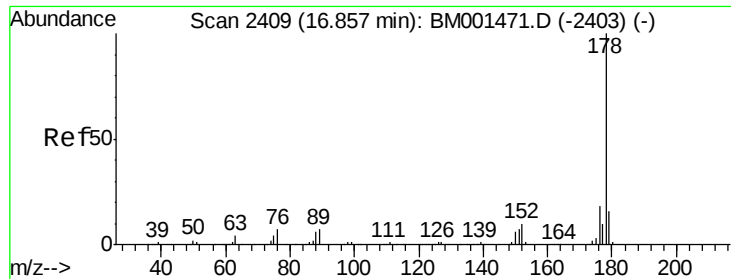

#69

Phenanthrene

Concen: 7.58 ng/u1

RT: 16.86 min Scan# 2409

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampleId :

BCRB7RE


Tgt Ion:178 Resp: 340336

Ion Ratio Lower Upper

178 100

179 15.5 11.9 17.9




176 18.2 15.0 22.4

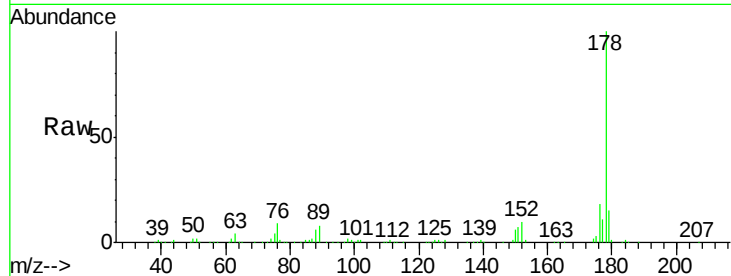

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

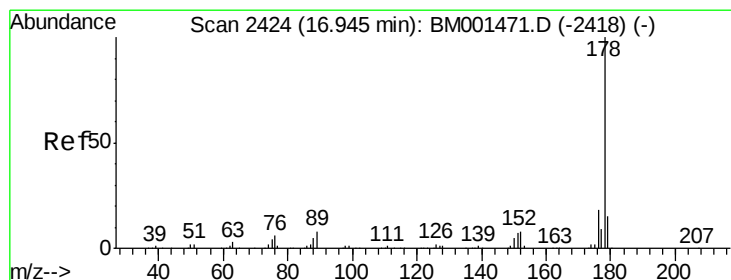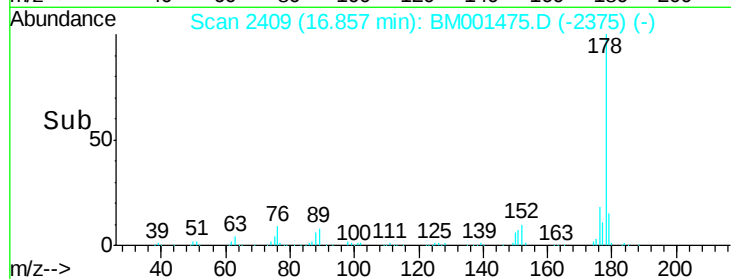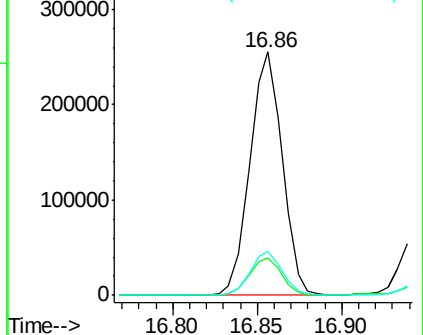

#71

Anthracene

Concen: 2.04 ng/u1

RT: 16.94 min Scan# 2424

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:178 Resp: 94255

Ion Ratio Lower Upper

178 100

179 15.6 12.1 18.1



176 19.4 14.5 21.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

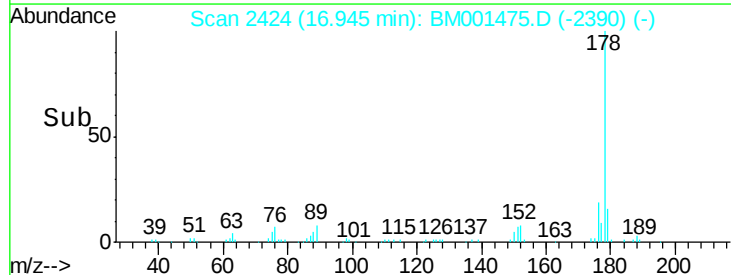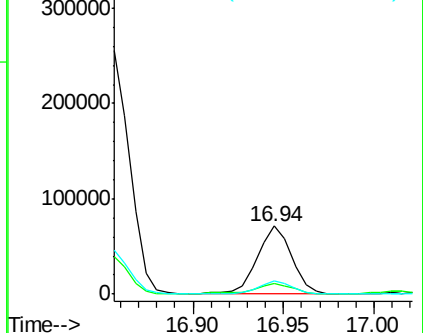



#73

Di-n-butylphthalate

Concen: 1.45 ng/ul

RT: 17.80 min Scan# 2569

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampleId :

BCRB7RE


Tgt Ion:149 Resp: 72044

Ion Ratio Lower Upper

149 100

150 10.9 6.9 10.3#




104 4.8 4.0 6.0



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

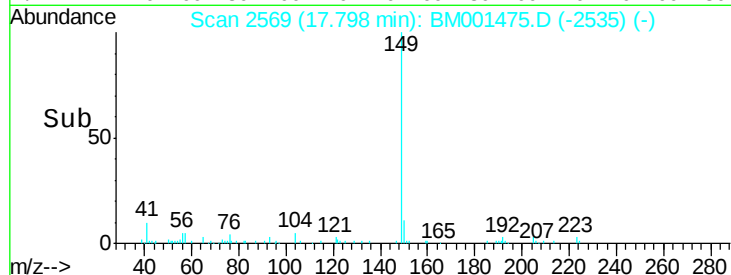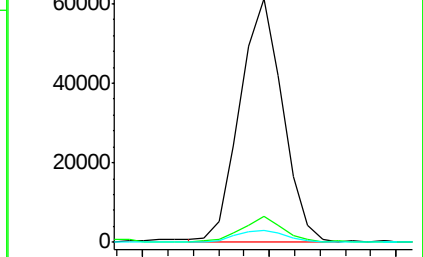

#74

Fluoranthene

Concen: 12.21 ng/ul

RT: 18.89 min Scan# 2754

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:202 Resp: 663862

Ion Ratio Lower Upper

202 100

101 9.7 8.6 12.8



100 8.1 6.5 9.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

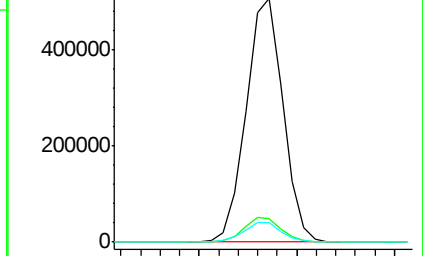

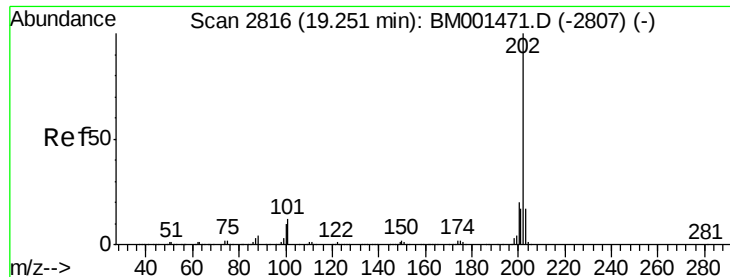

#77

Pyrene

Concen: 12.01 ng/ul

RT: 19.25 min Scan# 2816

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampled :

BCRB7RE


Tgt Ion:202 Resp: 555118

Ion Ratio Lower Upper

202 100

101 12.2 10.3 15.5




100 10.3 8.6 12.8

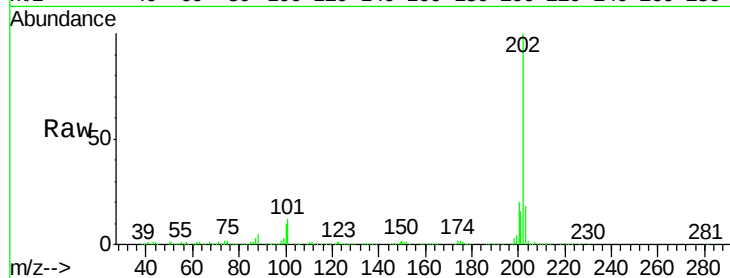

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

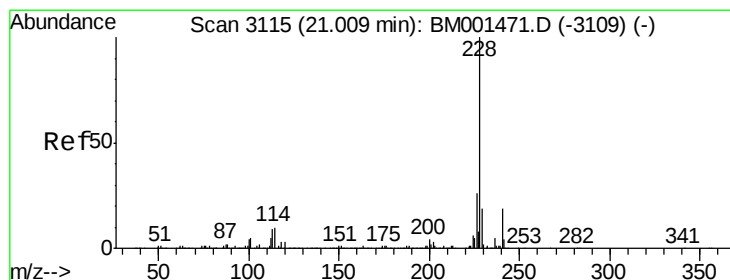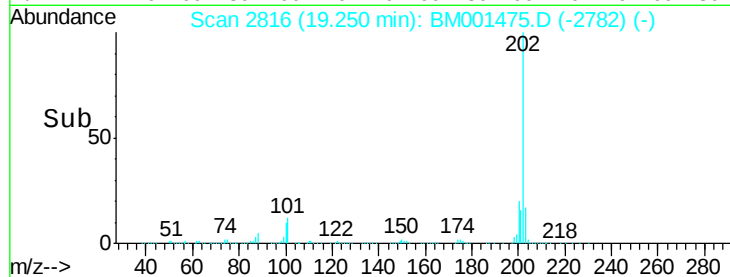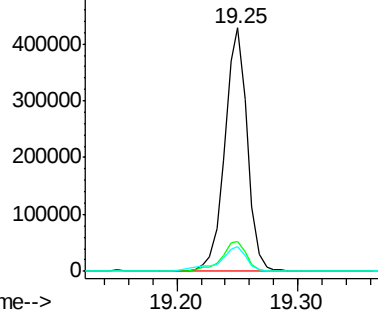

#80

Benzo(a)anthracene

Concen: 6.73 ng/ul

RT: 21.01 min Scan# 3115

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:228 Resp: 304219

Ion Ratio Lower Upper

228 100

229 19.6 15.8 23.8



226 28.0 20.6 30.8

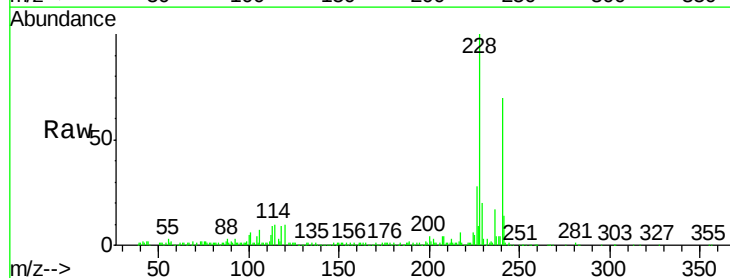


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

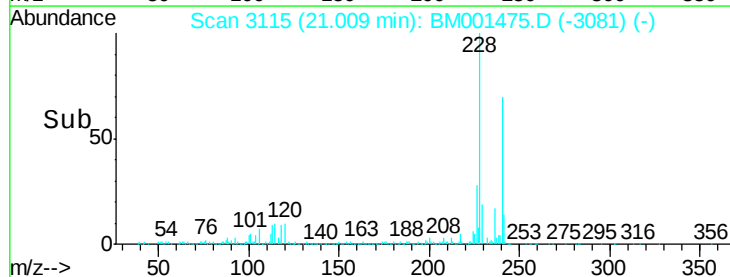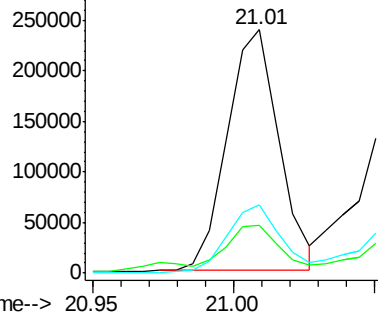


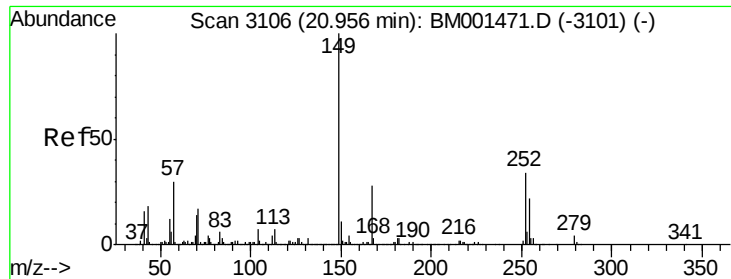




#81
 Bis(2-ethylhexyl)phthalate
 Concen: 1.35 ng/ul
 RT: 20.96 min Scan# 3106
 Delta R.T. -0.00 min
 Lab File: BM001475.D
 Acq: 30 May 2015 15:10

Instrument :
 BNA_M
 ClientSampleId :
 BCRB7RE

Tgt Ion	Ratio	Lower	Upper
149	100		
167	25.1	21.2	31.8
279	4.3	3.1	4.7

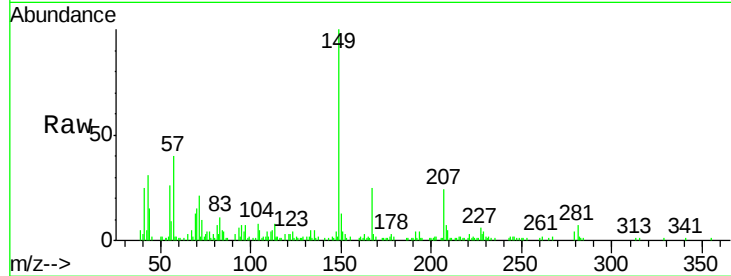


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

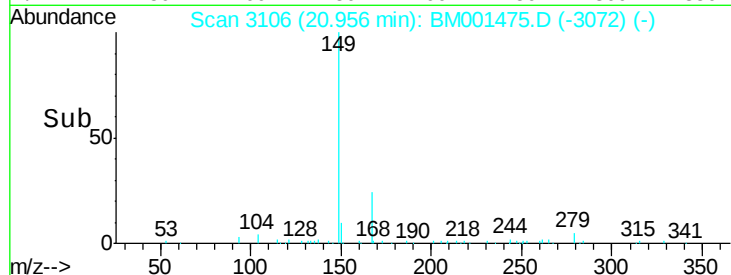
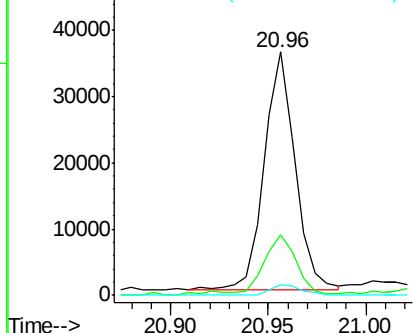



#82
 Chrysene
 Concen: 6.83 ng/ul
 RT: 21.06 min Scan# 3123
 Delta R.T. -0.00 min
 Lab File: BM001475.D
 Acq: 30 May 2015 15:10

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.4	23.0	34.4
229	22.2	15.7	23.5

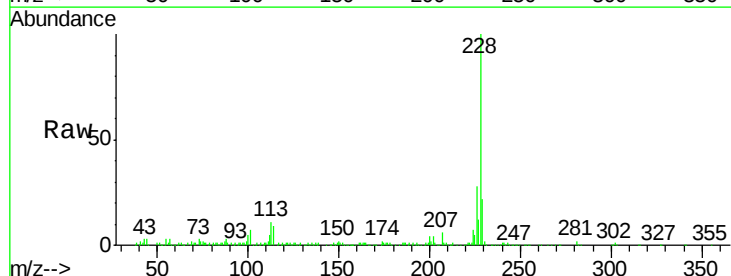

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E

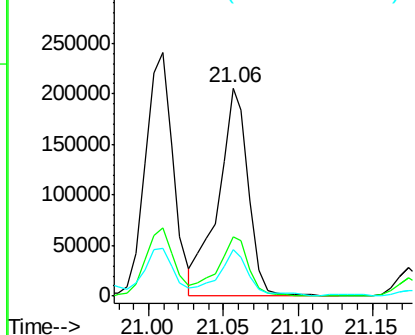

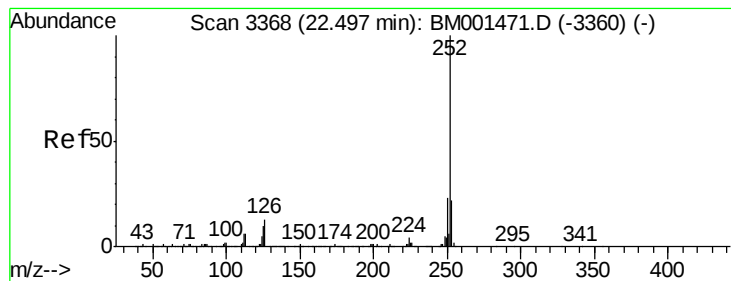

#85

Benzo(b)fluoranthene

Concen: 8.22 ng/ul

RT: 22.50 min Scan# 3368

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Instrument :

BNA_M

ClientSampleId :

BCRB7RE




Tgt Ion:	252	Resp:	355412
Ion Ratio	Lower	Upper	
252	100		
253	23.6	18.0	27.0
125	12.2	8.6	12.8



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

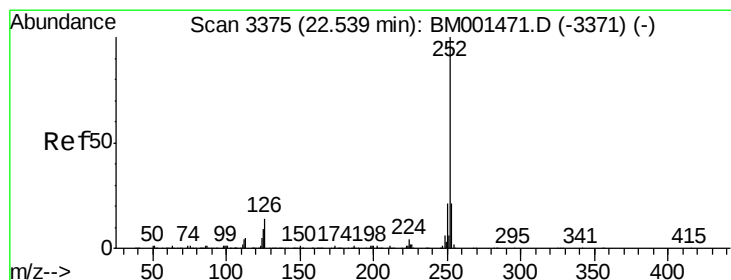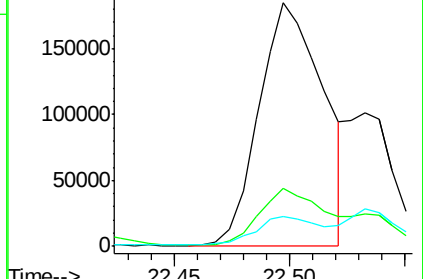

#86

Benzo(k)fluoranthene

Concen: 2.49 ng/ul


RT: 22.50 min Scan# 3368

Delta R.T. -0.04 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10



Tgt Ion:	252	Resp:	102993
Ion Ratio	Lower	Upper	
252	100		
253	23.6	17.4	26.0
125	12.2	8.6	13.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

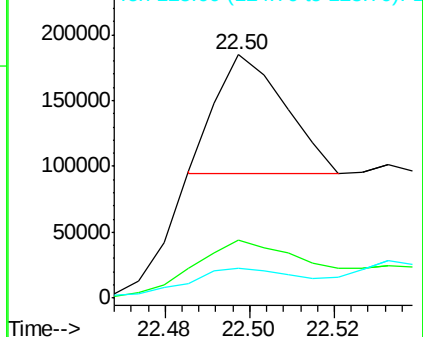



#88

Benzo(a)pyrene

Concen: 6.25 ng/ul

RT: 23.02 min Scan# 3457

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampleId :

BCRB7RE


Tgt Ion:252 Resp: 253258

Ion Ratio Lower Upper

252 100

253 21.9 17.0 25.4




125 10.7 8.8 13.2

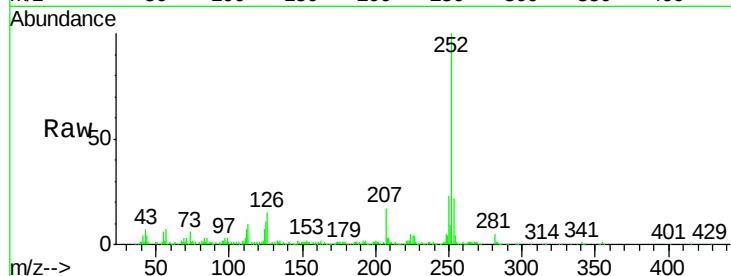

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

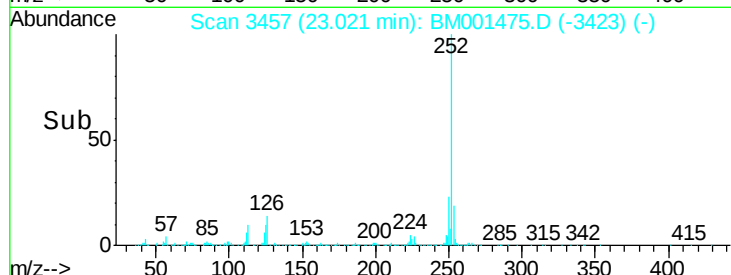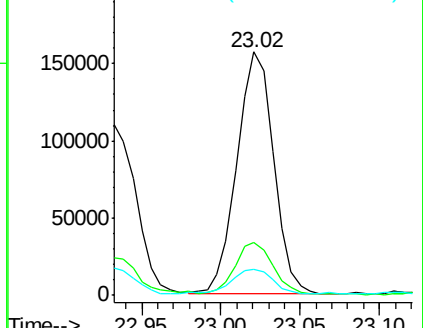

#89

Indeno(1,2,3-cd)pyrene

Concen: 3.92 ng/ul

RT: 25.16 min Scan# 3821

Delta R.T. -0.01 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:276 Resp: 167178

Ion Ratio Lower Upper

276 100

138 24.2 20.6 31.0



277 24.3 19.2 28.8




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

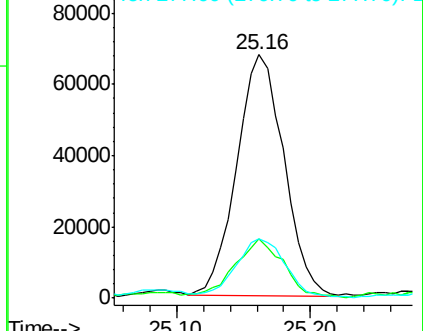

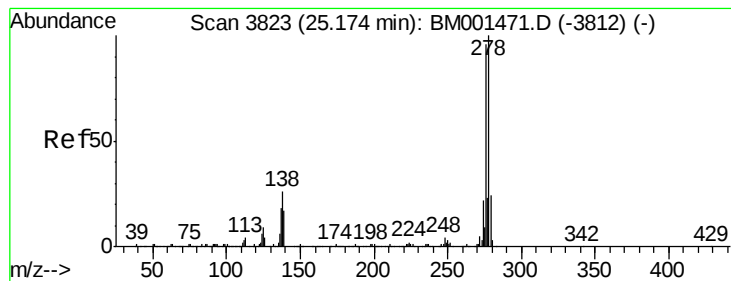

#90

Dibenzo(a,h)anthracene

Concen: 1.34 ng/ul

RT: 25.17 min Scan# 3822

Delta R.T. -0.01 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10

Instrument :

BNA_M

ClientSampleId :

BCRB7RE


Tgt Ion:278 Resp: 47870

Ion Ratio Lower Upper

278 100

139 27.1 13.8 20.8#




279 27.7 18.3 27.5#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

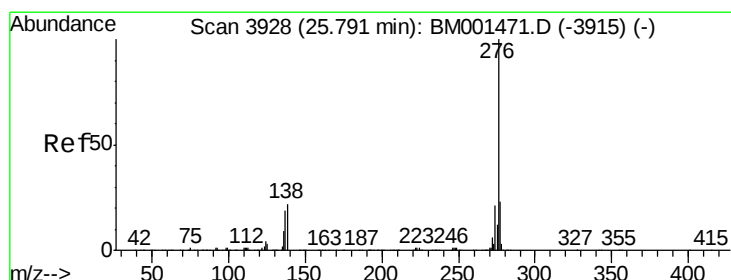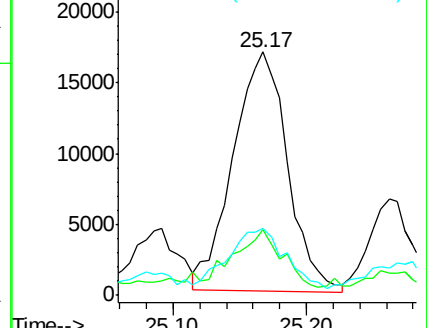

#91

Benzo(g,h,i)perylene

Concen: 4.42 ng/ul

RT: 25.79 min Scan# 3928

Delta R.T. -0.00 min

Lab File: BM001475.D

Acq: 30 May 2015 15:10


Tgt Ion:276 Resp: 155615

Ion Ratio Lower Upper

276 100

138 23.6 17.9 26.9

277 25.3 19.7 29.5



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

