

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053015\
 Data File : BM001488.D
 Acq On : 30 May 2015 23:40
 Operator : TP/IZ
 Sample : G2411-18RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BCRC9RE

Quant Time: May 31 04:30:54 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 31 04:25:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	265626	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1050136	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.06	164	562497	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.82	188	1084509	20.00	ng/ul	0.00
75) Chrysene-d12	21.02	240	1021182	20.00	ng/ul	0.00
83) Perylene-d12	23.11	264	935228	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.80	96	30742	5.78	ng/uL	0.00
5) Phenol-d5	6.59	99	742686	37.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	442486	36.10	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	629736	39.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	590273	35.59	ng/ul	0.00
19) Nitrobenzene-d5	8.54	128	299434	43.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.26	143	342867	43.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	617798	39.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.31	131	711849	38.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.49	166	1554156	39.40	ng/ul	0.00
46) Acenaphthylene-d8	13.75	160	2123315	39.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.31	143	276032	34.32	ng/ul	0.00
57) Fluorene-d10	15.07	176	1351326	34.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.21	200	130585	19.56	ng/ul	0.00
70) Anthracene-d10	16.92	188	1829403	36.59	ng/ul	0.00
76) Pyrene-d10	19.23	212	1770741	39.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	22.99	264	1363976	32.99	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.53	163	450181	10.11	ng/ul	98
81) Bis(2-ethylhexyl)phthalate	20.96	149	38547	1.01	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053015\
Data File : BM001488.D
Acq On : 30 May 2015 23:40
Operator : TP/IZ
Sample : G2411-18RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BCRC9RE

Quant Time: May 31 04:30:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 31 04:25:51 2015
Response via : Initial Calibration




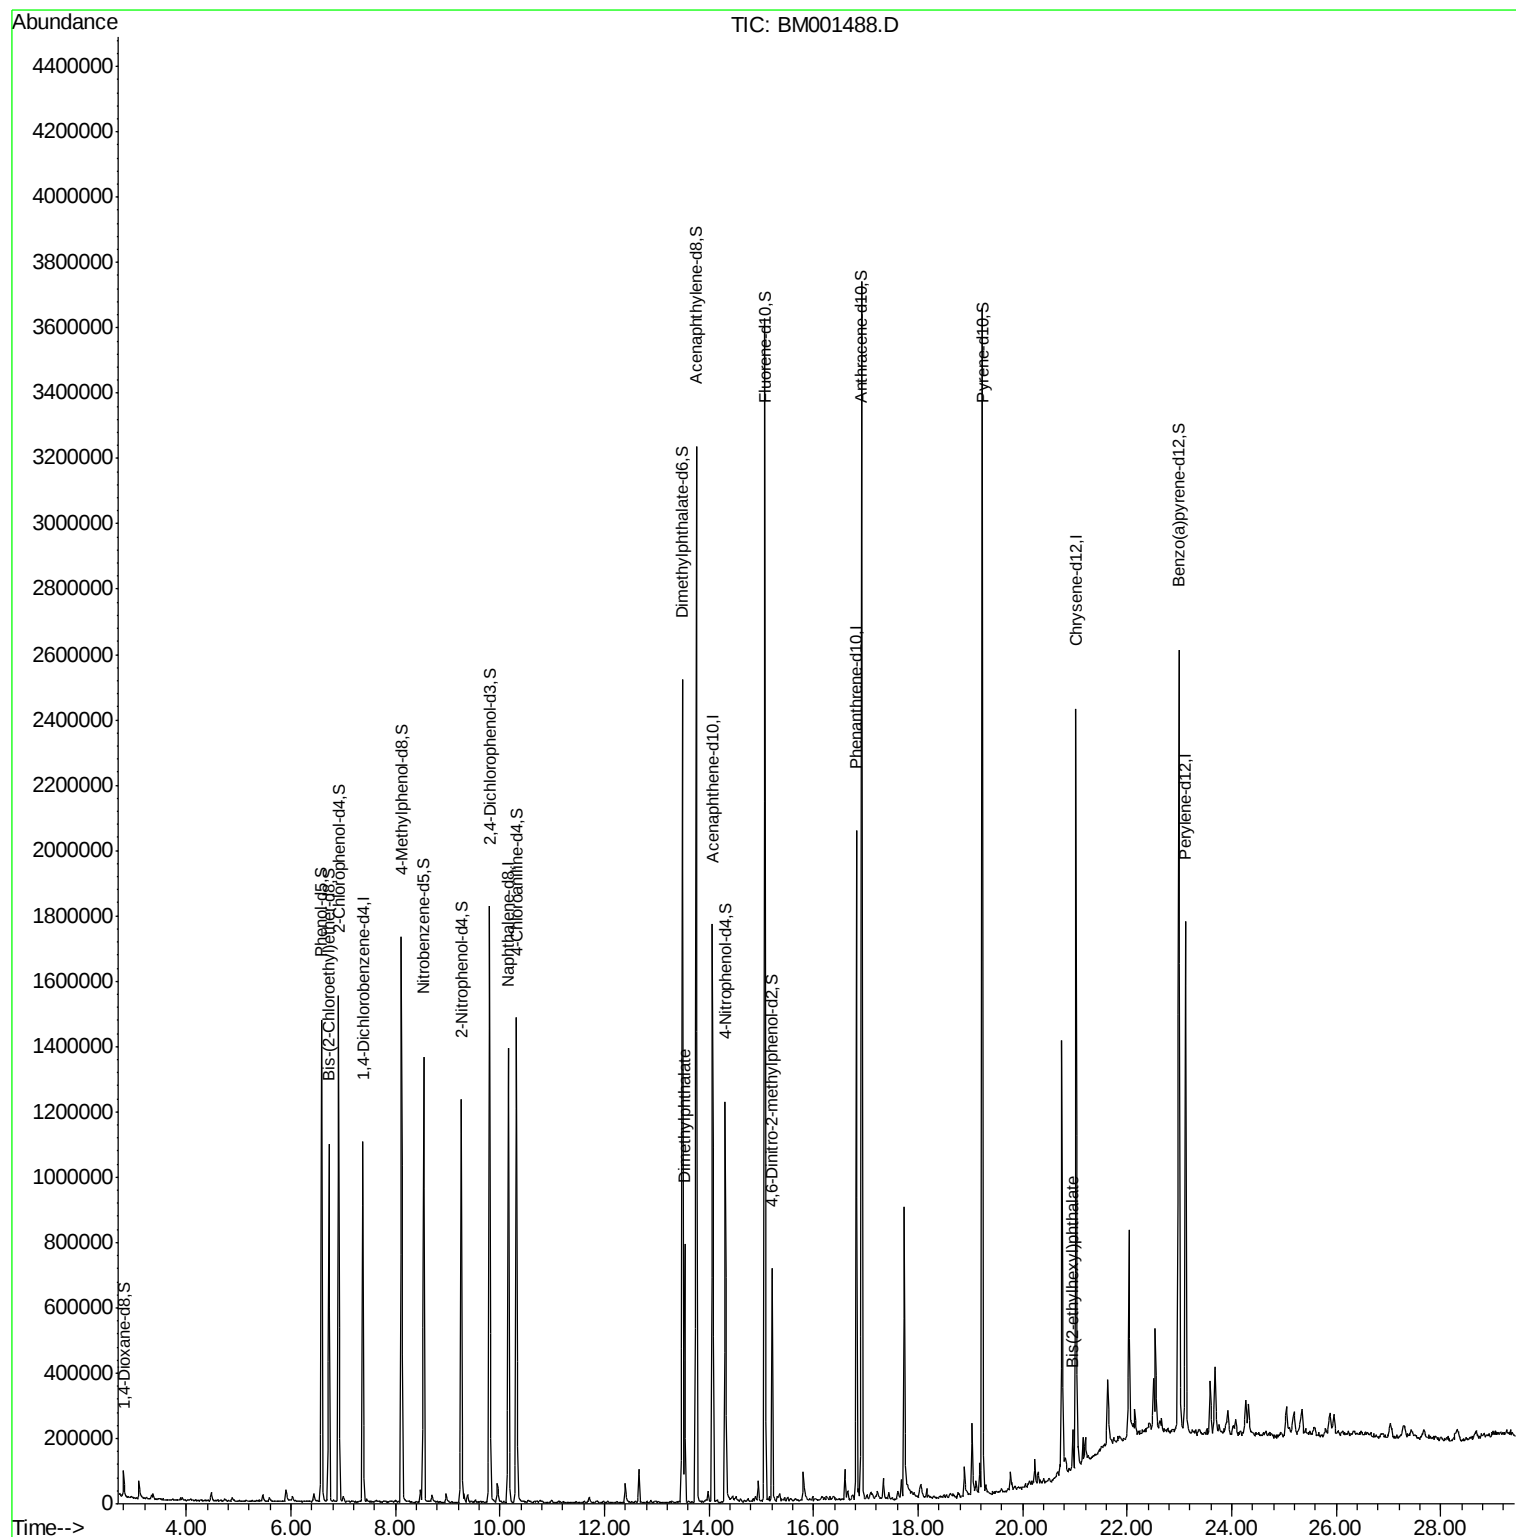


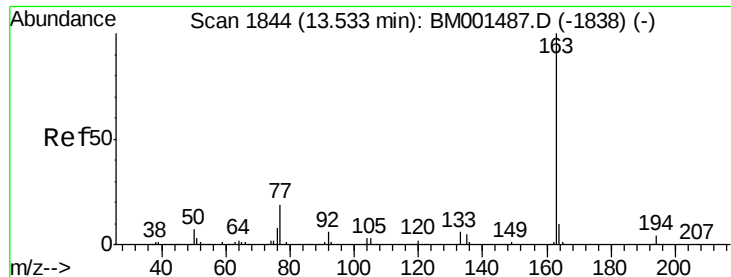

#44
 Dimethylphthalate
 Concen: 10.11 ng/ul
 RT: 13.53 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BM001488.D
 Acq: 30 May 2015 23:40

Instrument :
 BNA_M
 ClientSampleId :
 BCRC9RE

Tgt Ion:163 Resp: 450181
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.0 4.6
 164 9.3 8.2 12.4

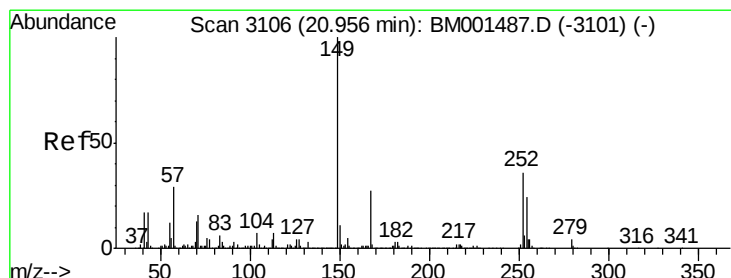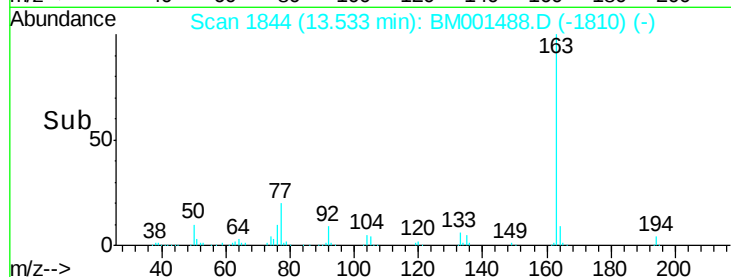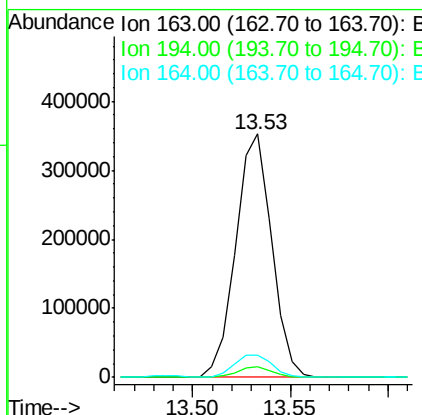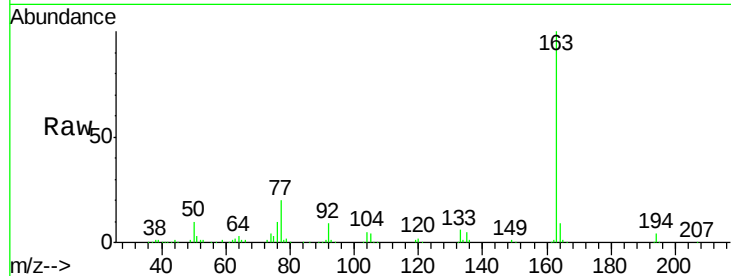

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 1.01 ng/ul
 RT: 20.96 min Scan# 3106
 Delta R.T. -0.00 min
 Lab File: BM001488.D
 Acq: 30 May 2015 23:40

Tgt Ion:149 Resp: 38547
 Ion Ratio Lower Upper
 149 100
 167 26.9 21.2 31.8
 279 3.9 3.1 4.7

