


Data Path : Z:\HPCHEM1\BNA_M\Data\BM053015\
 Data File : BM001470.D
 Acq On : 30 May 2015 11:59
 Operator : TP/IZ
 Sample : DFTPP52
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP52

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
 Title : SVOA CALIBRATION
 Last Update : Thu May 14 05:09:17 2015

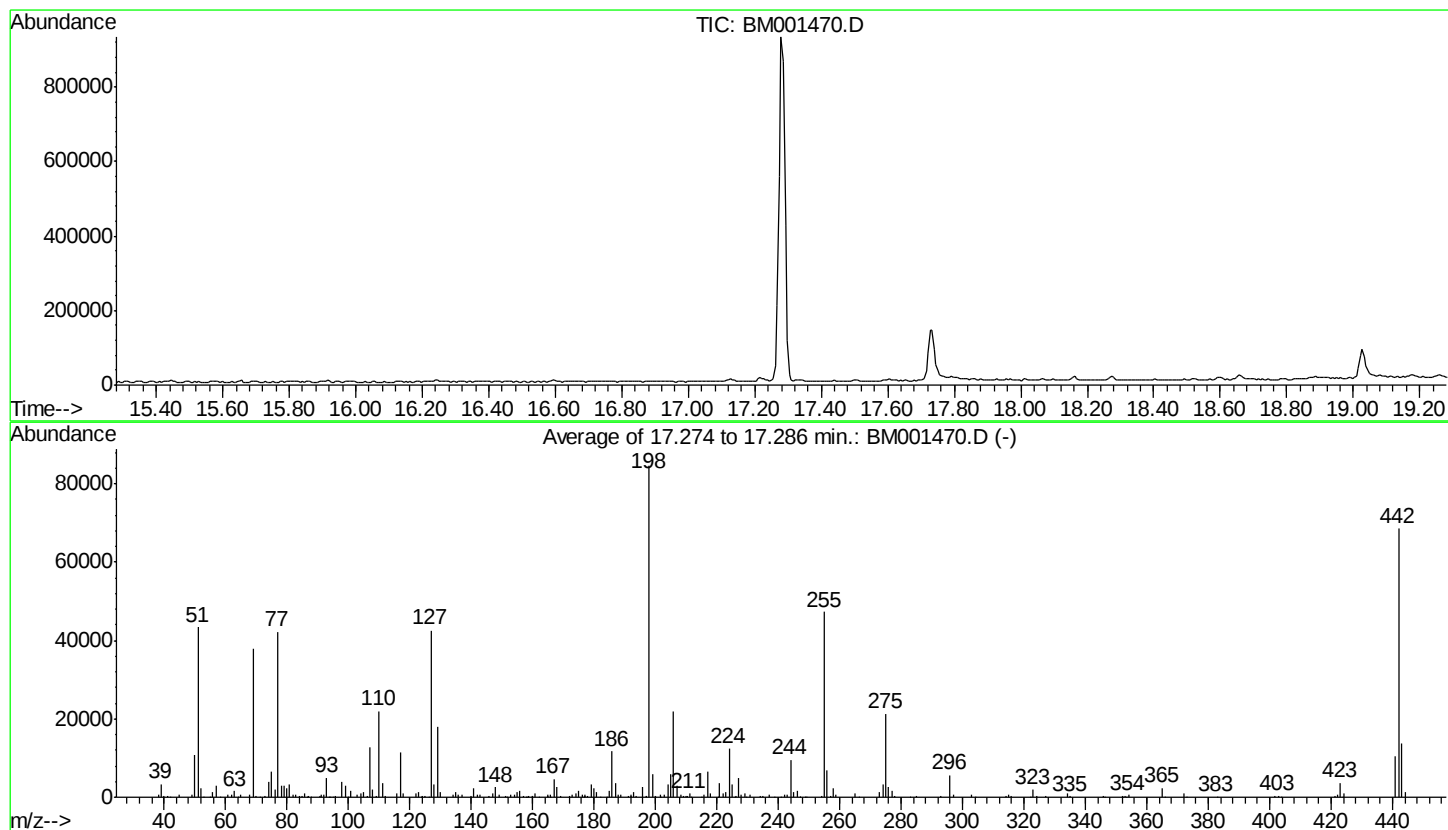

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	43394	PASS
68	69	0.00	2	1.8	688	PASS
69	198	0.00	100	44.7	37818	PASS
70	69	0.00	2	0.8	289	PASS
127	198	10	80	50.3	42562	PASS
197	198	0.00	2	0.4	307	PASS
198	198	100	100	100.0	84658	PASS
199	198	5	9	6.8	5795	PASS
275	198	10	60	25.2	21300	PASS
365	198	1	100	2.9	2445	PASS
441	443	0.01	100	77.0	10611	PASS
442	198	50	100	80.9	68504	PASS
443	442	15	24	20.1	13773	PASS

m/z	Abundance
38.10	350.0
39.10	3512.0
39.90	1160.0
41.00	798.0
43.00	1126.0
44.00	4024.0
44.90	462.0
48.90	546.0
50.00	9180.0
51.10	35168.0
52.00	1781.0
52.90	324.0
55.00	648.0
56.00	1073.0
57.10	2744.0
61.00	628.0
62.10	406.0
63.00	1351.0
65.00	691.0
68.00	651.0
69.00	30864.0
70.00	503.0
71.10	320.0
73.00	507.0
74.10	3455.0
75.00	4764.0
76.10	1569.0
77.10	34688.0
78.20	1813.0
79.00	2176.0
79.90	2012.0
81.00	2666.0
82.00	719.0
83.10	794.0
83.90	302.0
85.00	779.0
86.00	740.0
86.80	372.0
90.80	573.0
92.00	679.0
92.90	4352.0
96.00	334.0
98.00	2976.0
99.00	2720.0
100.90	1507.0
103.00	421.0
103.90	564.0
105.00	1310.0
107.00	10004.0
108.00	1225.0
109.10	472.0
110.00	16363.0
111.10	2471.0
116.00	763.0
117.00	8942.0
118.00	769.0
122.10	583.0
123.10	1024.0
123.70	393.0
125.00	339.0
127.00	33776.0
128.00	2646.0
129.00	14458.0
129.90	1289.0
134.00	466.0
135.00	1256.0
136.00	555.0
137.10	536.0
141.00	1702.0
142.20	605.0
142.90	421.0
146.90	696.0
147.90	1914.0
149.10	363.0
152.80	413.0
154.10	569.0
154.90	1149.0
156.00	937.0
158.90	372.0
159.90	666.0
161.10	811.0
164.80	747.0
165.80	321.0
167.00	3502.0
168.00	1931.0
169.00	307.0
172.80	327.0
174.00	853.0
175.00	1172.0
176.00	445.0
176.70	456.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

177.90	375.0
179.00	2234.0
180.00	1795.0
180.90	832.0
181.90	362.0
184.90	1606.0
186.00	8138.0
187.00	2807.0
188.00	378.0
188.80	527.0
191.90	938.0
193.00	1213.0
195.90	1931.0
197.00	438.0
198.00	59824.0
199.10	4123.0
199.80	424.0
201.50	310.0
203.00	469.0
204.00	1991.0
205.00	3483.0
206.00	15151.0
207.10	3223.0
208.10	484.0
209.00	400.0
210.20	321.0
211.00	380.0
215.90	477.0
217.00	4288.0
218.00	736.0
221.00	2596.0
222.00	702.0
223.10	1077.0
224.00	7688.0
225.00	2126.0
226.90	3464.0
227.90	576.0
229.00	888.0
230.90	337.0
234.00	444.0
237.00	546.0
242.10	620.0
243.00	416.0
244.10	6557.0
244.90	906.0
246.00	1175.0
246.90	395.0
255.00	30600.0
256.00	4919.0
256.90	350.0
258.00	1591.0
259.00	369.0
264.90	700.0
273.00	803.0
274.00	2314.0
275.00	14300.0
275.90	1800.0
277.00	1102.0
296.00	3163.0
297.10	543.0
303.00	505.0
314.00	322.0
322.90	864.0
324.00	319.0
334.00	465.0
335.00	300.0
346.00	388.0
351.90	366.0
353.00	393.0
354.10	362.0
365.00	1632.0
372.10	631.0
421.90	548.0
423.00	1911.0
423.80	524.0
441.00	6123.0
442.00	35592.0
443.00	6945.0
444.00	878.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
38.10	915.0
39.10	3991.0
39.90	1017.0
41.10	708.0
42.10	304.0
43.00	1127.0
44.00	3850.0
45.00	525.0
49.00	836.0
50.10	13793.0
51.00	53792.0
52.00	3260.0
55.10	921.0
56.00	1540.0
57.00	3878.0
61.00	853.0
62.10	610.0
63.10	2098.0
64.00	310.0
65.00	1156.0
68.10	951.0
69.00	46040.0
73.10	828.0
74.00	4537.0
75.00	8033.0
76.00	2251.0
77.00	51328.0
78.10	4239.0
79.00	4212.0
80.00	2782.0
80.90	3689.0
82.00	920.0
82.90	692.0
84.00	400.0
85.00	983.0
86.00	1092.0
87.00	602.0
88.00	303.0
91.00	1001.0
92.00	713.0
93.00	5927.0
93.90	339.0
95.90	457.0
98.00	5110.0
99.00	3614.0
100.10	449.0
101.00	1601.0
102.90	752.0
104.00	1217.0
105.00	1290.0
106.10	394.0
107.00	15971.0
108.00	2355.0
108.90	633.0
110.00	27360.0
111.00	4734.0
112.00	546.0
116.00	822.0
117.00	14059.0
118.00	843.0
122.10	1251.0
123.00	1590.0
123.90	984.0
125.00	680.0
127.00	50376.0
128.00	3965.0
129.00	21312.0
130.00	1574.0
134.10	864.0
135.00	1614.0
135.90	751.0
136.90	971.0
140.00	359.0
141.00	2628.0
142.00	1031.0
143.00	487.0
146.00	560.0
147.00	1333.0
147.90	2608.0
149.00	776.0
151.10	695.0
152.80	1008.0
154.00	822.0
155.00	1529.0
156.00	1999.0
157.10	389.0
157.80	416.0
159.00	347.0
160.10	886.0
161.00	1125.0
164.80	779.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

166.00	1156.0
167.00	5731.0
168.00	3238.0
168.80	421.0
172.00	696.0
172.90	607.0
174.00	1103.0
175.10	1955.0
176.00	546.0
176.90	875.0
178.00	447.0
179.00	3817.0
180.00	2757.0
181.00	1760.0
184.00	415.0
184.90	1832.0
186.00	14566.0
187.00	4474.0
188.10	671.0
188.80	874.0
191.20	471.0
192.10	1291.0
192.90	1378.0
193.90	539.0
195.90	2934.0
196.80	485.0
197.90	99320.0
199.00	6728.0
200.00	697.0
201.50	805.0
203.00	790.0
204.00	3711.0
205.00	7394.0
206.00	25608.0
207.10	4029.0
208.10	825.0
209.00	577.0
209.80	331.0
210.30	361.0
211.10	967.0
214.90	435.0
216.00	725.0
217.00	7835.0
218.00	1195.0
220.30	385.0
221.00	4226.0
221.80	1347.0
223.00	1385.0
224.00	14507.0
225.00	3846.0
226.00	501.0
227.00	5579.0
228.00	1042.0
229.00	1000.0
230.90	765.0
234.00	479.0
235.00	507.0
236.90	733.0
238.90	354.0
241.00	344.0
241.90	746.0
243.00	773.0
244.10	10665.0
245.00	1600.0
246.00	2145.0
247.10	415.0
248.90	516.0
254.10	400.0
255.00	56584.0
256.00	8048.0
256.90	421.0
258.00	3066.0
258.90	743.0
265.00	1209.0
266.10	343.0
273.00	1798.0
274.00	4017.0
275.00	23264.0
276.00	2961.0
277.00	2016.0
277.90	317.0
283.00	335.0
285.10	442.0
293.00	362.0
296.00	6315.0
297.00	774.0
303.00	643.0
304.00	300.0
314.90	724.0
315.90	380.0
323.00	2461.0
324.00	524.0
326.90	478.0
333.90	1123.0
335.00	462.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

346.20	359.0
352.10	497.0
353.20	329.0
354.10	566.0
365.00	2773.0
372.10	1423.0
401.80	365.0
402.90	561.0
421.00	756.0
421.90	765.0
423.00	4135.0
424.10	1184.0
441.00	11386.0
442.00	75328.0
443.00	15727.0
444.00	1807.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
38.10	796.0
39.10	3615.0
39.90	1104.0
41.10	914.0
43.00	950.0
44.00	3715.0
44.90	709.0
48.90	585.0
50.00	9493.0
51.10	41224.0
52.00	1796.0
55.10	907.0
55.90	1577.0
57.10	3354.0
58.10	326.0
60.90	528.0
62.00	1027.0
63.00	1262.0
64.90	562.0
67.90	463.0
69.00	36552.0
70.00	366.0
73.10	650.0
74.00	4131.0
75.00	6392.0
76.10	2121.0
77.10	40928.0
78.00	3099.0
79.00	2698.0
80.00	2179.0
81.00	3025.0
82.10	758.0
82.90	723.0
85.00	605.0
85.90	728.0
87.10	496.0
91.10	1022.0
92.00	764.0
93.00	4831.0
94.10	443.0
95.00	301.0
97.10	349.0
97.90	3559.0
99.00	2850.0
101.00	1767.0
102.90	354.0
104.00	1137.0
105.00	1006.0
106.00	380.0
107.00	12735.0
108.00	2042.0
110.00	22016.0
111.00	3466.0
111.90	487.0
116.00	945.0
117.00	11397.0
118.10	1097.0
122.00	782.0
123.00	1321.0
124.00	503.0
124.90	449.0
126.10	302.0
127.00	43536.0
128.00	3277.0
129.00	17960.0
130.00	1281.0
134.00	511.0
135.00	1267.0
136.10	556.0
137.10	891.0
140.00	397.0
140.90	2319.0
142.00	726.0
143.00	699.0
145.90	421.0
147.10	1260.0
147.90	3004.0
149.10	639.0
151.80	395.0
152.90	801.0
154.00	623.0
155.00	1560.0
156.00	2103.0
157.00	314.0
158.10	426.0
158.80	466.0
159.90	730.0
160.90	1423.0
161.90	308.0
165.00	1135.0
165.90	861.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

167.00	4851.0
168.00	2645.0
169.00	752.0
171.90	570.0
172.90	639.0
174.00	913.0
175.00	1702.0
176.10	648.0
176.80	908.0
177.10	967.0
179.10	3476.0
180.00	2293.0
181.00	1639.0
185.00	1845.0
186.00	12224.0
187.00	3372.0
188.10	651.0
188.80	984.0
191.00	544.0
192.10	1163.0
193.00	1214.0
193.80	400.0
195.90	3312.0
197.10	718.0
198.00	94832.0
199.00	6535.0
199.90	500.0
201.30	554.0
201.80	353.0
203.10	877.0
204.00	3781.0
205.00	6320.0
206.00	25352.0
207.00	3547.0
208.10	870.0
208.90	331.0
209.80	347.0
210.20	321.0
211.00	1198.0
211.70	363.0
215.90	674.0
217.00	7465.0
217.90	906.0
221.00	4023.0
222.00	1052.0
223.00	1499.0
224.00	14769.0
225.00	3798.0
226.20	646.0
227.00	5682.0
228.00	676.0
229.10	1295.0
229.70	302.0
230.90	436.0
234.10	349.0
234.80	566.0
237.00	582.0
242.00	422.0
243.00	695.0
244.10	11287.0
245.00	1461.0
246.10	1753.0
249.10	350.0
254.10	690.0
255.00	54816.0
256.00	7800.0
257.00	607.0
257.90	2396.0
258.80	506.0
265.00	1269.0
272.90	1792.0
274.00	3959.0
275.00	26336.0
276.00	2899.0
277.00	2279.0
277.90	485.0
285.00	447.0
293.10	345.0
296.00	7254.0
297.00	1156.0
303.00	513.0
314.00	351.0
315.00	919.0
316.00	758.0
322.00	351.0
323.00	2309.0
323.90	320.0
326.90	678.0
334.00	1189.0
345.90	444.0
352.00	676.0
352.90	500.0
354.10	963.0
365.00	2932.0
366.00	427.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

371.90	920.0
373.00	400.0
382.90	382.0
401.90	593.0
402.90	779.0
403.90	418.0
421.10	506.0
422.00	710.0
423.00	5031.0
424.00	1330.0
441.00	14326.0
442.00	94592.0
443.00	18648.0
444.00	1329.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

Scan 2475 (17.245 min): BM001470.D
DFTPP52

m/z	Abundance
39.10	325.0
39.90	797.0
41.00	616.0
43.10	1082.0
44.00	4071.0
55.10	787.0
57.00	301.0
73.00	362.0
85.10	337.0
97.00	301.0
207.10	616.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52