

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053115\
 Data File : BM001493.D
 Acq On : 31 May 2015 03:18
 Operator : TP/IZ
 Sample : SSTDICC002
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC002

Quant Time: May 31 05:13:51 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM053115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun May 31 05:09:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	14016	5.00	ng	0.00
6) Naphthalene-d8	10.15	136	52030	5.00	ng	0.00
9) Acenaphthene-d10	14.07	164	26664	5.00	ng	0.00
15) Phenanthrene-d10	16.81	188	52770	5.00	ng	0.00
17) Chrysene-d12	21.03	240	42254	5.00	ng	0.00
21) Perylene-d12	23.11	264	36741	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 2-Fluorophenol	4.97	112	5498	2.36	ng	0.00
3) Phenol-d6	6.57	99	7329	2.95	ng	0.00
7) Nitrobenzene-d5	8.53	82	5870	2.09	ng	0.00
10) 2,4,6-Tribromophenol	15.57	330	1966	2.37	ng	0.00
11) 2-Fluorobiphenyl	12.67	172	16097	2.14	ng	0.00
18) Terphenyl-d14	19.46	244	11742	2.22	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
4) bis(2-Chloroethyl)ether	6.80	93	5519	2.13	ng	86
5) n-Nitroso-di-n-propylamine	8.18	70	4710	3.05	ng	# 96
8) bis(2-Chloroethoxy)methane	9.58	93	7220	2.55	ng	97
12) 2,6-Dinitrotoluene	13.65	165	2880	2.52	ng	94
13) 2,4-Dinitrotoluene	14.45	165	3338	2.53	ng	# 82
14) 4-Chlorophenyl-phenylether	15.11	204	7809	1.94	ng	97
16) 4-Bromophenyl-phenylether	16.02	248	4478	2.16	ng	97
19) Benzo(a)anthracene	21.00	228	23230	8.74	ng	# 85
20) 3,3'-Dichlorobenzidine	20.95	252	8039	2.87	ng	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053115\
Data File : BM001493.D
Acq On : 31 May 2015 03:18
Operator : TP/IZ
Sample : SSTDICC002
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC002

Quant Time: May 31 05:13:51 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM053115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 31 05:09:58 2015
Response via : Initial Calibration

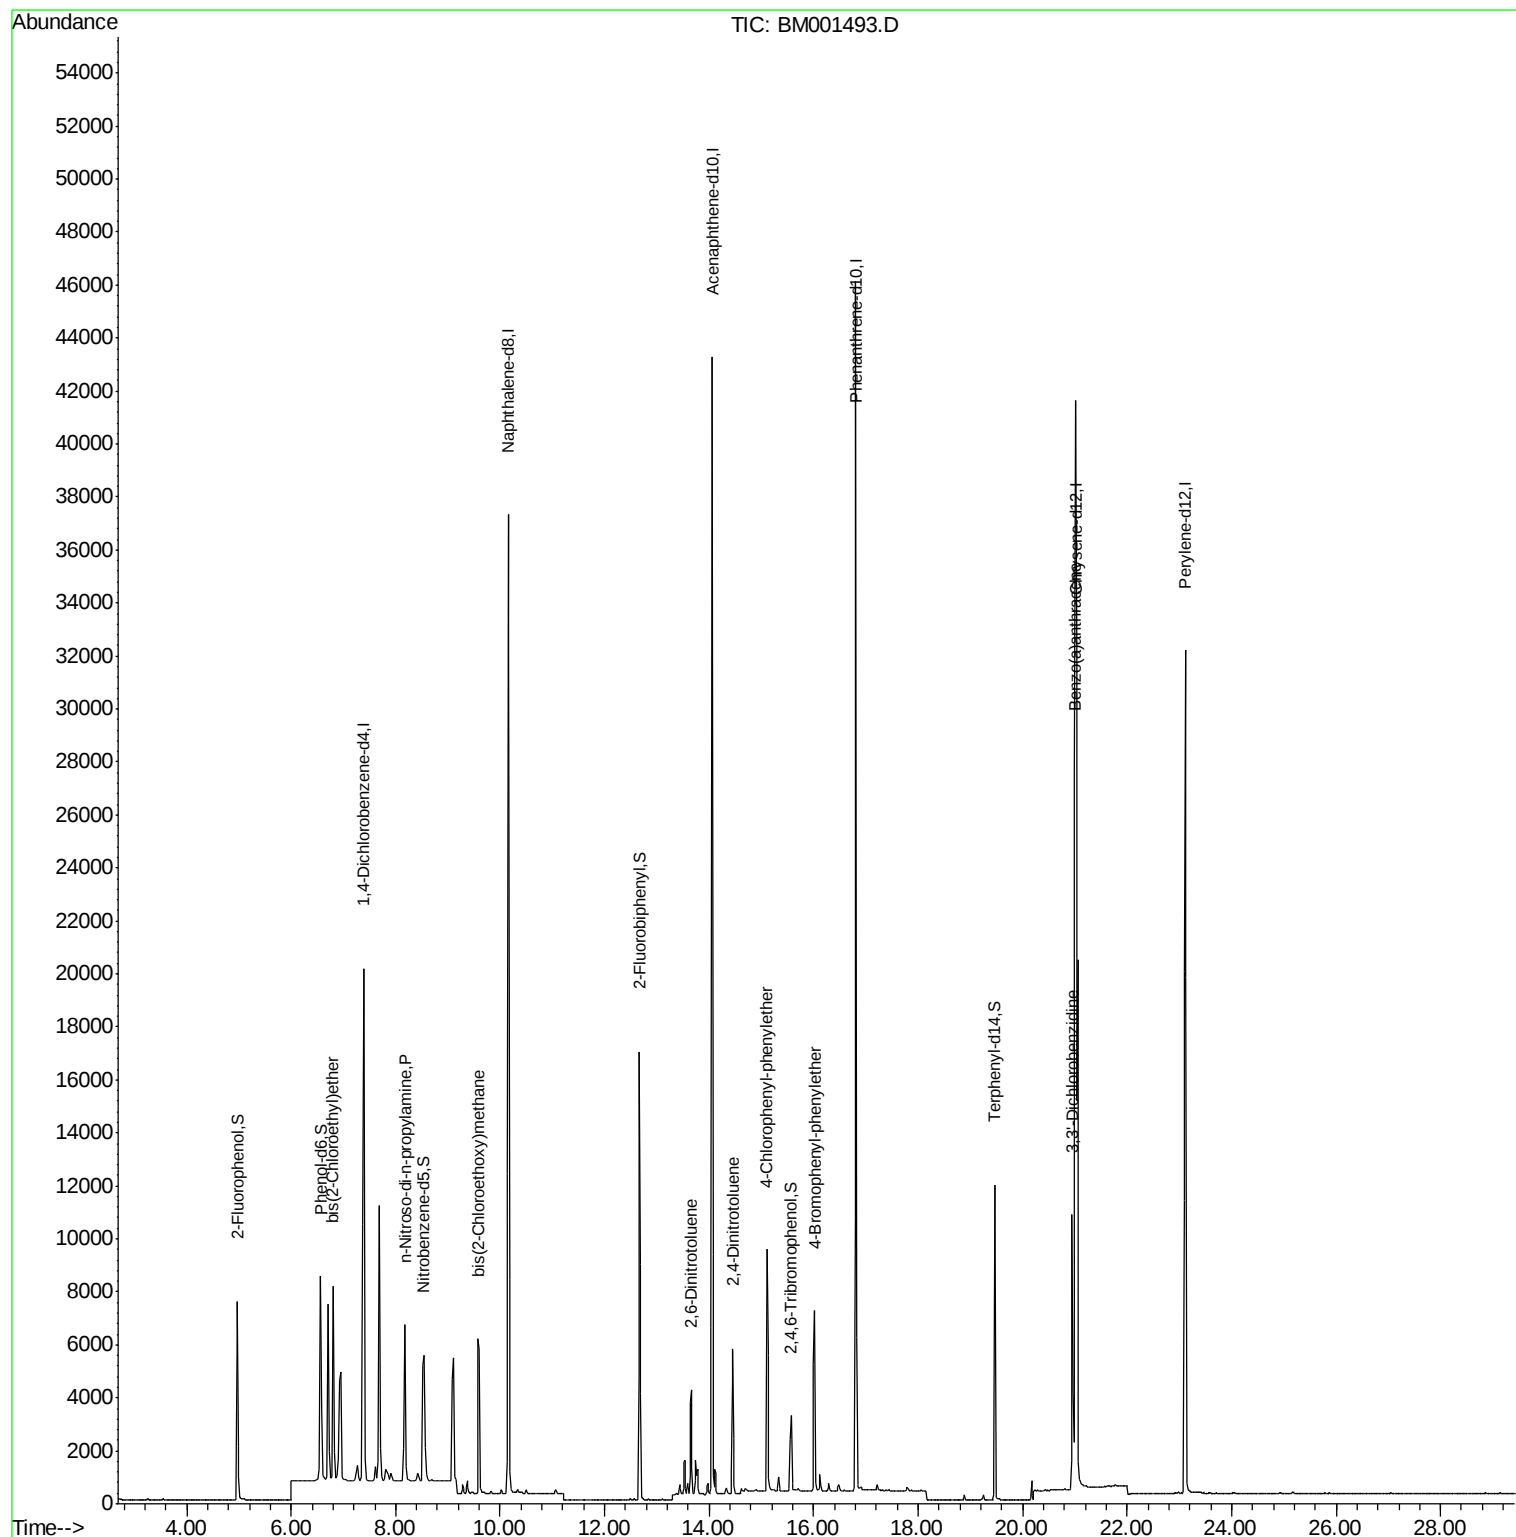




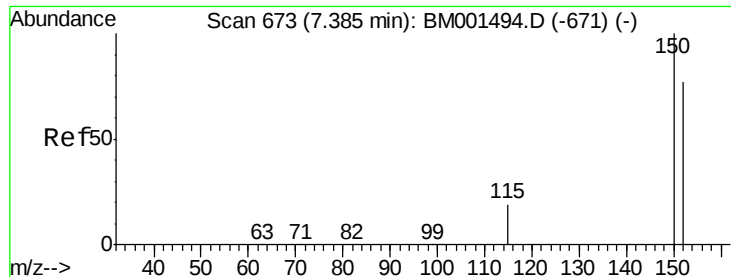


#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.38 min Scan# 673
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18

Instrument :
BNA_M
ClientSampleId :
SSTDIC002




Tgt Ion:152 Resp: 14016
Ion Ratio Lower Upper
152 100
150 134.0 103.8 155.8
115 27.6 20.7 31.1

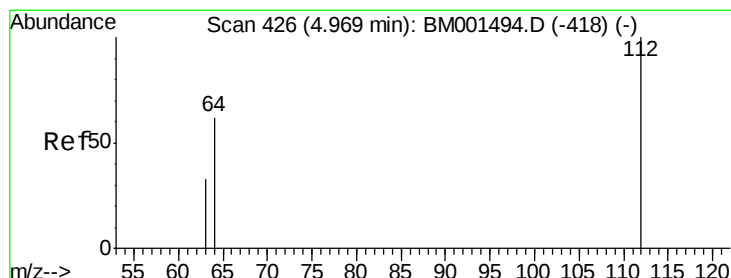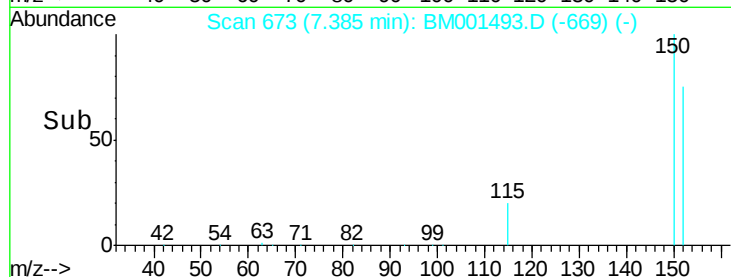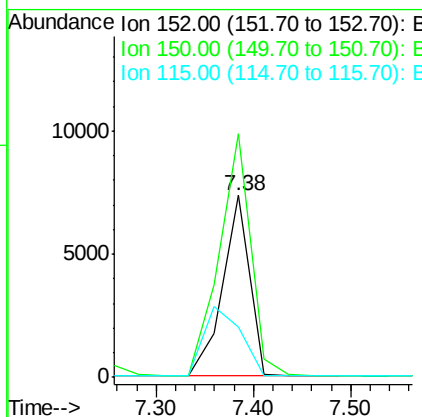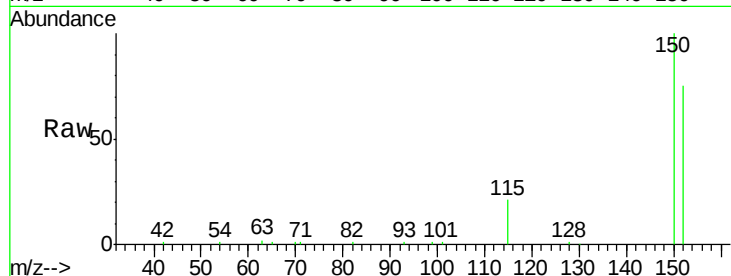


#2

2-Fluorophenol
Concen: 2.36 ng
RT: 4.97 min Scan# 426
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18

Tgt Ion:112 Resp: 5498
Ion Ratio Lower Upper
112 100
64 64.5 50.2 75.2
63 35.8 28.2 42.4

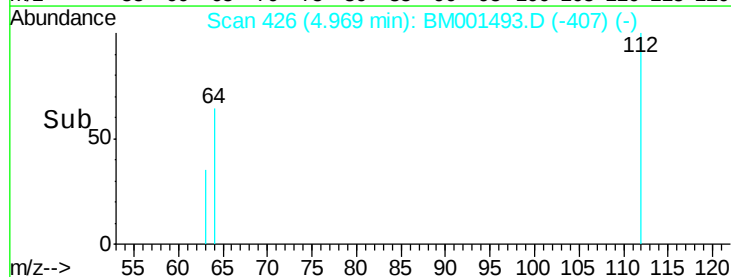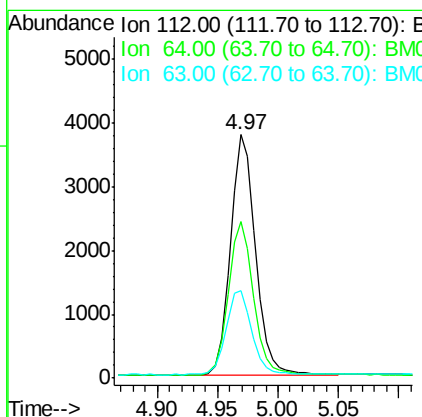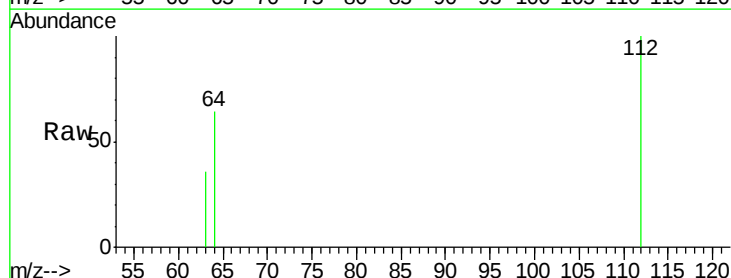

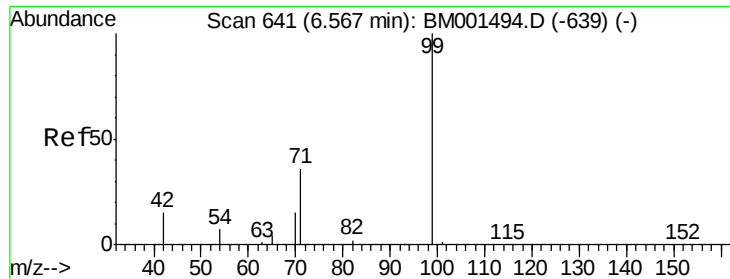

#3

Phenol-d6

Concen: 2.95 ng

RT: 6.57 min Scan# 641

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC002


Tgt Ion: 99 Resp: 7329

Ion Ratio Lower Upper

99 100

42 20.2 15.2 22.8




71 40.7 30.6 46.0

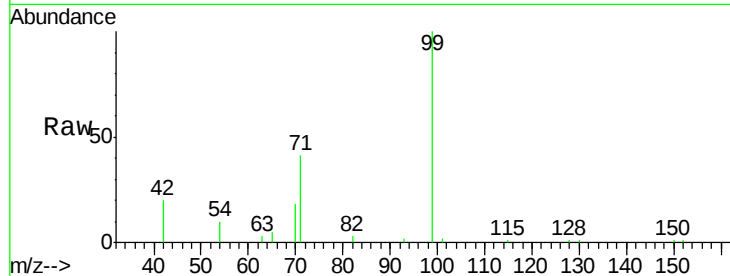

Abundance Ion 99.00 (98.70 to 99.70): BM001493.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM001493.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM001493.D (-637) (-)

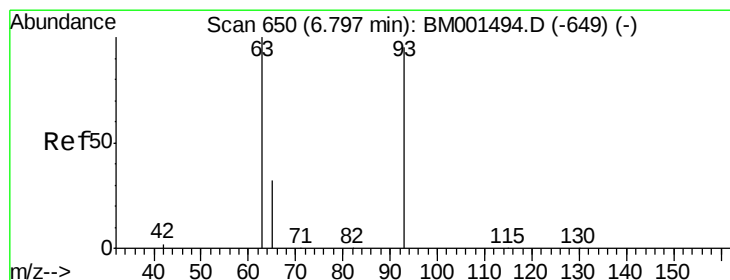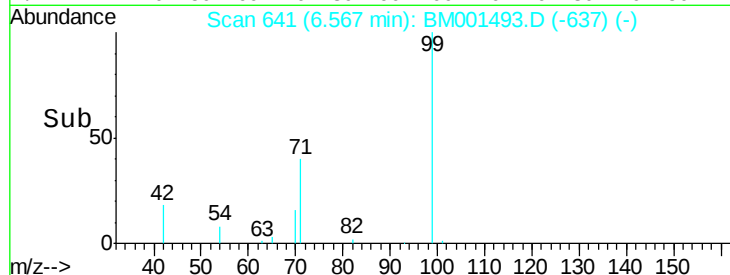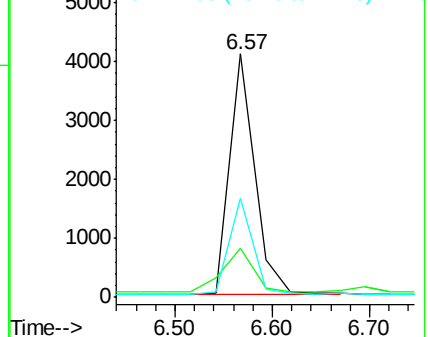

#4

bis(2-Chloroethyl)ether

Concen: 2.13 ng

RT: 6.80 min Scan# 650

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18


Tgt Ion: 93 Resp: 5519

Ion Ratio Lower Upper

93 100

63 121.0 86.8 126.8



95 0.0 0.0 20.0

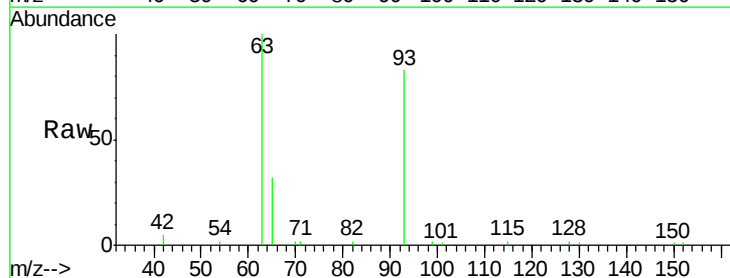


Abundance Ion 93.00 (92.70 to 93.70): BM001493.D (-646) (-)

Ion 63.00 (62.70 to 63.70): BM001493.D (-646) (-)

Ion 95.00 (94.70 to 95.70): BM001493.D (-646) (-)

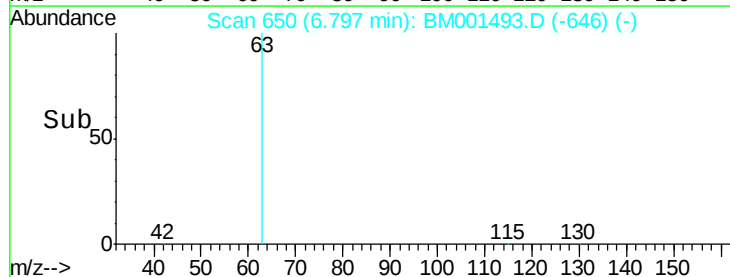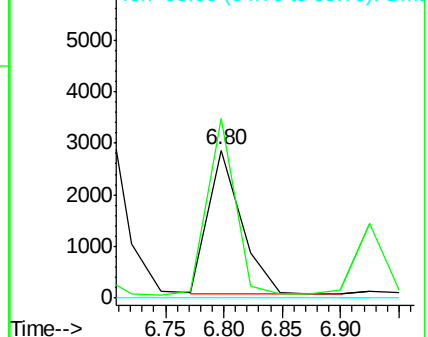

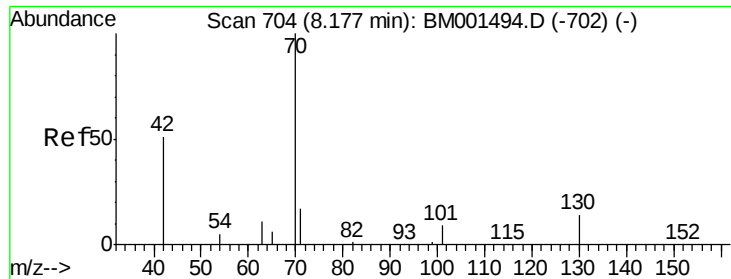

#5

n-Nitroso-di-n-propylamine

Concen: 3.05 ng

RT: 8.18 min Scan# 704

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18





Instrument :

BNA_M

ClientSampleId :

SSTDICC002

Tgt Ion:	70	Resp:	4710
Ion	Ratio	Lower	Upper
70	100		
42	55.6	44.2	66.2
101	10.0	10.3	15.5#
130	12.7	13.9	20.9#

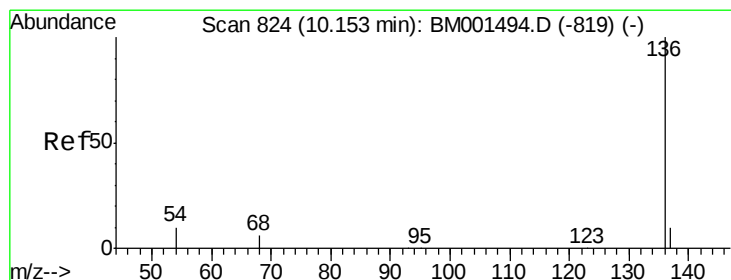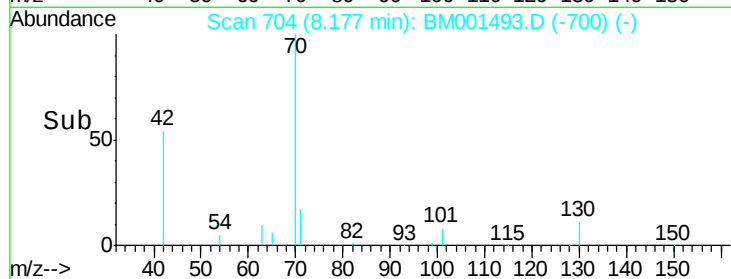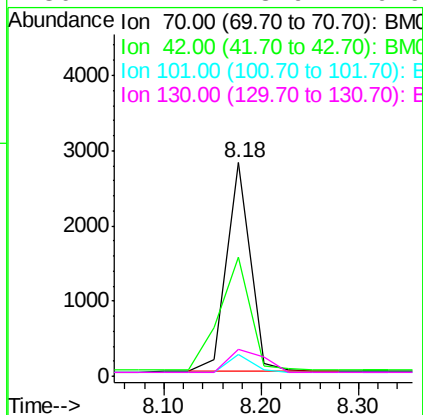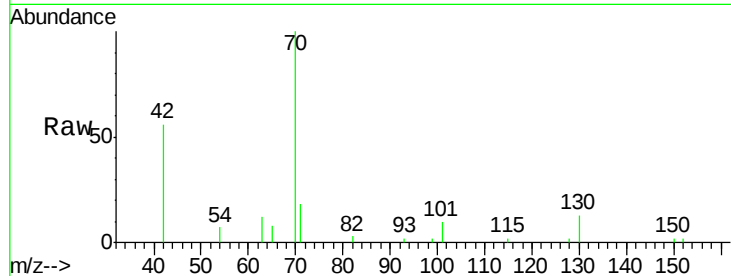

#6

Naphthalene-d8

Concen: 5.00 ng




RT: 10.15 min Scan# 824


Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Tgt Ion:	136	Resp:	52030
Ion	Ratio	Lower	Upper
136	100		
137	10.2	8.3	12.5
54	11.9	8.5	12.7
68	6.8	5.0	7.4

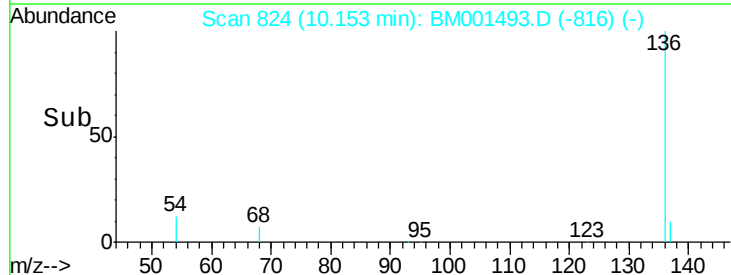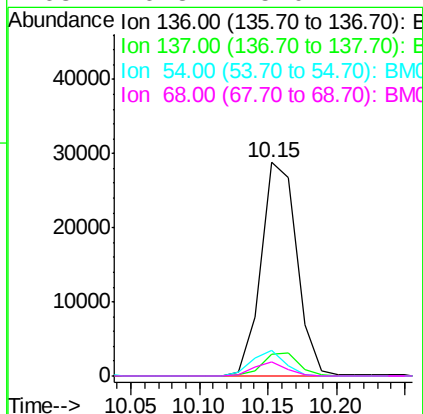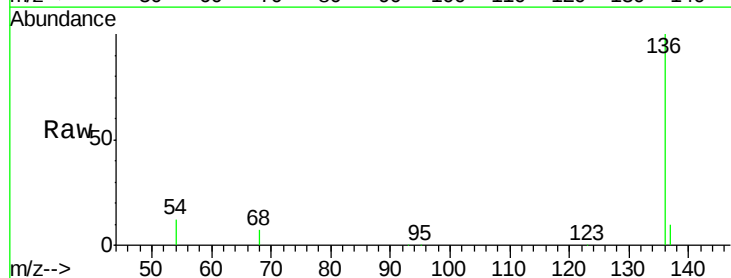

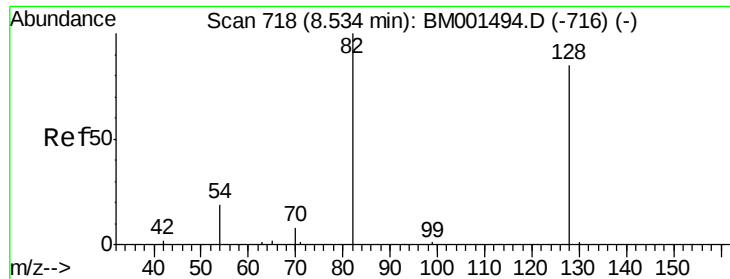

#7

Nitrobenzene-d5

Concen: 2.09 ng

RT: 8.53 min Scan# 718

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC002


Tgt Ion: 82 Resp: 5870

Ion Ratio Lower Upper

82 100

128 74.3 68.2 102.2

54 22.5 21.0 31.4



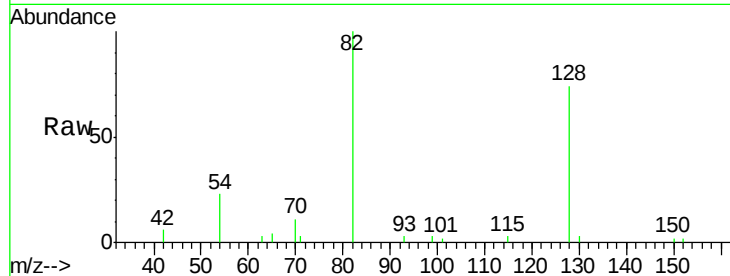


Abundance Ion 82.00 (81.70 to 82.70): BM001493.D (-714) (-)

Ion 128.00 (127.70 to 128.70): BM001493.D (-714) (-)

Ion 54.00 (53.70 to 54.70): BM001493.D (-714) (-)

Time-->

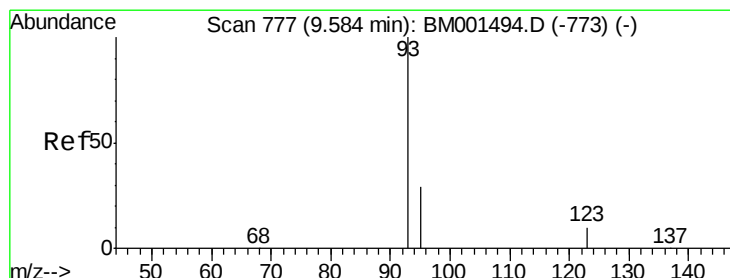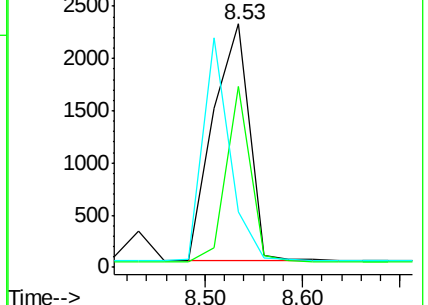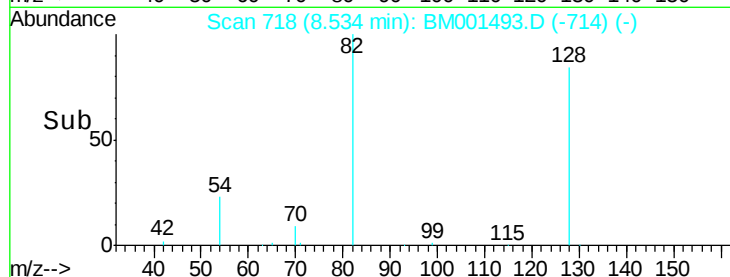

#8

bis(2-Chloroethoxy)methane

Concen: 2.55 ng

RT: 9.58 min Scan# 777

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18


Tgt Ion: 93 Resp: 7220

Ion Ratio Lower Upper

93 100

95 29.9 25.0 37.6

123 10.1 9.5 14.3


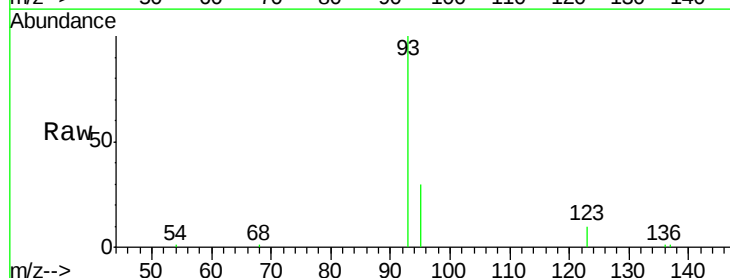



Abundance Ion 93.00 (92.70 to 93.70): BM001493.D (-769) (-)

Ion 95.00 (94.70 to 95.70): BM001493.D (-769) (-)

Ion 123.00 (122.70 to 123.70): BM001493.D (-769) (-)

Time-->

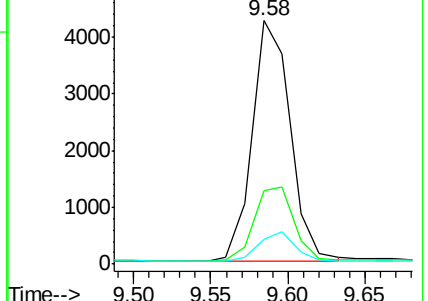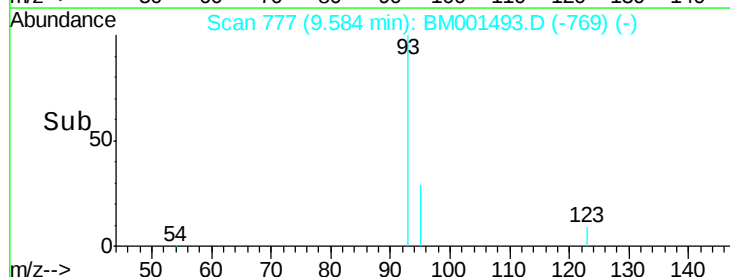

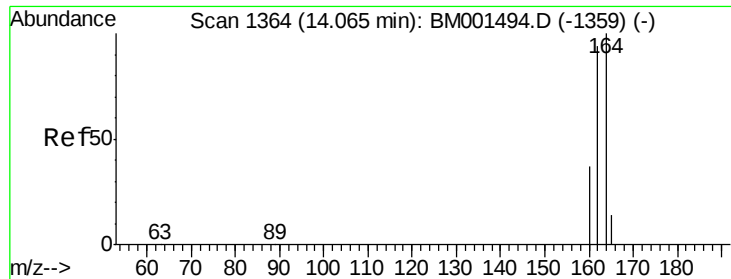

#9

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.07 min Scan# 1364

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC002


Tgt Ion:164 Resp: 26664

Ion Ratio Lower Upper

164 100

162 94.5 75.3 112.9




160 38.1 30.1 45.1

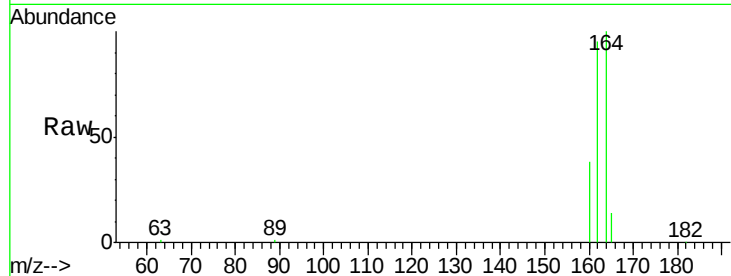

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

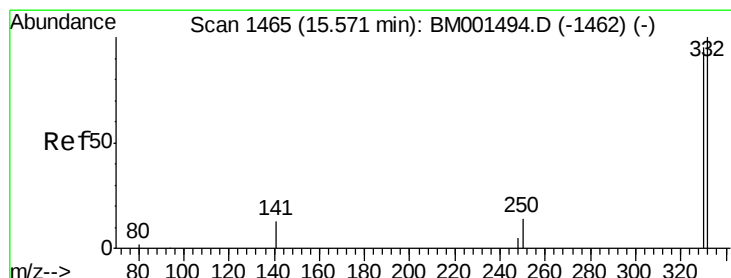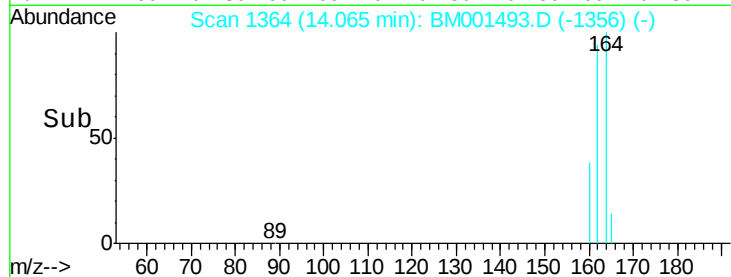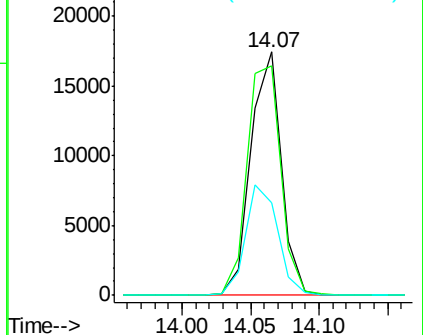

#10

2,4,6-Tribromophenol

Concen: 2.37 ng

RT: 15.57 min Scan# 1465

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18


Tgt Ion:330 Resp: 1966

Ion Ratio Lower Upper

330 100

332 98.0 77.6 116.4



141 44.1 34.3 51.5

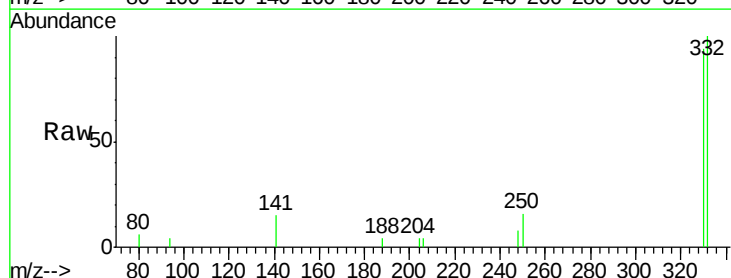


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

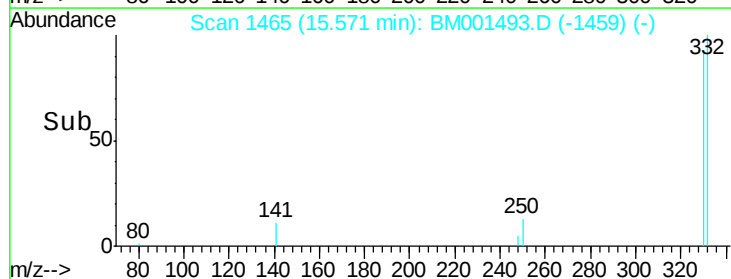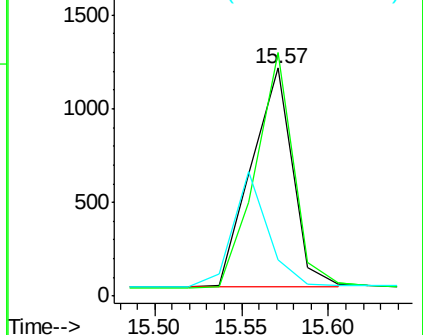

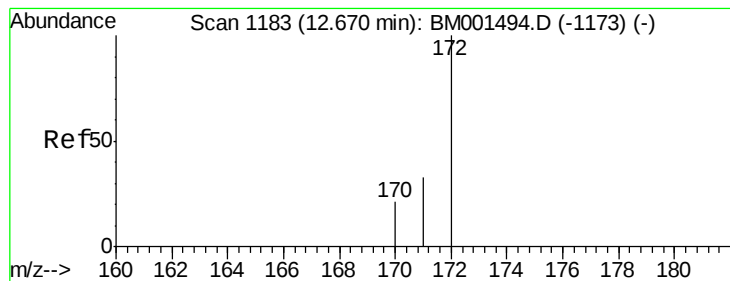

#11

2-Fluorobiphenyl

Concen: 2.14 ng

RT: 12.67 min Scan# 1183

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC002


Tgt Ion:172 Resp: 16097

Ion Ratio Lower Upper

172 100

171 34.0 27.2 40.8




170 22.2 17.8 26.6

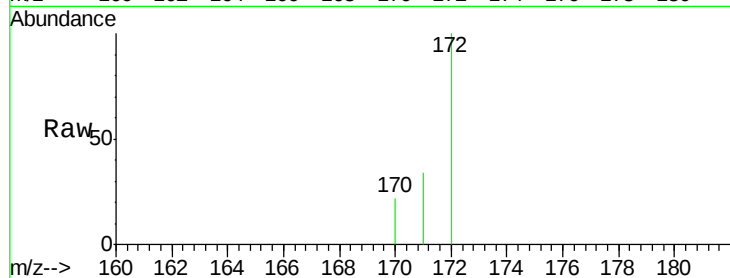

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

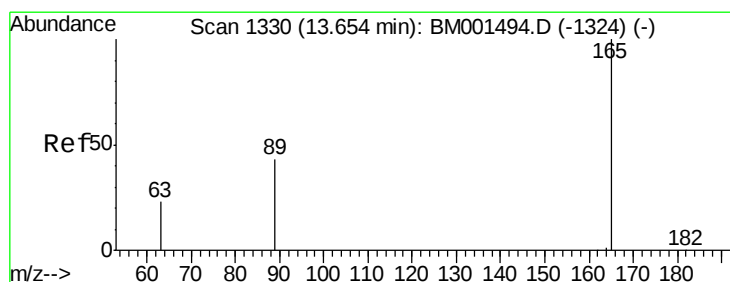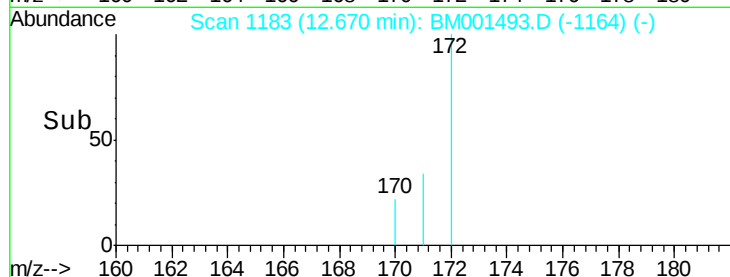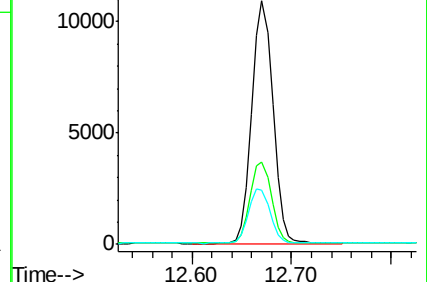

#12

2,6-Dinitrotoluene

Concen: 2.52 ng

RT: 13.65 min Scan# 1330

Delta R.T. -0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18


Tgt Ion:165 Resp: 2880

Ion Ratio Lower Upper

165 100

63 40.1 35.3 52.9



89 42.3 37.4 56.2

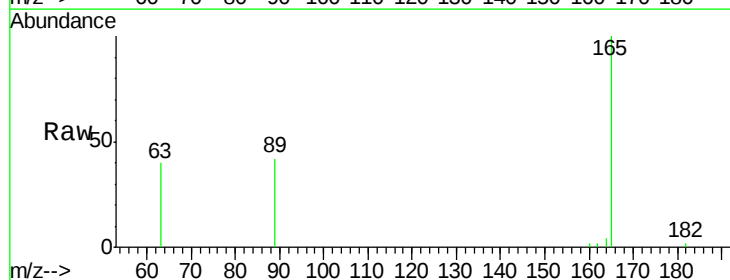


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 89.00 (88.70 to 89.70): BM0



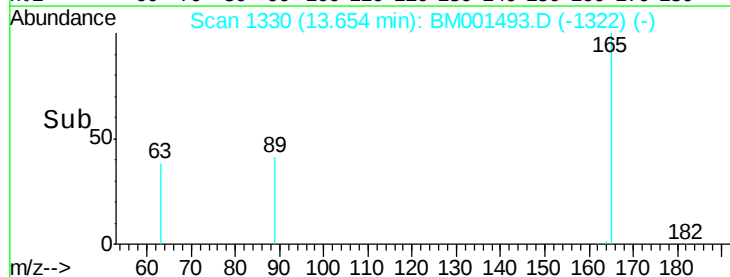
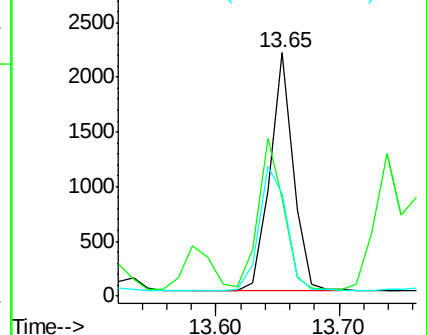


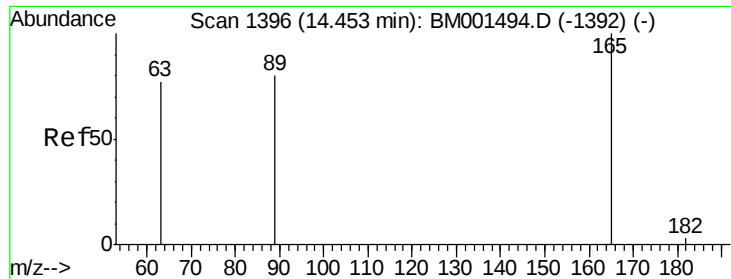

#13
 2,4-Dinitrotoluene
 Concen: 2.53 ng
 RT: 14.45 min Scan# 1396
 Delta R.T. -0.00 min
 Lab File: BM001493.D
 Acq: 31 May 2015 03:18




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC002


Tgt Ion:165 Resp: 3338
 Ion Ratio Lower Upper
 165 100
 63 62.3 63.9 95.9#
 89 65.4 65.0 97.6
 182 4.6 6.2 9.4#

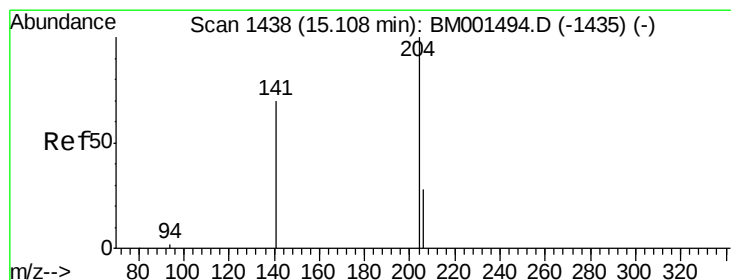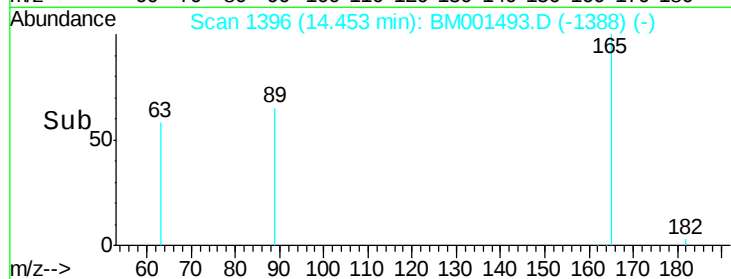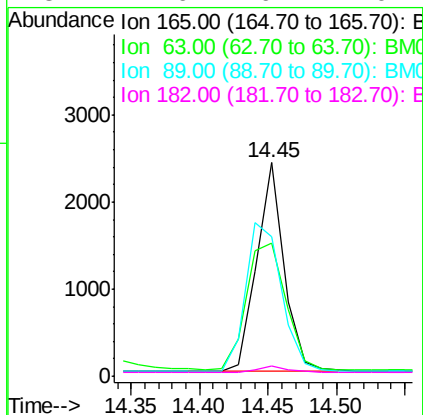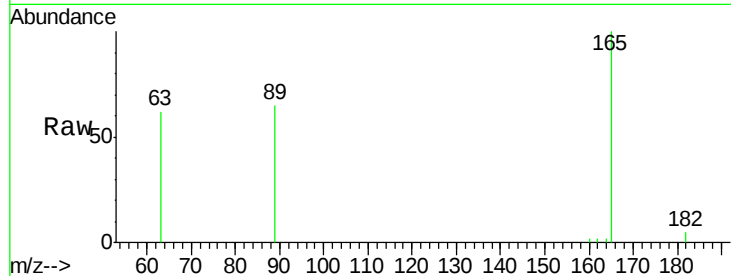

#14
 4-Chlorophenyl-phenylether
 Concen: 1.94 ng
 RT: 15.11 min Scan# 1438
 Delta R.T. -0.00 min
 Lab File: BM001493.D
 Acq: 31 May 2015 03:18

Tgt Ion:204 Resp: 7809
 Ion Ratio Lower Upper
 204 100
 206 27.7 23.8 35.6
 141 73.0 56.6 85.0


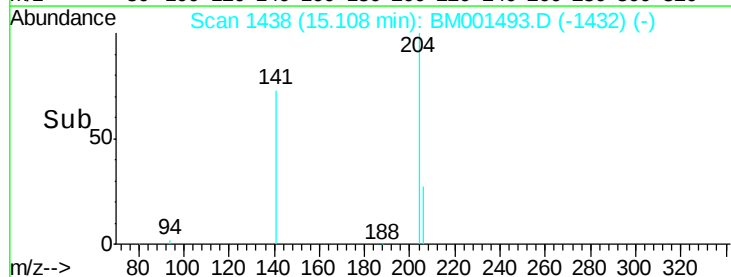
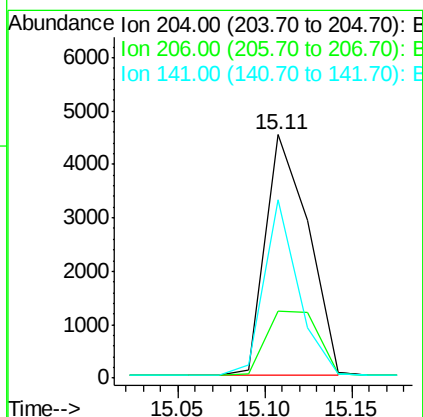
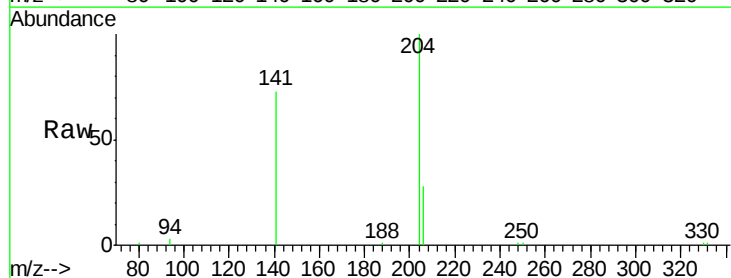


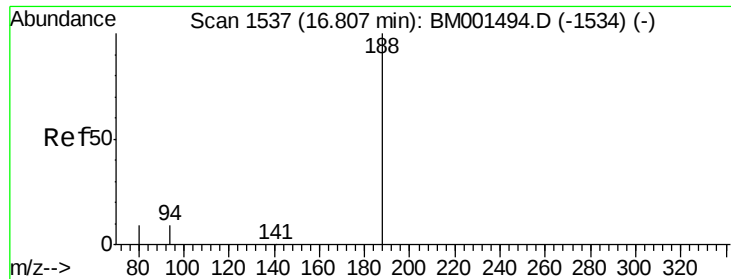

#15
Phenanthrene-d10
Concen: 5.00 ng
RT: 16.81 min Scan# 1537
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18




Instrument :
BNA_M
ClientSampleId :
SSTDICC002


Tgt Ion:188 Resp: 52770
Ion Ratio Lower Upper
188 100
94 9.2 7.1 10.7
80 9.5 7.3 10.9

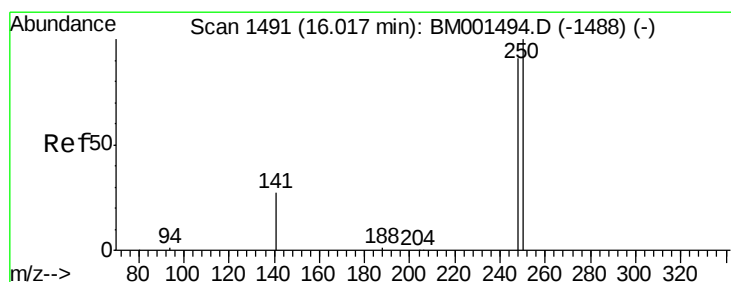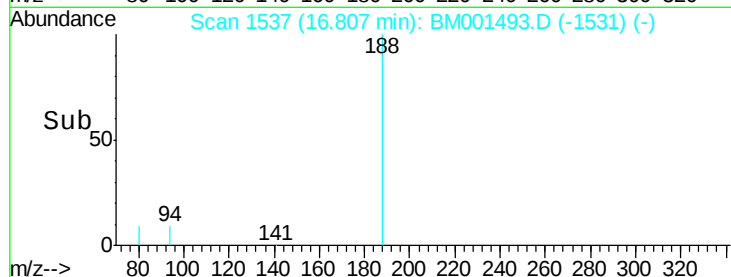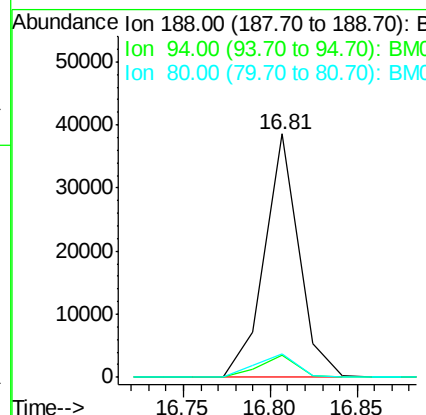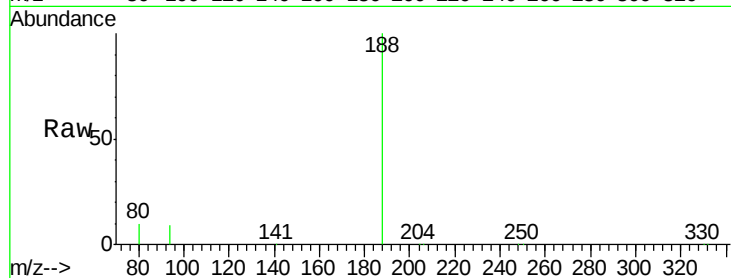

#16
4-Bromophenyl-phenylether
Concen: 2.16 ng
RT: 16.02 min Scan# 1491
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18

Tgt Ion:248 Resp: 4478
Ion Ratio Lower Upper
248 100
250 111.6 87.3 130.9
141 29.9 25.8 38.8


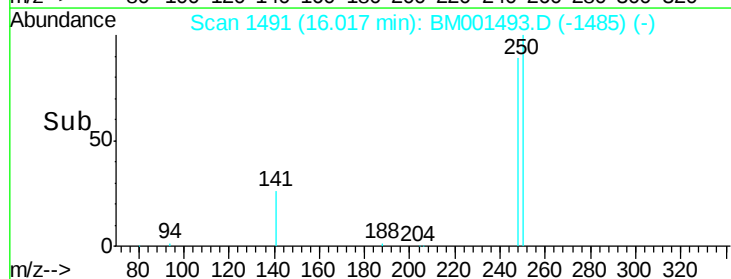
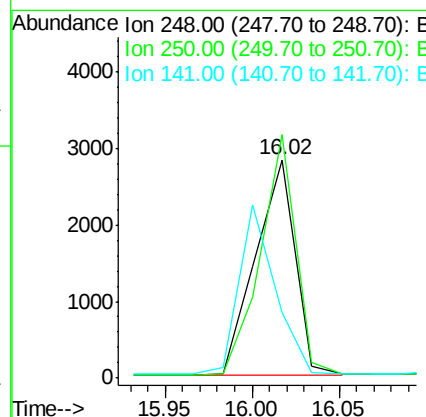
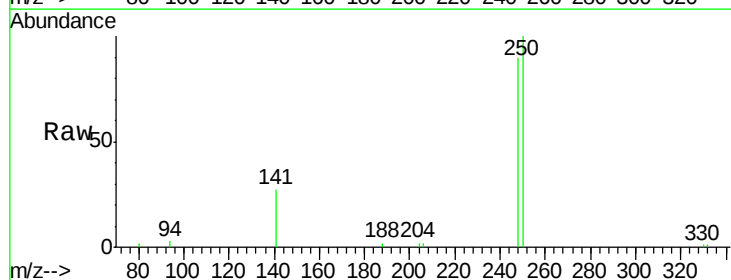


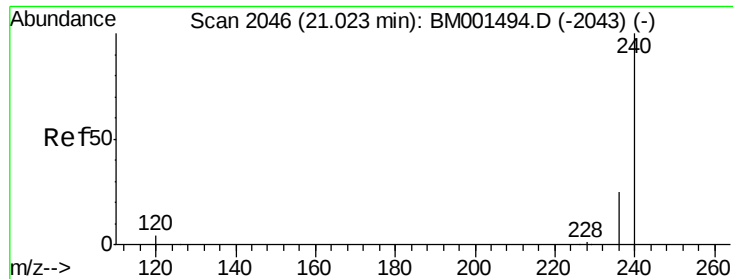

#17
Chrysene-d12
Concen: 5.00 ng
RT: 21.03 min Scan# 2049
Delta R.T. 0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18




Instrument :
BNA_M
ClientSampleId :
SSTDICC002


Tgt Ion:240 Resp: 42254
Ion Ratio Lower Upper
240 100
120 2.6 3.7 5.5#
236 22.8 19.8 29.8

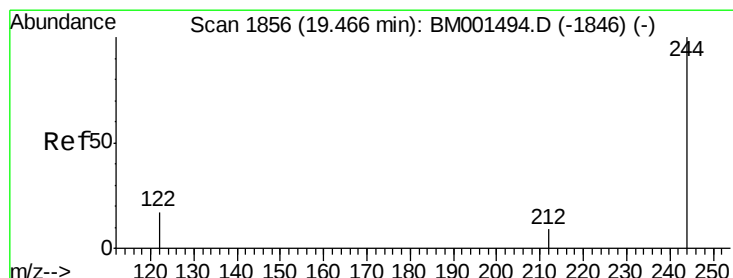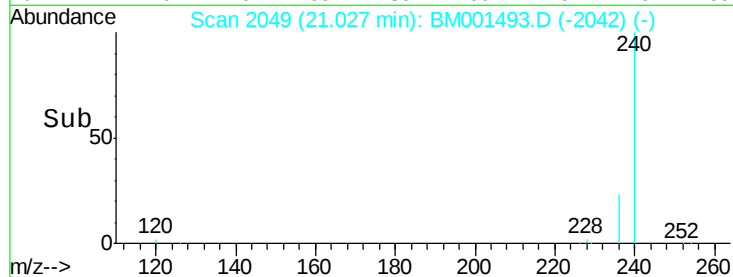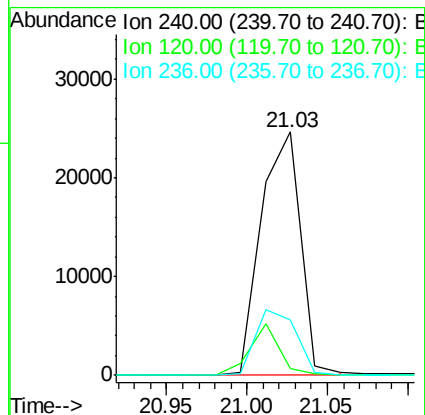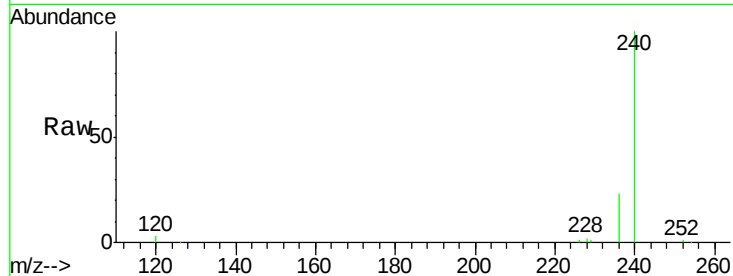

#18
Terphenyl-d14
Concen: 2.22 ng
RT: 19.46 min Scan# 1858
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18

Tgt Ion:244 Resp: 11742
Ion Ratio Lower Upper
244 100
212 9.9 8.0 12.0
122 18.4 14.1 21.1

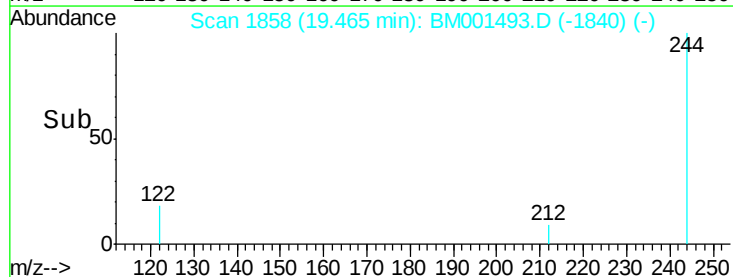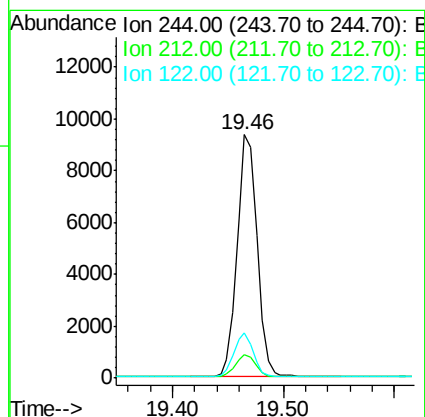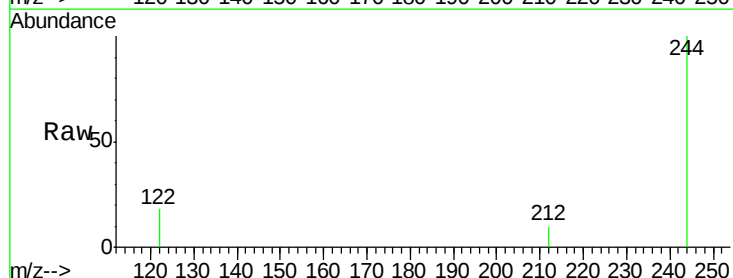

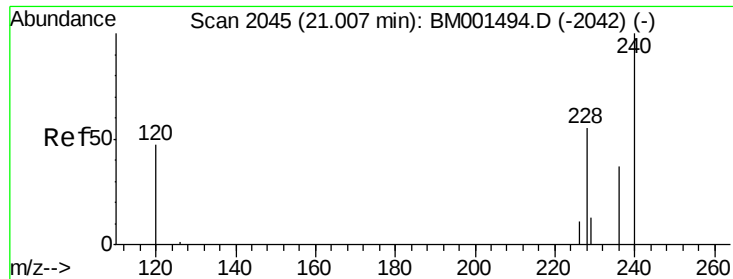

#19

Benzo(a)anthracene

Concen: 8.74 ng

RT: 21.00 min Scan# 2047

Delta R.T. -0.01 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC002


Tgt Ion:228 Resp: 23230

Ion Ratio Lower Upper

228 100

226 29.6 17.5 26.3#




229 17.1 19.0 28.4#

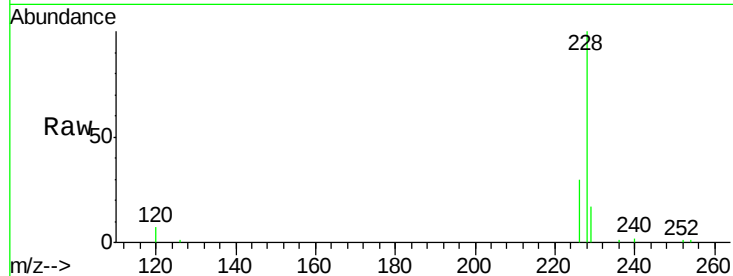

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

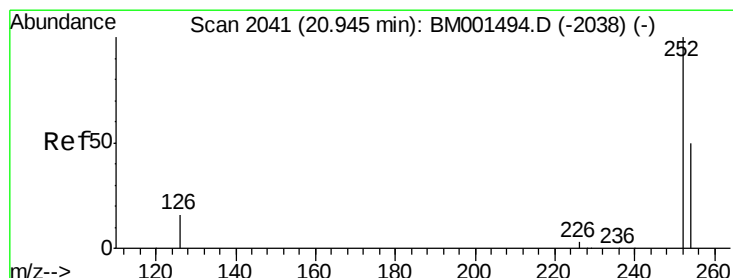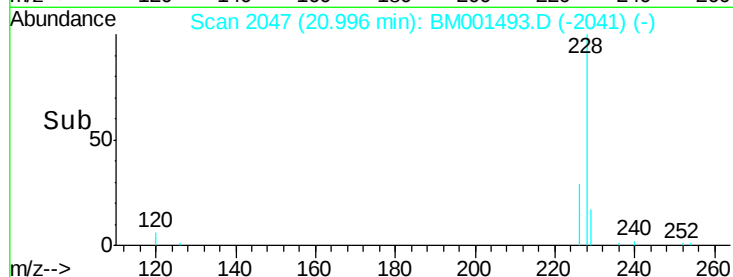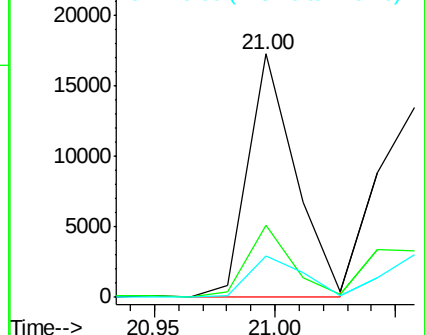

#20

3,3'-Dichlorobenzidine

Concen: 2.87 ng

RT: 20.95 min Scan# 2044

Delta R.T. 0.00 min

Lab File: BM001493.D

Acq: 31 May 2015 03:18


Tgt Ion:252 Resp: 8039

Ion Ratio Lower Upper

252 100

254 60.1 41.2 61.8



126 8.7 14.7 22.1#

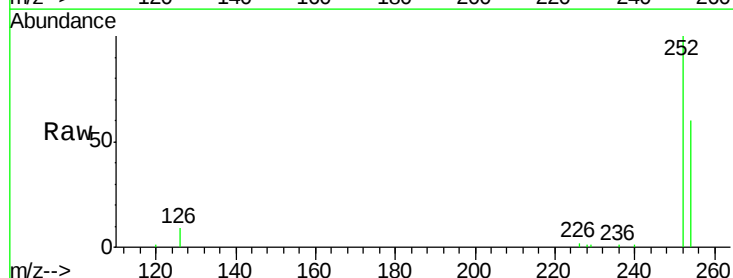


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

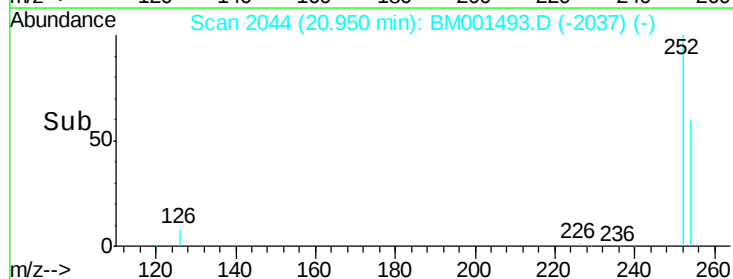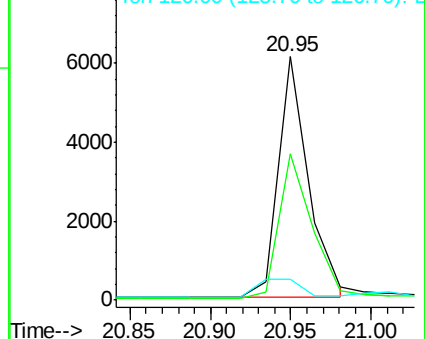

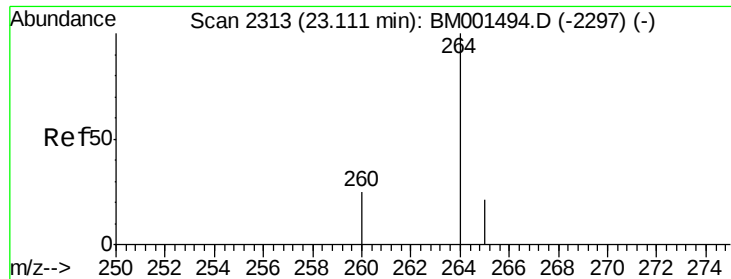

#21
Perylene-d12
Concen: 5.00 ng
RT: 23.11 min Scan# 2317
Delta R.T. -0.00 min
Lab File: BM001493.D
Acq: 31 May 2015 03:18

Instrument :
BNA_M
ClientSampleId :
SSTDICC002

Tgt Ion: 264 Resp: 36741
Ion Ratio Lower Upper
264 100
260 25.2 19.8 29.8
265 21.9 18.0 27.0

