


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM053115\
 Data File : BM001490.D
 Acq On : 31 May 2015 01:29
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM053115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun May 31 07:43:08 2015

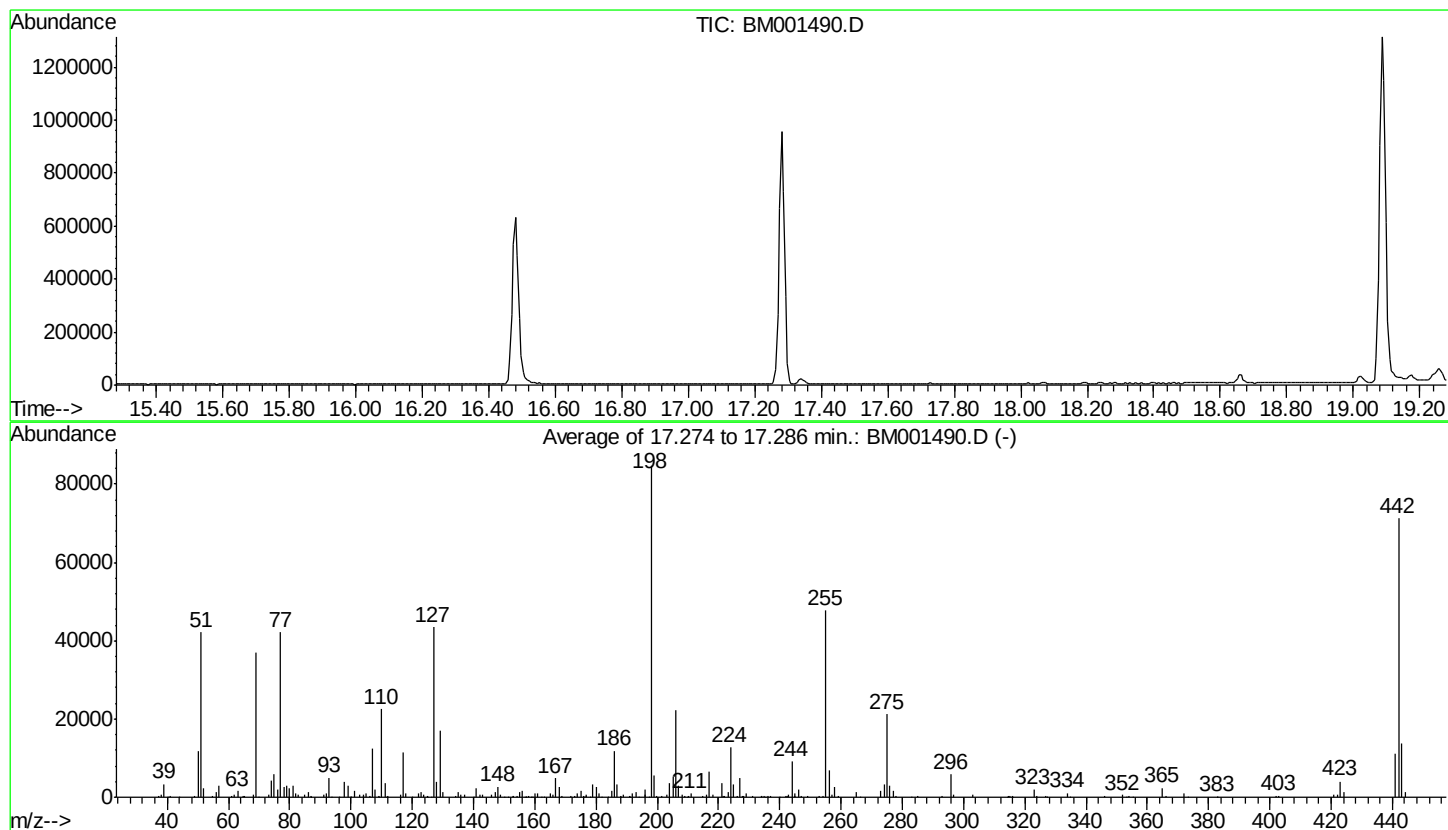

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	42149	PASS
68	69	0.00	2	2.0	754	PASS
69	198	0.00	100	43.5	36888	PASS
70	69	0.00	2	0.4	152	PASS
127	198	10	80	51.3	43442	PASS
197	198	0.00	2	0.2	160	PASS
198	198	100	100	100.0	84736	PASS
199	198	5	9	6.6	5581	PASS
275	198	10	60	25.0	21224	PASS
365	198	1	100	2.7	2318	PASS
441	442	0.01	24	15.6	11152	PASS
442	198	50	100	84.1	71290	PASS
443	442	15	24	19.2	13672	PASS