

Data File : BM010333.D
Acq On : 31 May 2017 15:56
Operator : SJ/MA
Sample : PB99357BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Time: Jun 01 00:58:49 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 01 00:58:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	293764	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	1065076	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	659687	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1522785	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	1950161	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2139769	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	44227	6.18	ng/uL	0.00
5) Phenol-d5	7.11	99	685358	30.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	402500	32.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	583414	32.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	533722	29.72	ng/ul	0.00
19) Nitrobenzene-d5	9.11	128	256054	32.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	306587	33.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	596544	32.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	685865	38.29	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1952995	35.63	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	2169184	33.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	220115	26.84	ng/ul	0.00
57) Fluorene-d10	15.55	176	1609245	33.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	299184	27.74	ng/ul	0.00
70) Anthracene-d10	17.40	188	2578615	34.80	ng/ul	0.00
76) Pyrene-d10	19.69	212	3004772	37.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	3465732	34.79	ng/ul	0.00

Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.64	70	18648	1.27 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010333.D

Acq On : 31 May 2017 15:56

Operator : SJ/MA

Sample : PB99357BL

Misc :

ALS Vial : 7 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SBLK57


Quant Time: Jun 01 00:58:49 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Jun 01 00:58:21 2017

Response via : Initial Calibration

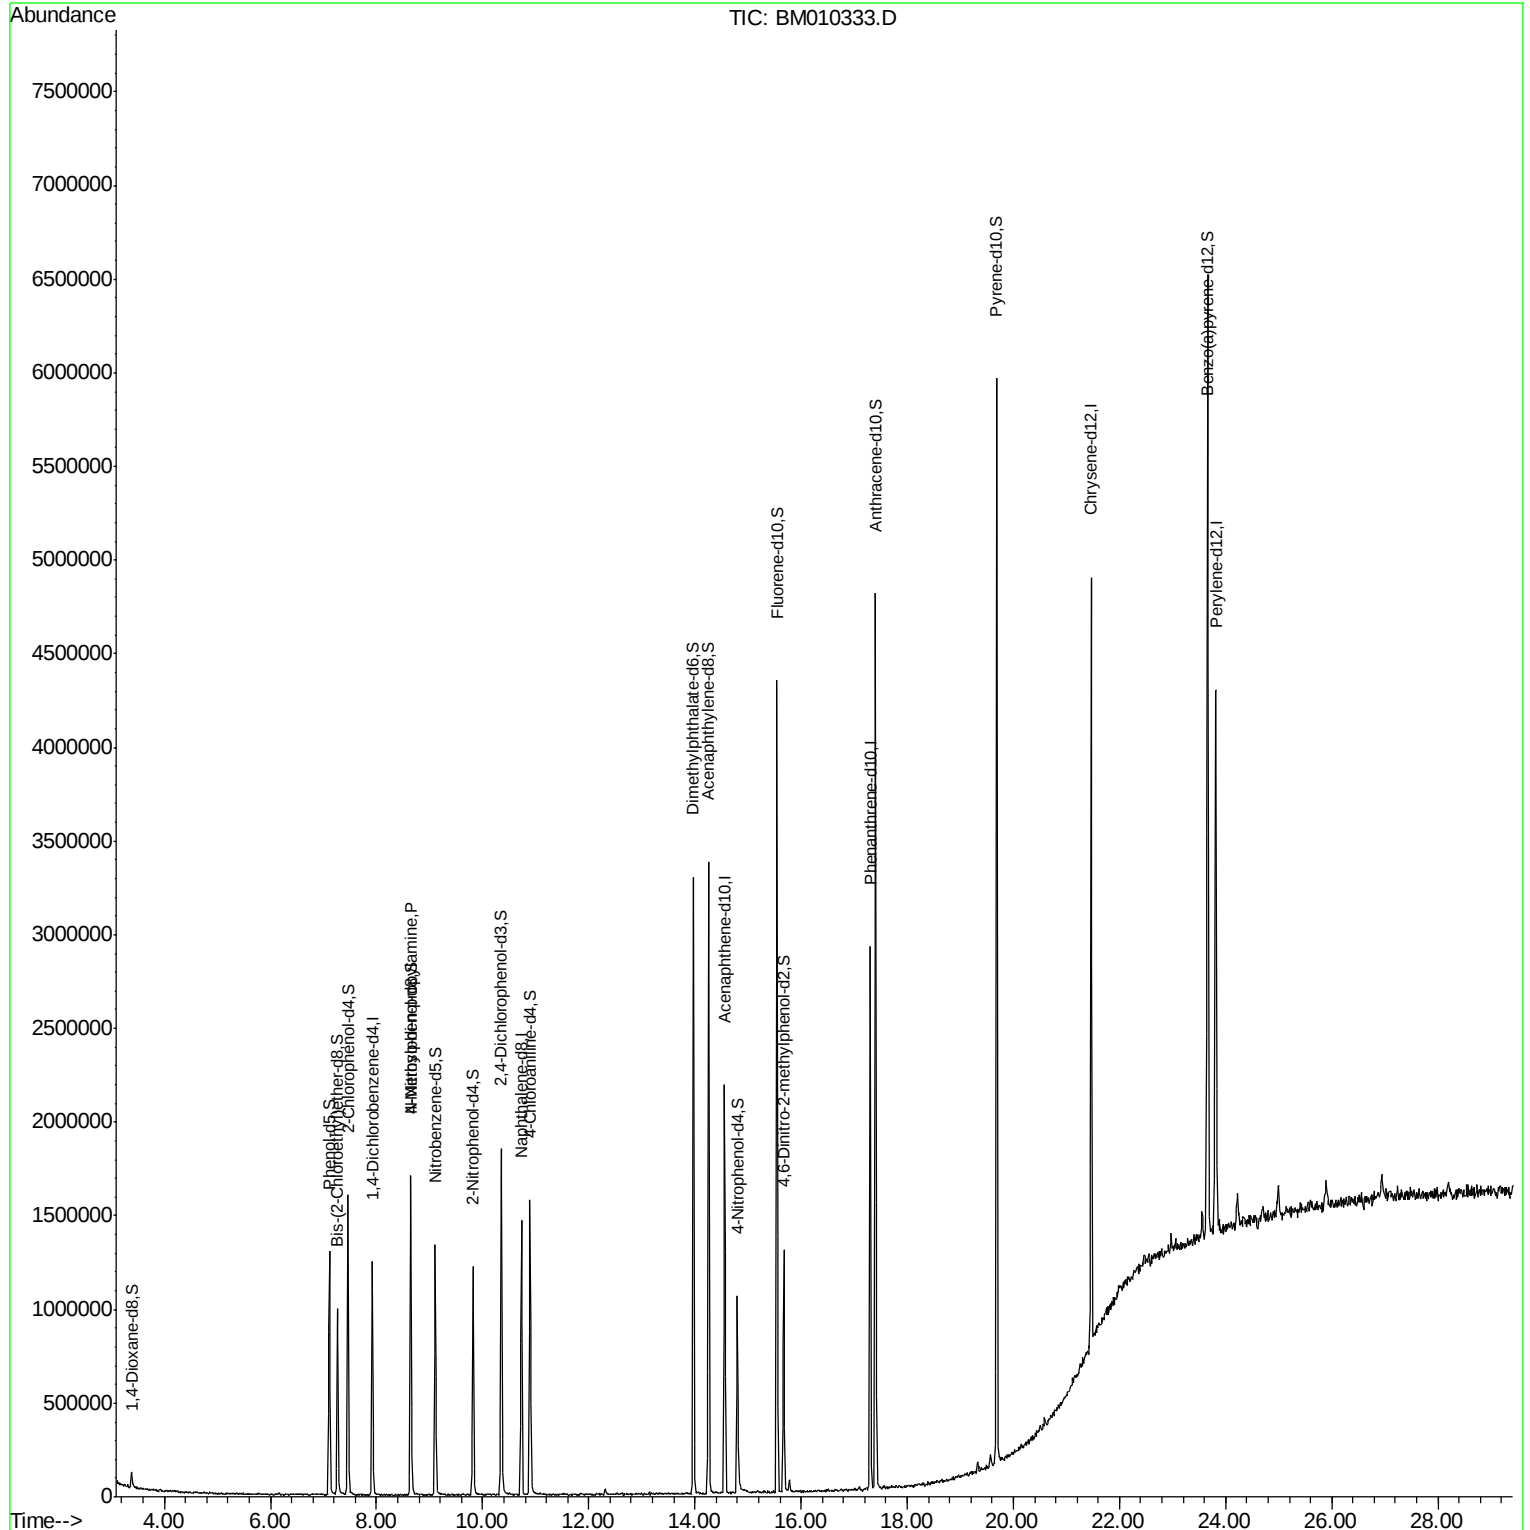

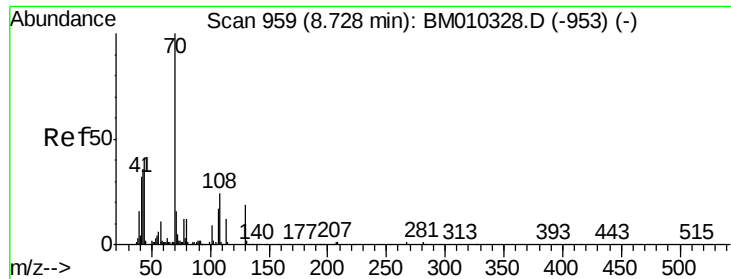

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.27 ng/ul
 RT: 8.64 min Scan# 944
 Delta R.T. -0.09 min
 Lab File: BM010333.D
 Acq: 31 May 2017 15:56

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Tgt Ion: 70 Resp: 18648
 Ion Ratio Lower Upper
 70 100
 42 223.4 41.1 61.7#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

