
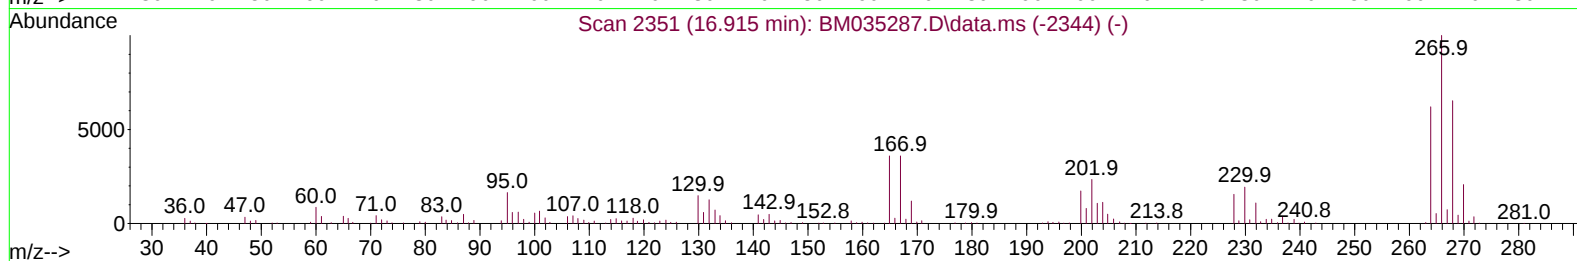
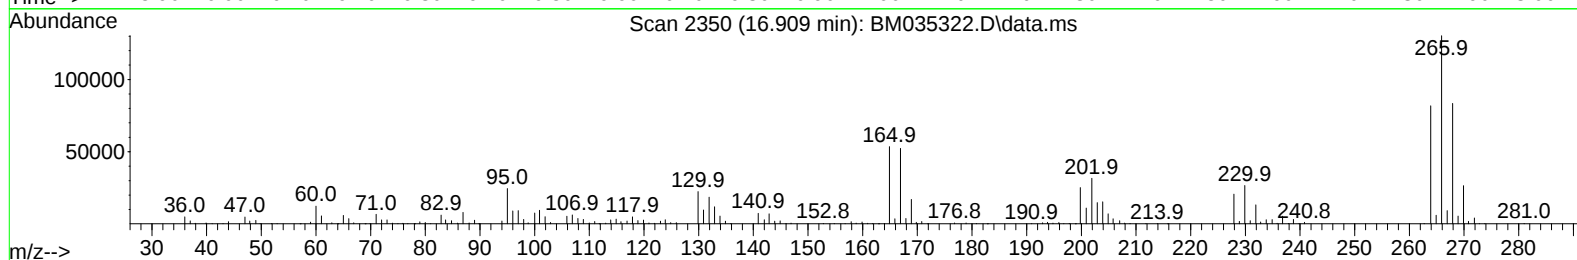


Quant Time: May 31 15:47:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 15:35:47 2022
Response via : Initial Calibration

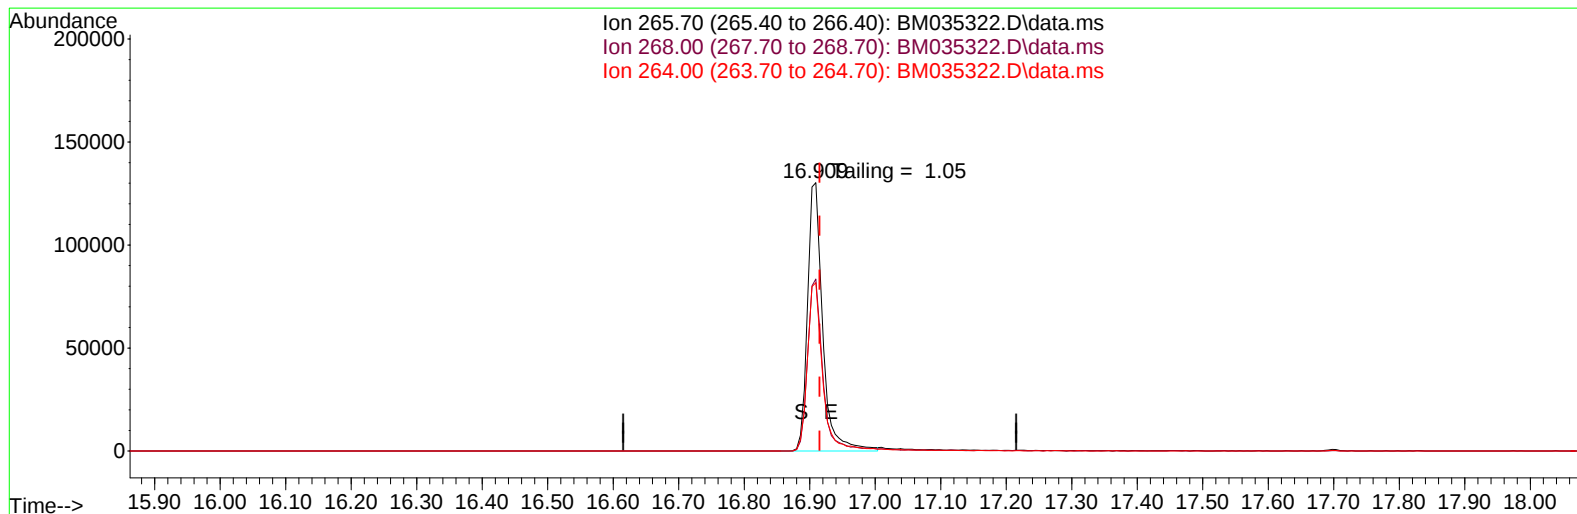

TIC: BM035322.D\data.ms

(70) Pentachlorophenol (C)




16.909min (-0.006) 0.00 ng

response **213342**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.07
264.00	63.30	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
 Data File : BM035322.D
 Acq On : 31 May 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 15:47:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 15:35:47 2022
 Response via : Initial Calibration

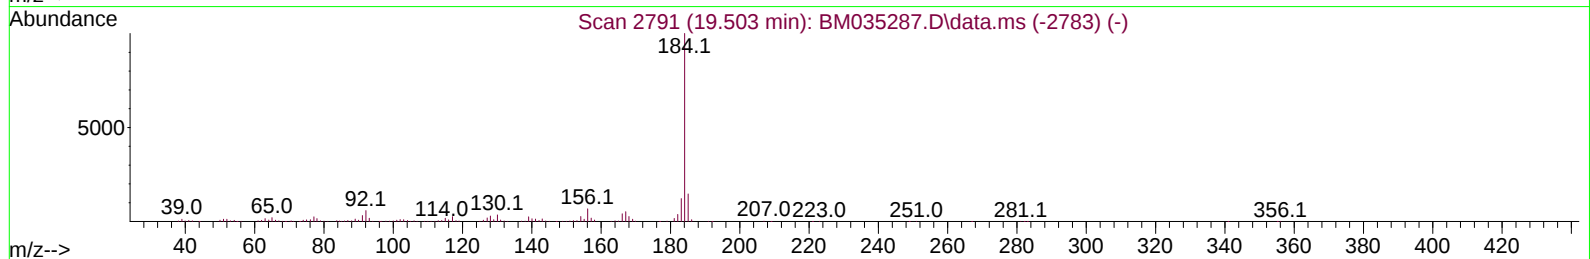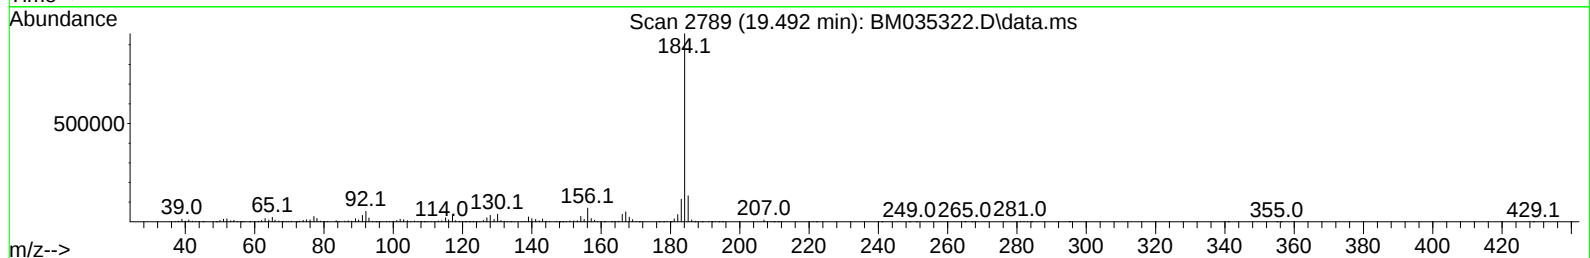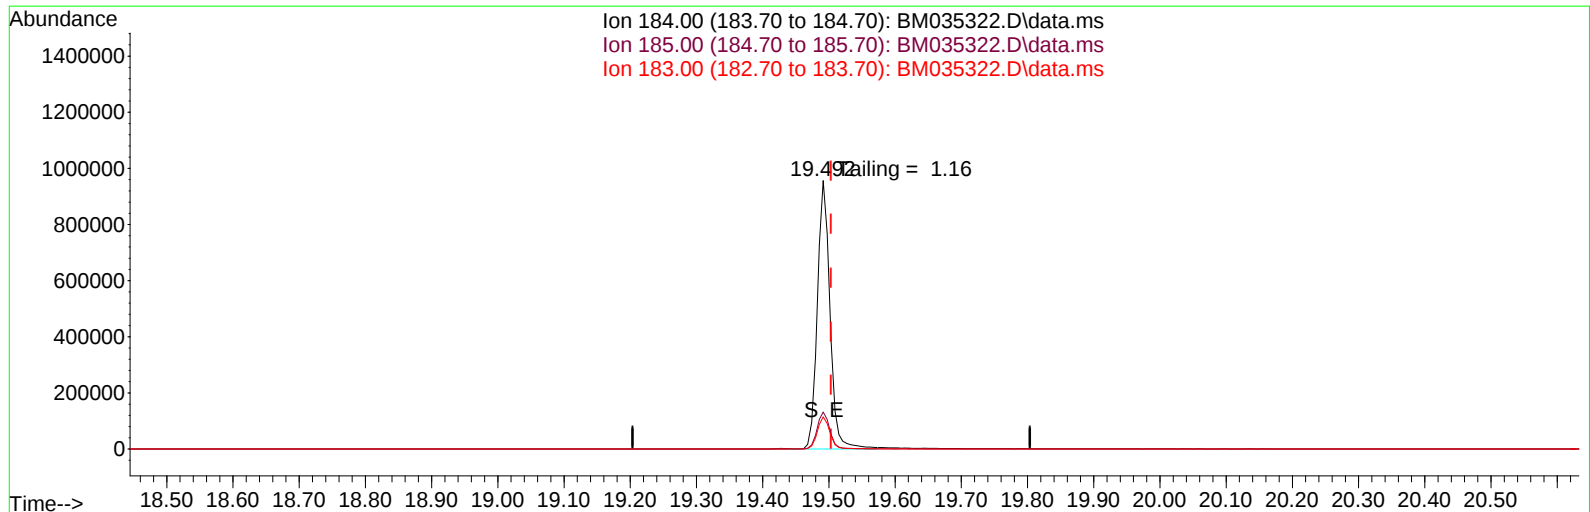

TIC: BM035322.D\data.ms

(77) Benzidine

19.492min (-0.012) 1167048.77 ng

response 1276602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.78
183.00	11.90	12.01
0.00	0.00	0.00