

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
 Data File : BM035324.D
 Acq On : 31 May 2022 12:21
 Operator : CG/JU
 Sample : PB145186BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145186BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	422	rBV	2391044	3456480	48.94%	10.543%
2	7.046	666	673	688	rBV	2155369	3468457	49.11%	10.579%
3	7.869	806	813	820	rBV	434874	712604	10.09%	2.174%
4	9.028	1001	1010	1032	rBV	1384167	2292701	32.46%	6.993%
5	10.669	1281	1289	1304	rBV	528579	948979	13.44%	2.894%
6	13.133	1701	1708	1721	rBV	3881859	5699523	80.69%	17.384%
7	14.504	1935	1941	1955	rBV	853624	1255528	17.78%	3.830%
8	15.998	2188	2195	2219	rBV	2719125	3988297	56.47%	12.165%
9	17.251	2401	2408	2422	rBV	943036	1392260	19.71%	4.247%
10	19.874	2848	2854	2865	rBV	5539317	7063209	100.00%	21.544%
11	21.433	3114	3119	3125	rBV	1016034	1289627	18.26%	3.934%
12	23.797	3515	3521	3531	rVB2	597730	1218024	17.24%	3.715%




Sum of corrected areas: 32785689

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035324.D
Acq On : 31 May 2022 12:21
Operator : CG/JU
Sample : PB145186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145186BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

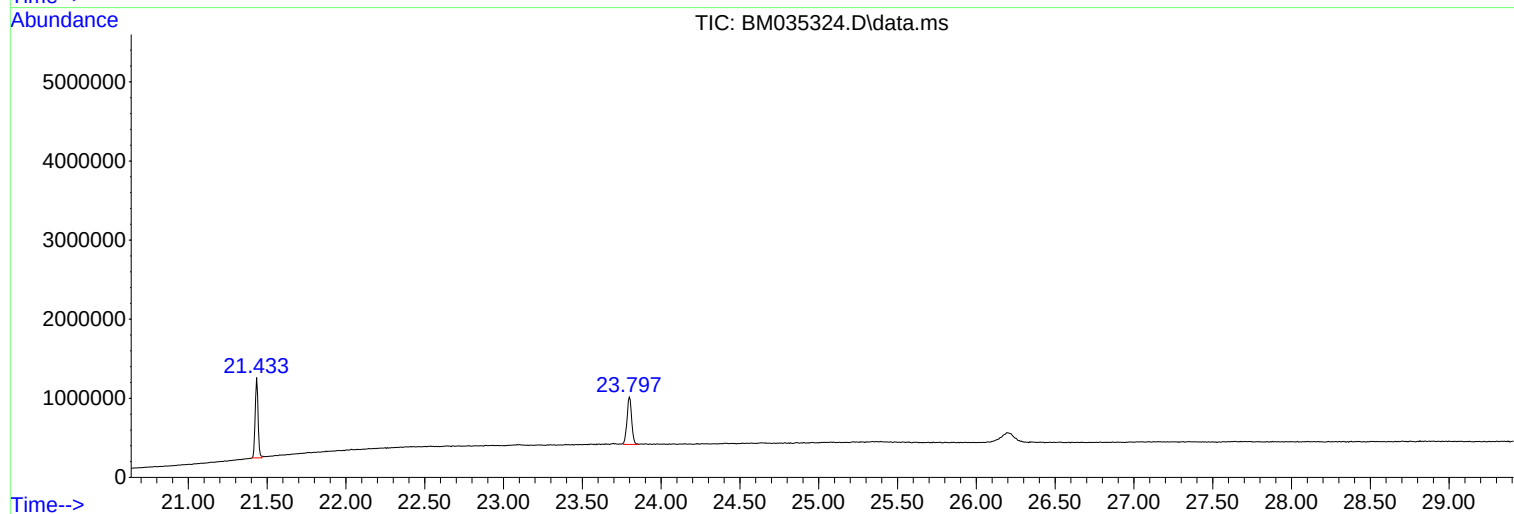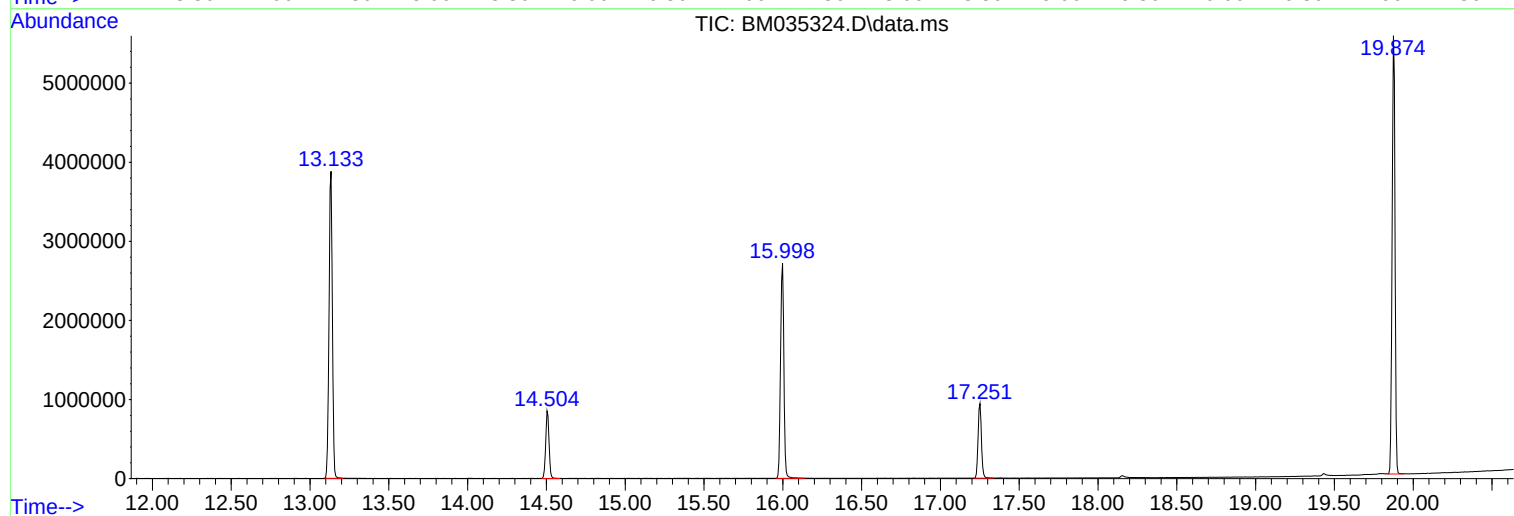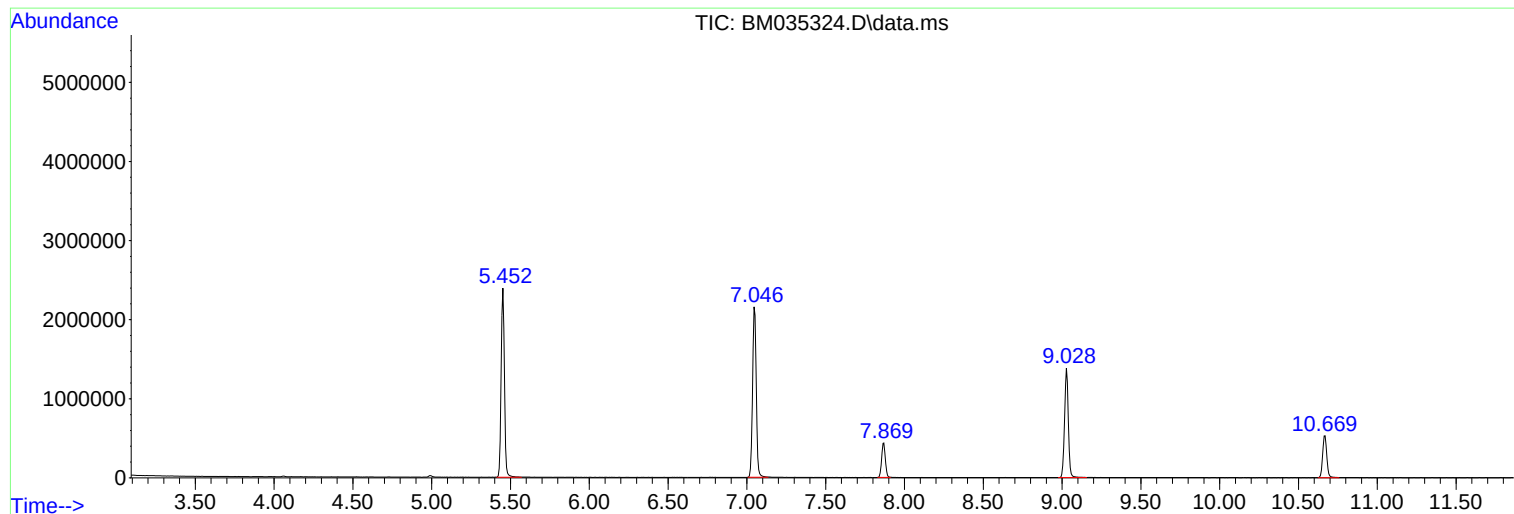

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035324.D
Acq On : 31 May 2022 12:21
Operator : CG/JU
Sample : PB145186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145186BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035324.D
Acq On : 31 May 2022 12:21
Operator : CG/JU
Sample : PB145186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145186BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------