

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
 Data File : BM035338.D
 Acq On : 31 May 2022 22:53
 Operator : CG/JU
 Sample : N2952-07 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P037-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	397	403	414	rBV	115024	192594	8.89%	1.711%
2	7.051	667	674	685	rBV	98520	190162	8.78%	1.689%
3	7.869	805	813	824	rBV	535836	885720	40.88%	7.869%
4	9.028	1004	1010	1022	rBV	63159	127605	5.89%	1.134%
5	10.669	1280	1289	1302	rBV	656532	1153184	53.22%	10.245%
6	13.128	1699	1707	1716	rBV	217709	337320	15.57%	2.997%
7	14.504	1934	1941	1953	rBV	974132	1484970	68.53%	13.193%
8	14.933	2009	2014	2020	rBV5	14309	25921	1.20%	0.230%
9	15.998	2190	2195	2202	rBV	141583	217817	10.05%	1.935%
10	17.251	2401	2408	2415	rBV	1218506	1723538	79.55%	15.313%
11	18.151	2557	2561	2570	rBV2	78772	134510	6.21%	1.195%
12	19.427	2775	2778	2784	rBV4	50058	86191	3.98%	0.766%
13	19.874	2849	2854	2859	rBV	386286	500831	23.11%	4.450%
14	21.433	3114	3119	3124	rBV	1525602	2028646	93.63%	18.023%
15	23.797	3515	3521	3530	rVB2	1116011	2166736	100.00%	19.250%


Sum of corrected areas: 11255745

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035338.D
Acq On : 31 May 2022 22:53
Operator : CG/JU
Sample : N2952-07 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P037-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

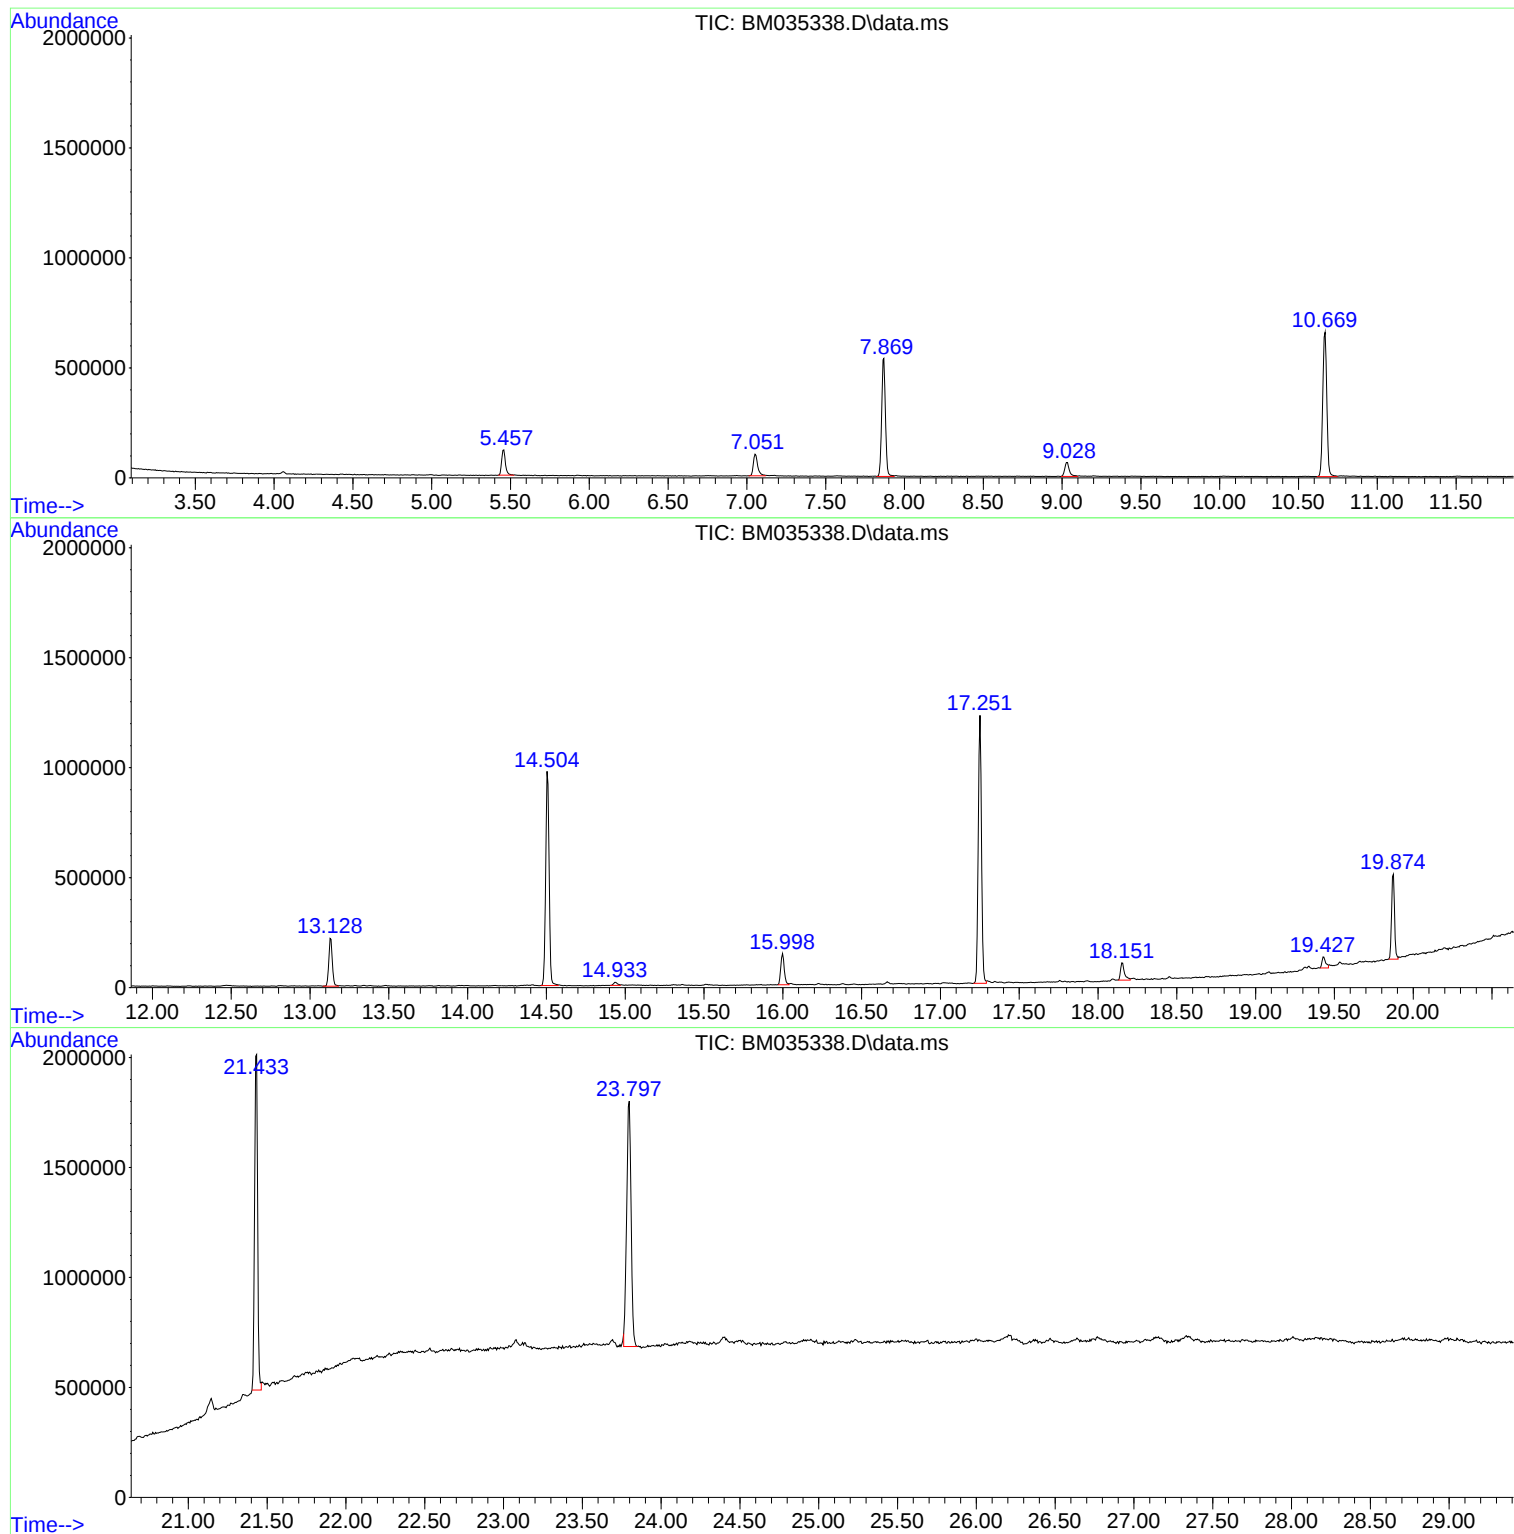

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035338.D
Acq On : 31 May 2022 22:53
Operator : CG/JU
Sample : N2952-07 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P037-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035338.D
Acq On : 31 May 2022 22:53
Operator : CG/JU
Sample : N2952-07 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P037-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------