
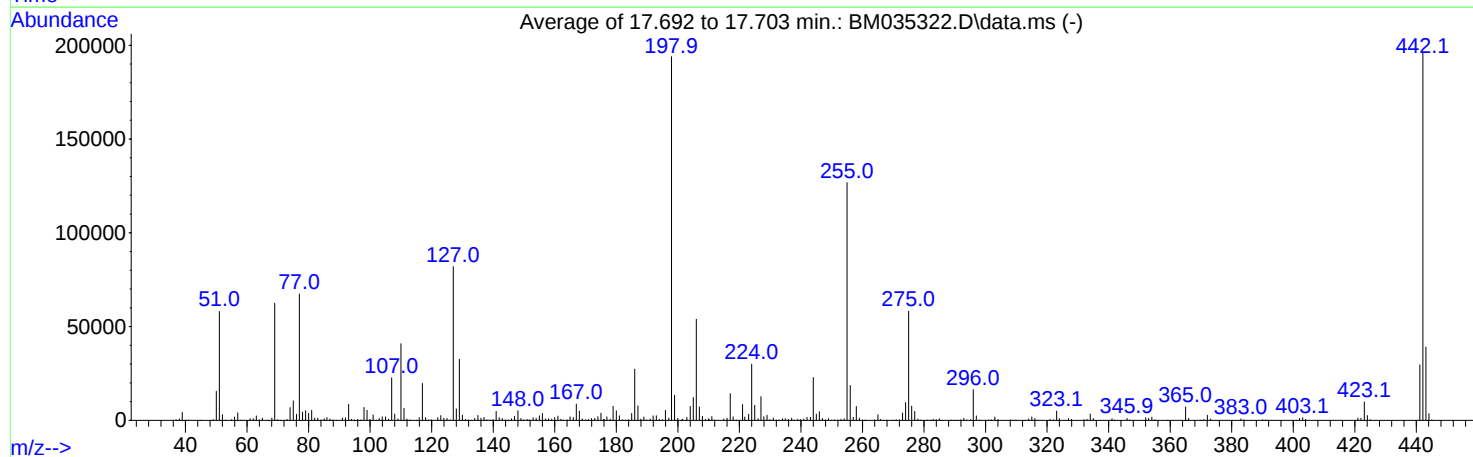


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
 Data File : BM035322.D
 Acq On : 31 May 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 31 15:35:47 2022

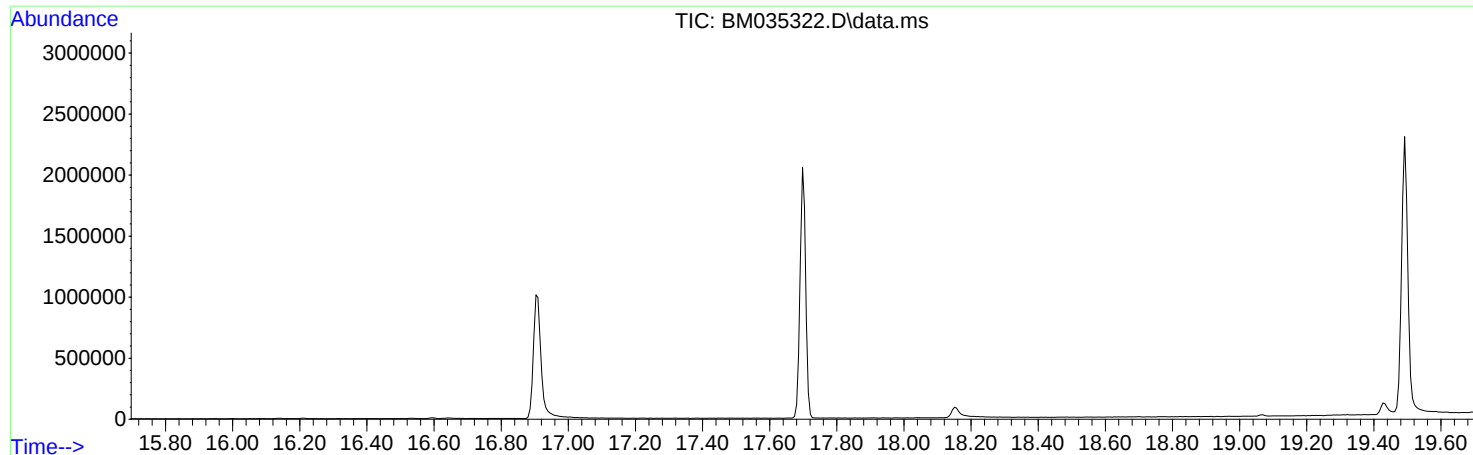




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	58123	PASS
68	69	0.00	2	1.9	1204	PASS
69	198	0.00	100	32.2	62416	PASS
70	69	0.00	2	0.5	317	PASS
127	198	10	80	42.3	82011	PASS
197	198	0.00	2	0.6	1176	PASS
198	198	100	100	100.0	193899	PASS
199	198	5	9	6.9	13388	PASS
275	198	10	60	30.0	58197	PASS
365	198	1	100	3.7	7080	PASS
441	198	0.01	100	15.3	29624	PASS
442	442	50	100	100.0	196133	PASS
443	442	15	24	19.9	39107	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\  
Data File : BM035322.D  
Acq On    : 31 May 2022  11:07  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 31 15:47:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue May 31 15:35:47 2022
Response via : Initial Calibration

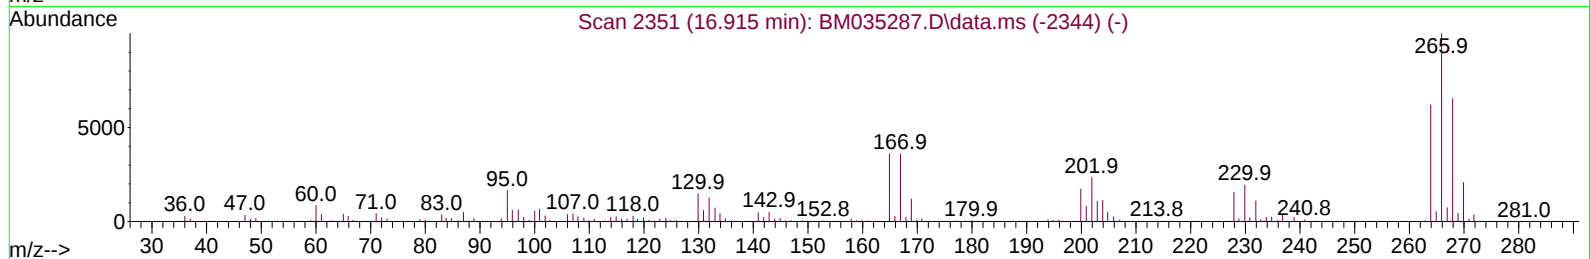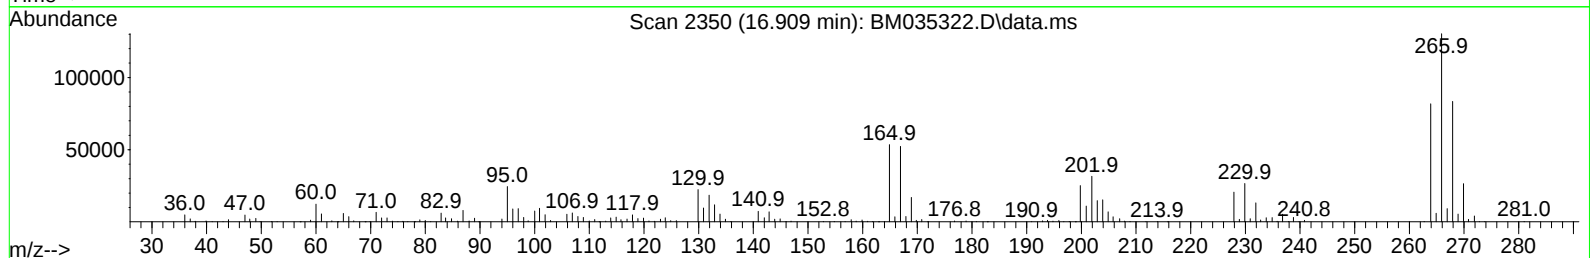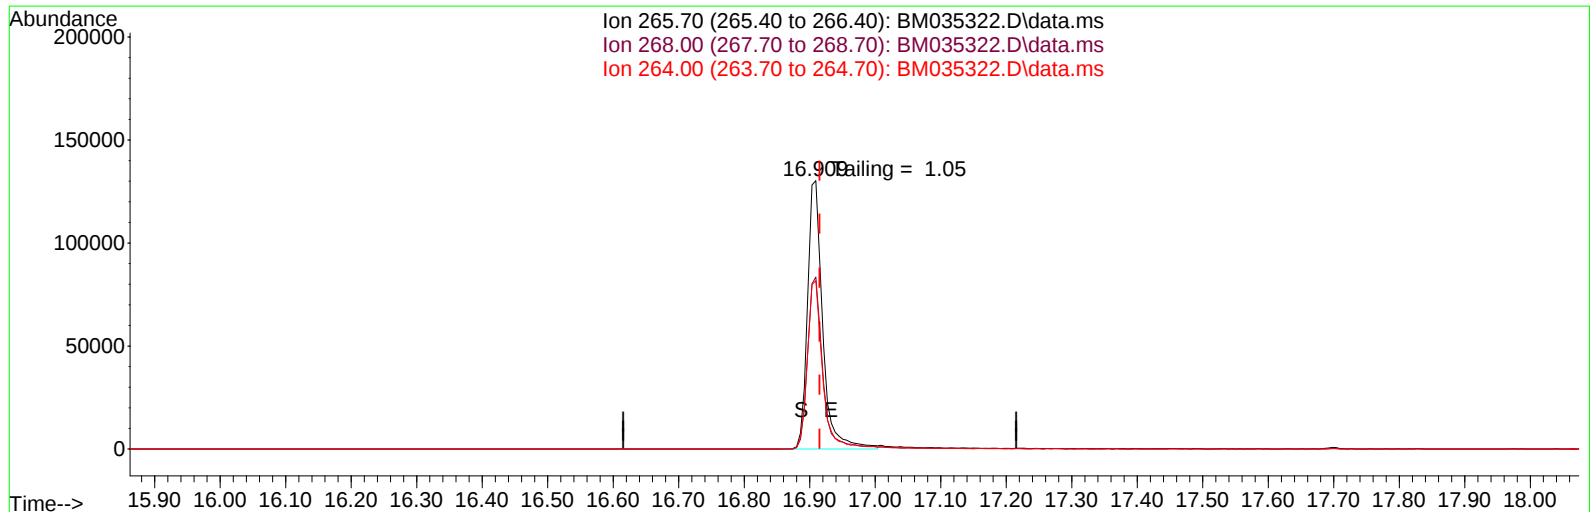

TIC: BM035322.D\data.ms

(70) Pentachlorophenol (C)

16.909min (-0.006) 0.00 ng




response 213342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.07
264.00	63.30	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053122\
Data File : BM035322.D
Acq On : 31 May 2022 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 31 15:47:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 15:35:47 2022
Response via : Initial Calibration

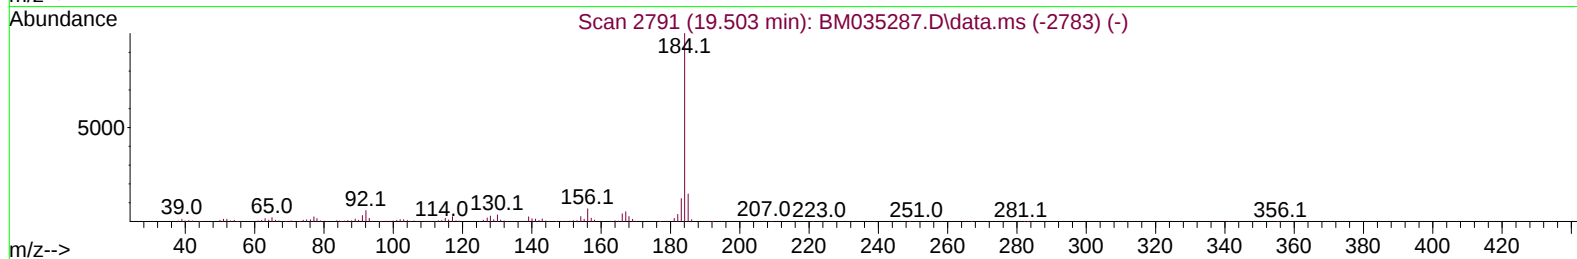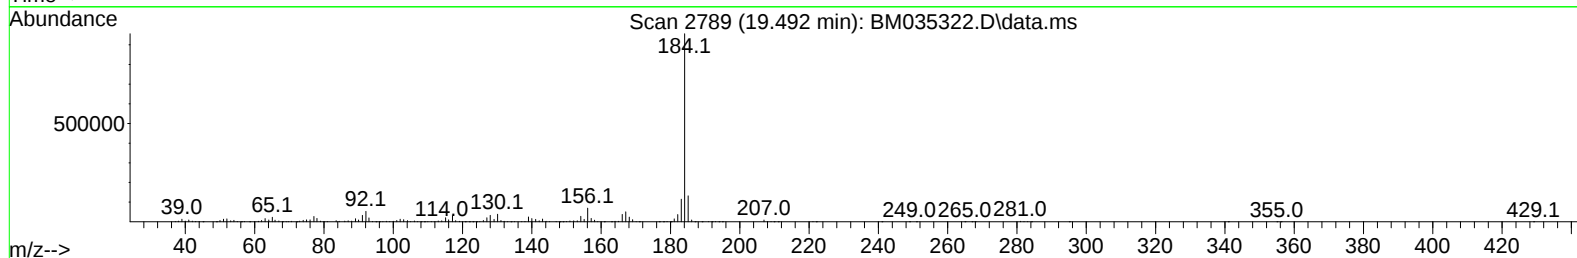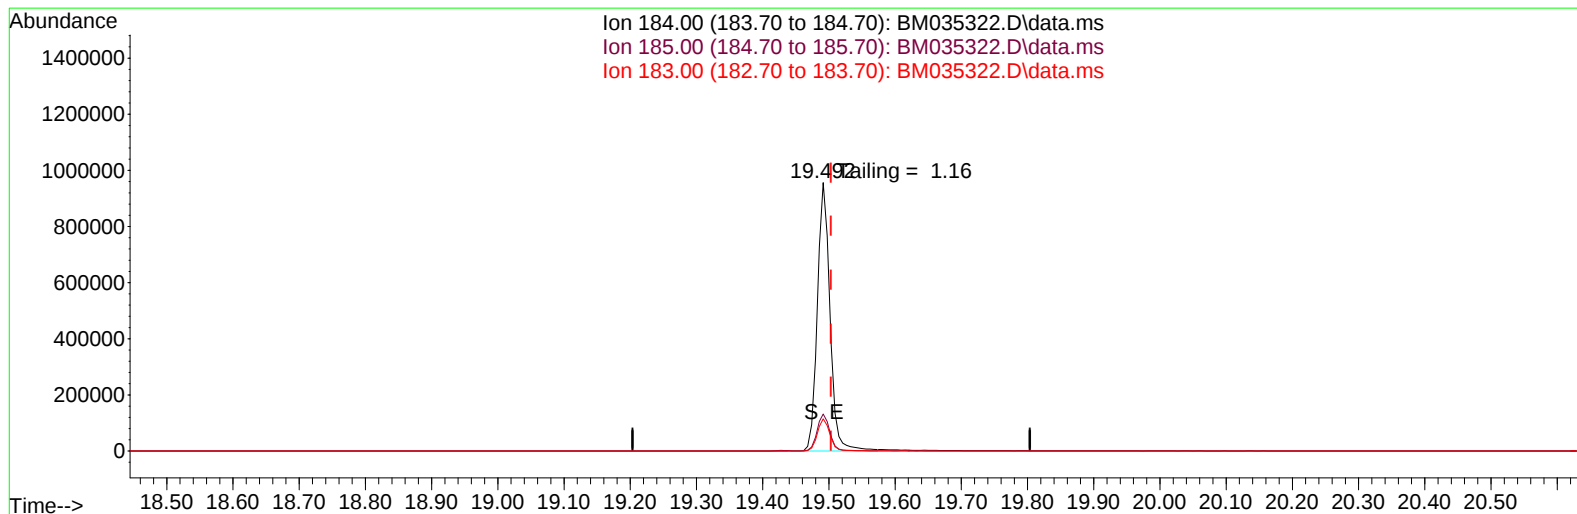

TIC: BM035322.D\data.ms

(77) Benzidine

19.492min (-0.012) 1167048.77 ng

response 1276602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.78
183.00	11.90	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/31/2022	BNA_M	<u>BM035322.D</u>
Compound Name	Response	Retention Time
DDT	709004	20.72
DDD	3739	20.29
DDE	860	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4599	713603	0.64

Instrument :
BNA_M
ClientSampleId :
DFTPP