

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
 Data File : BM040082.D
 Acq On : 31 May 2023 16:49
 Operator : CG/JU
 Sample : PB153107BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK107

Quant Time: Jun 01 00:19:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 31 18:20:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	5540	0.400	ng/ul	0.00
4) Naphthalene-d8	10.817	136	19314	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.637	164	9355	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	16389	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	9029	0.400	ng/ul	0.00
23) Perylene-d12	23.988	264	10591	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	47696	7.004	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.400	152	8343	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.398	212	10808	0.410	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.765	202	2868	0.073	ng/ul#	1
26) Benzo(a)pyrene	23.830	252	5690	0.157	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
Data File : BM040082.D
Acq On : 31 May 2023 16:49
Operator : CG/JU
Sample : PB153107BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK107

Quant Time: Jun 01 00:19:36 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 18:20:24 2023
Response via : Initial Calibration




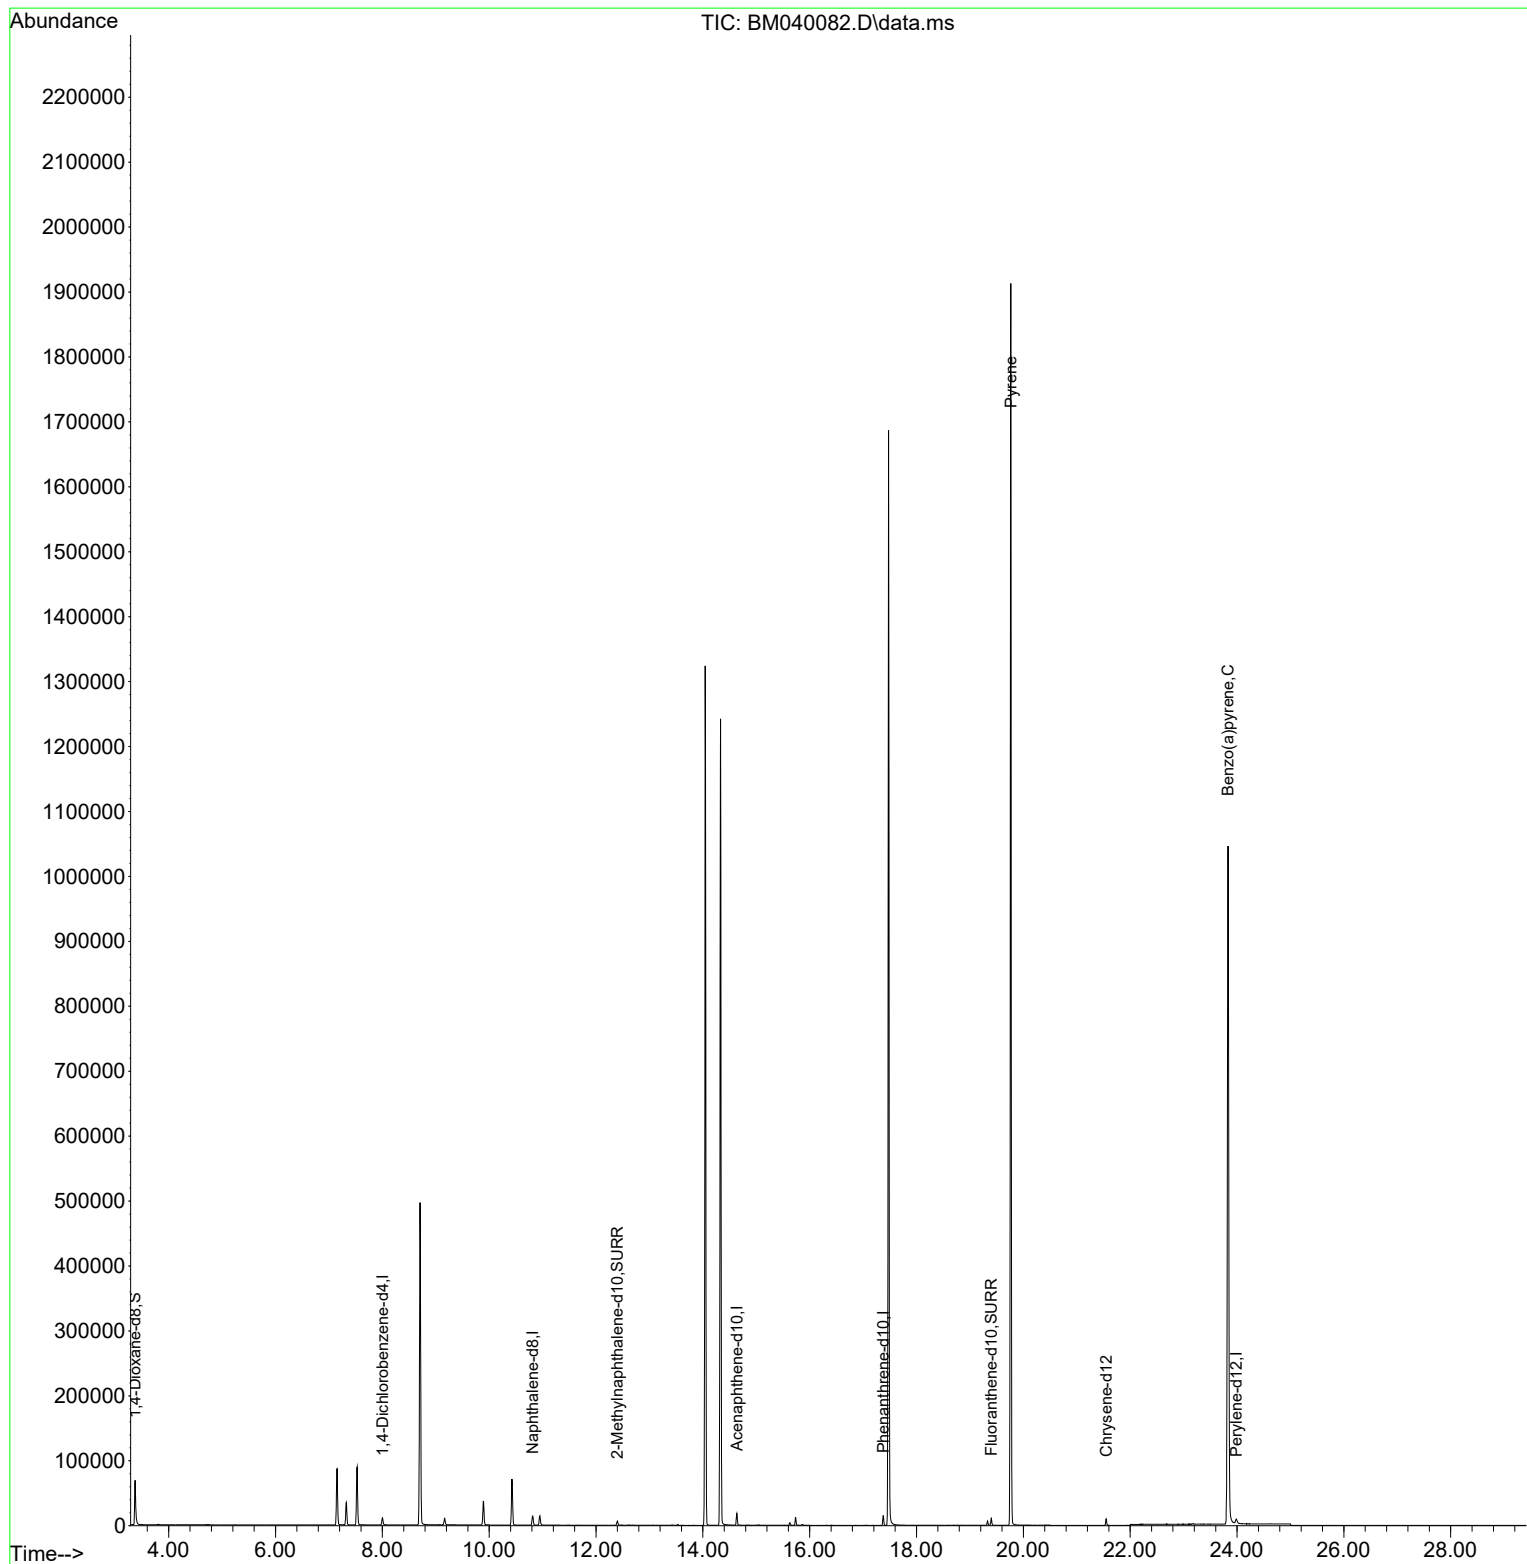


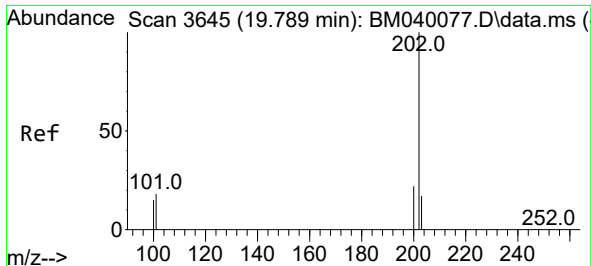

#20
Pyrene
Concen: 0.073 ng/ul
RT: 19.765 min Scan# 3640
Delta R.T. -0.023 min
Lab File: BM040082.D
Acq: 31 May 2023 16:49

Instrument :
BNA_M
ClientSampleId :
SBLK107

Tgt Ion:202 Resp: 2868
Ion Ratio Lower Upper
202 100
101 153.2 14.7 22.1#
100 1105.4 12.2 18.2#

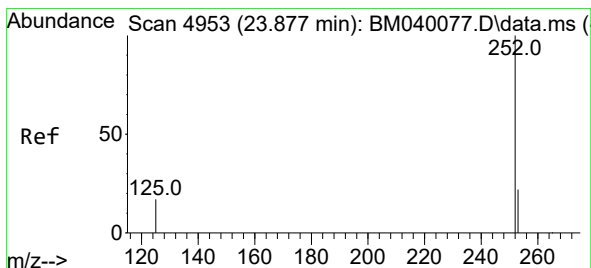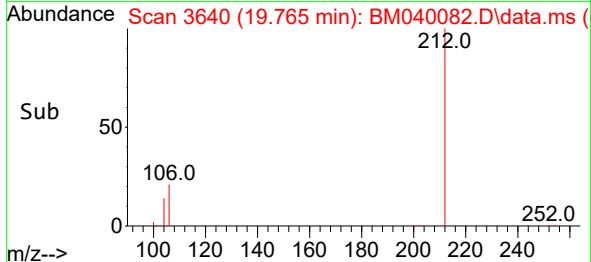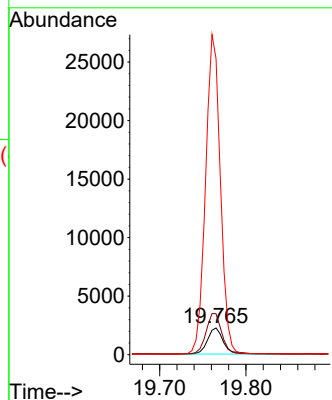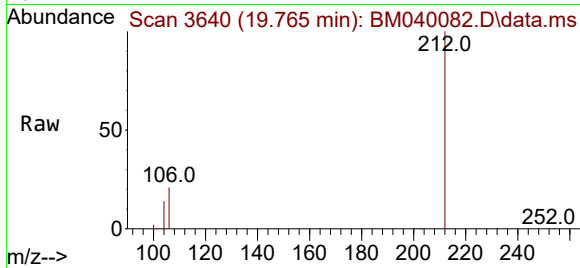

#26
Benzo(a)pyrene
Concen: 0.157 ng/ul
RT: 23.830 min Scan# 4937
Delta R.T. -0.047 min
Lab File: BM040082.D
Acq: 31 May 2023 16:49

Tgt Ion:252 Resp: 5690
Ion Ratio Lower Upper
252 100
253 38.7 21.0 31.4#
125 37.8 19.8 29.8#

