

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
 Data File : BM040090.D
 Acq On : 31 May 2023 21:43
 Operator : CG/JU
 Sample : 02961-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FP3RE

Quant Time: Jun 01 00:20:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 31 18:20:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	7124	0.400	ng/ul	0.00
4) Naphthalene-d8	10.811	136	25439	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.637	164	12673	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	22450	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	11946	0.400	ng/ul	0.00
23) Perylene-d12	23.985	264	12420	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	34827	3.977	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	9905	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.398	212	15735	0.451	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.627	166	4246	0.096	ng/ul#	12
16) Anthracene	17.476	178	1119	0.021	ng/ul#	1
20) Pyrene	19.765	202	3835	0.074	ng/ul#	1
26) Benzo(a)pyrene	23.830	252	6440	0.151	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
Data File : BM040090.D
Acq On : 31 May 2023 21:43
Operator : CG/JU
Sample : 02961-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FP3RE

Quant Time: Jun 01 00:20:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 18:20:24 2023
Response via : Initial Calibration




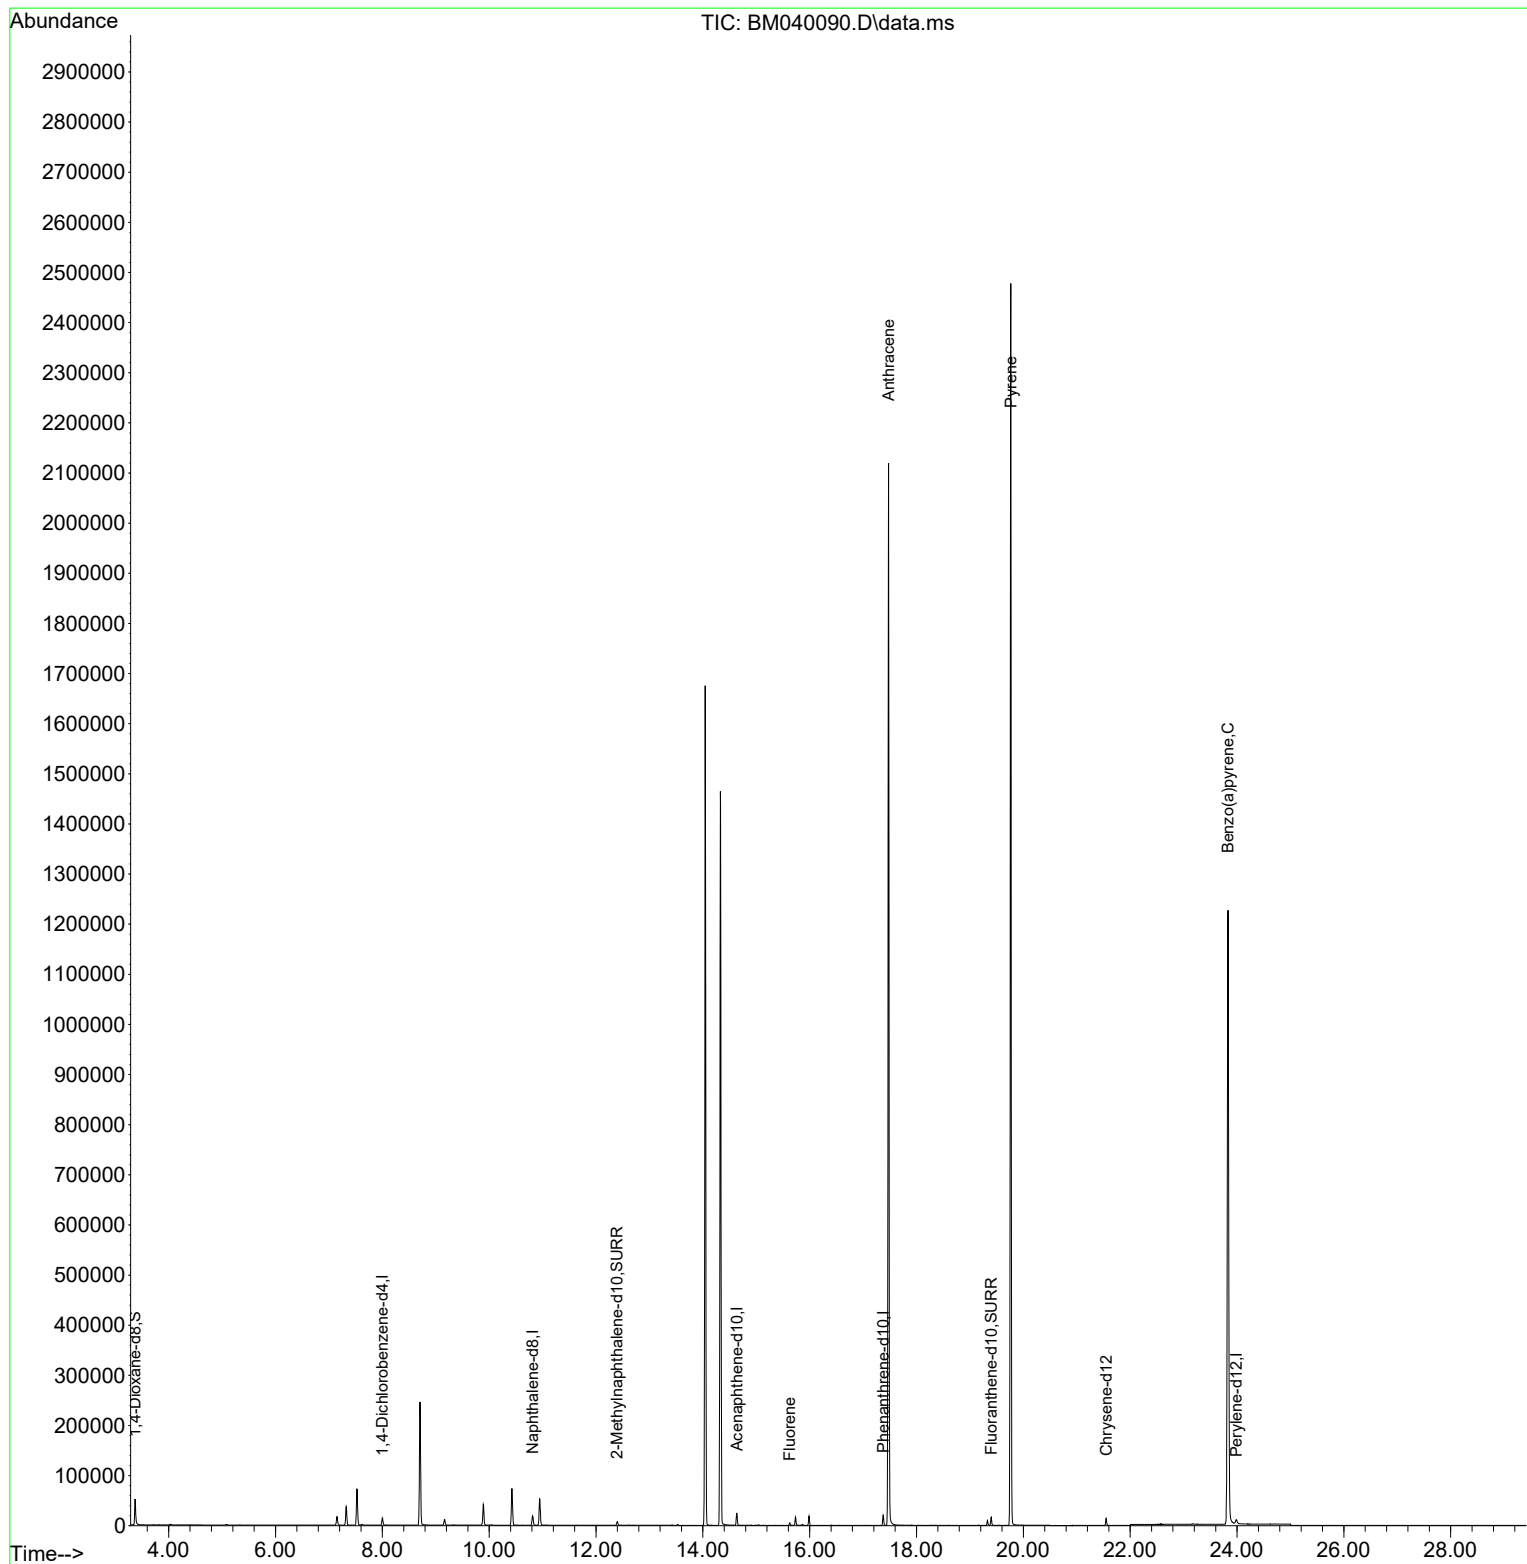


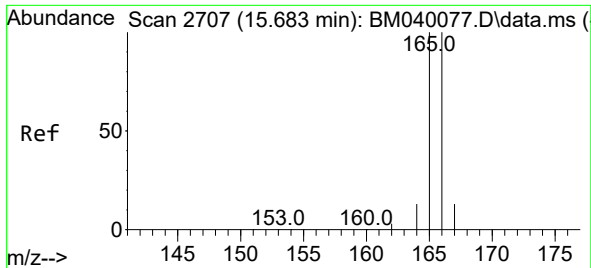

#12
 Fluorene
 Concen: 0.096 ng/ul
 RT: 15.627 min Scan# 21
 Delta R.T. -0.056 min
 Lab File: BM040090.D
 Acq: 31 May 2023 21:43




Instrument :
 BNA_M
 ClientSampleId :
 H0FP3RE


Tgt Ion:166 Resp: 4246
 Ion Ratio Lower Upper
 166 100
 165 7.0 79.8 119.8#
 167 34.2 11.2 16.8#

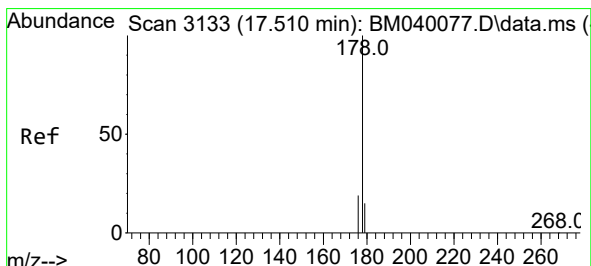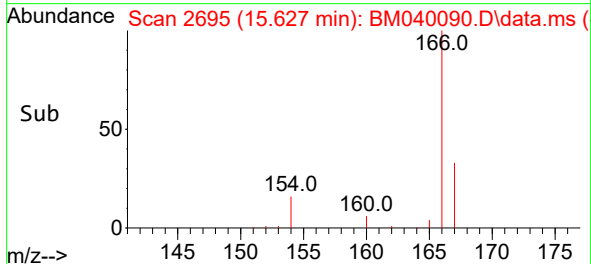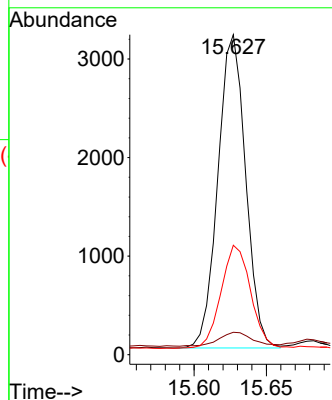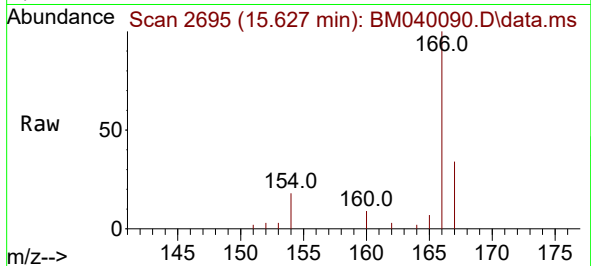

#16
 Anthracene
 Concen: 0.021 ng/ul
 RT: 17.476 min Scan# 3125
 Delta R.T. -0.034 min
 Lab File: BM040090.D
 Acq: 31 May 2023 21:43

Tgt Ion:178 Resp: 1119
 Ion Ratio Lower Upper
 178 100
 179 234.5 12.6 19.0#
 176 13.8 15.8 23.6#


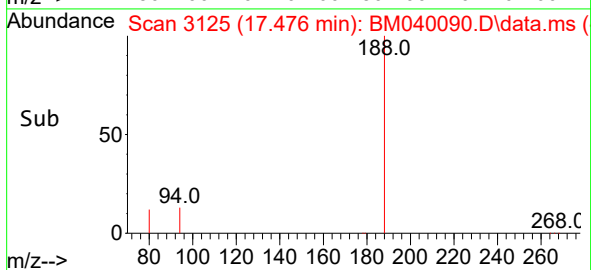
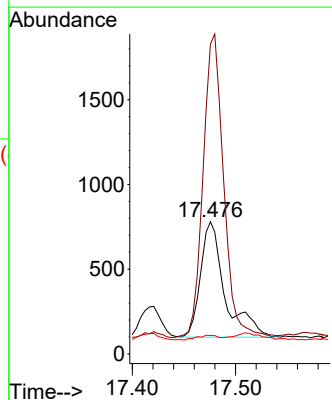
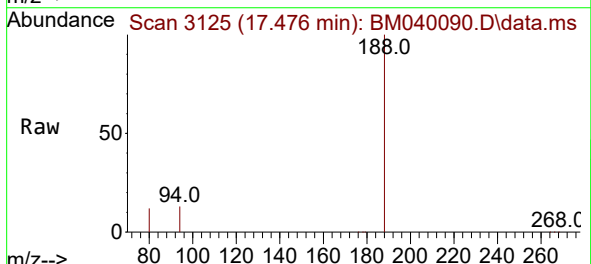


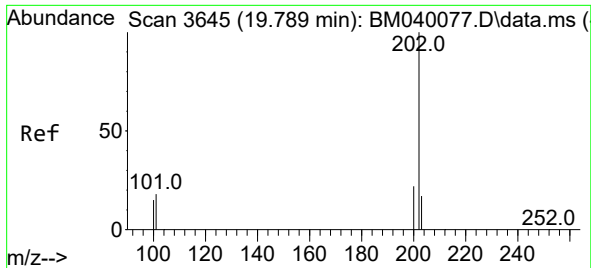

#20
Pyrene
Concen: 0.074 ng/ul
RT: 19.765 min Scan# 30
Delta R.T. -0.023 min
Lab File: BM040090.D
Acq: 31 May 2023 21:43

Instrument :
BNA_M
ClientSampleId :
H0FP3RE

Tgt Ion:202 Resp: 3835
Ion Ratio Lower Upper
202 100
101 145.4 14.7 22.1#
100 1038.7 12.2 18.2#

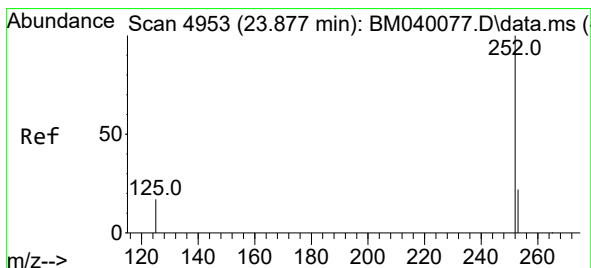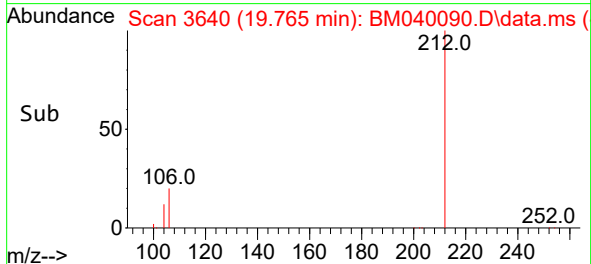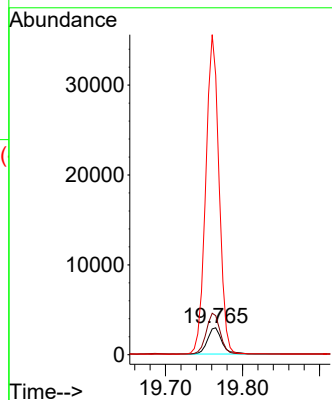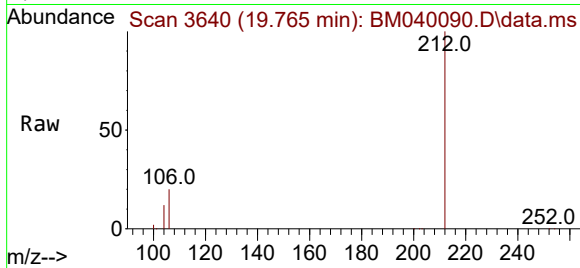

#26
Benzo(a)pyrene
Concen: 0.151 ng/ul
RT: 23.830 min Scan# 4937
Delta R.T. -0.047 min
Lab File: BM040090.D
Acq: 31 May 2023 21:43

Tgt Ion:252 Resp: 6440
Ion Ratio Lower Upper
252 100
253 38.7 21.0 31.4#
125 37.2 19.8 29.8#

