

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
 Data File : BM040097.D
 Acq On : 01 Jun 2023 01:57
 Operator : CG/JU
 Sample : 02851-06RE
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ9RE

Quant Time: Jun 01 02:28:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 31 18:20:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	7792	0.400	ng/u1	0.00
4) Naphthalene-d8	10.811	136	27860	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.633	164	13914	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.375	188	24996	0.400	ng/u1	0.00
17) Chrysene-d12	21.547	240	12387	0.400	ng/u1	0.00
23) Perylene-d12	23.979	264	12798	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	57612	6.015	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.395	152	15289	0.452	ng/u1	0.00
18) Fluoranthene-d10	19.398	212	22113	0.611	ng/u1	0.00
Target Compounds						
19) Fluoranthene	19.426	202	1241	0.023	ng/u1#	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053123\
Data File : BM040097.D
Acq On : 01 Jun 2023 01:57
Operator : CG/JU
Sample : 02851-06RE
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FJ9RE


Quant Time: Jun 01 02:28:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM053123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 18:20:24 2023
Response via : Initial Calibration

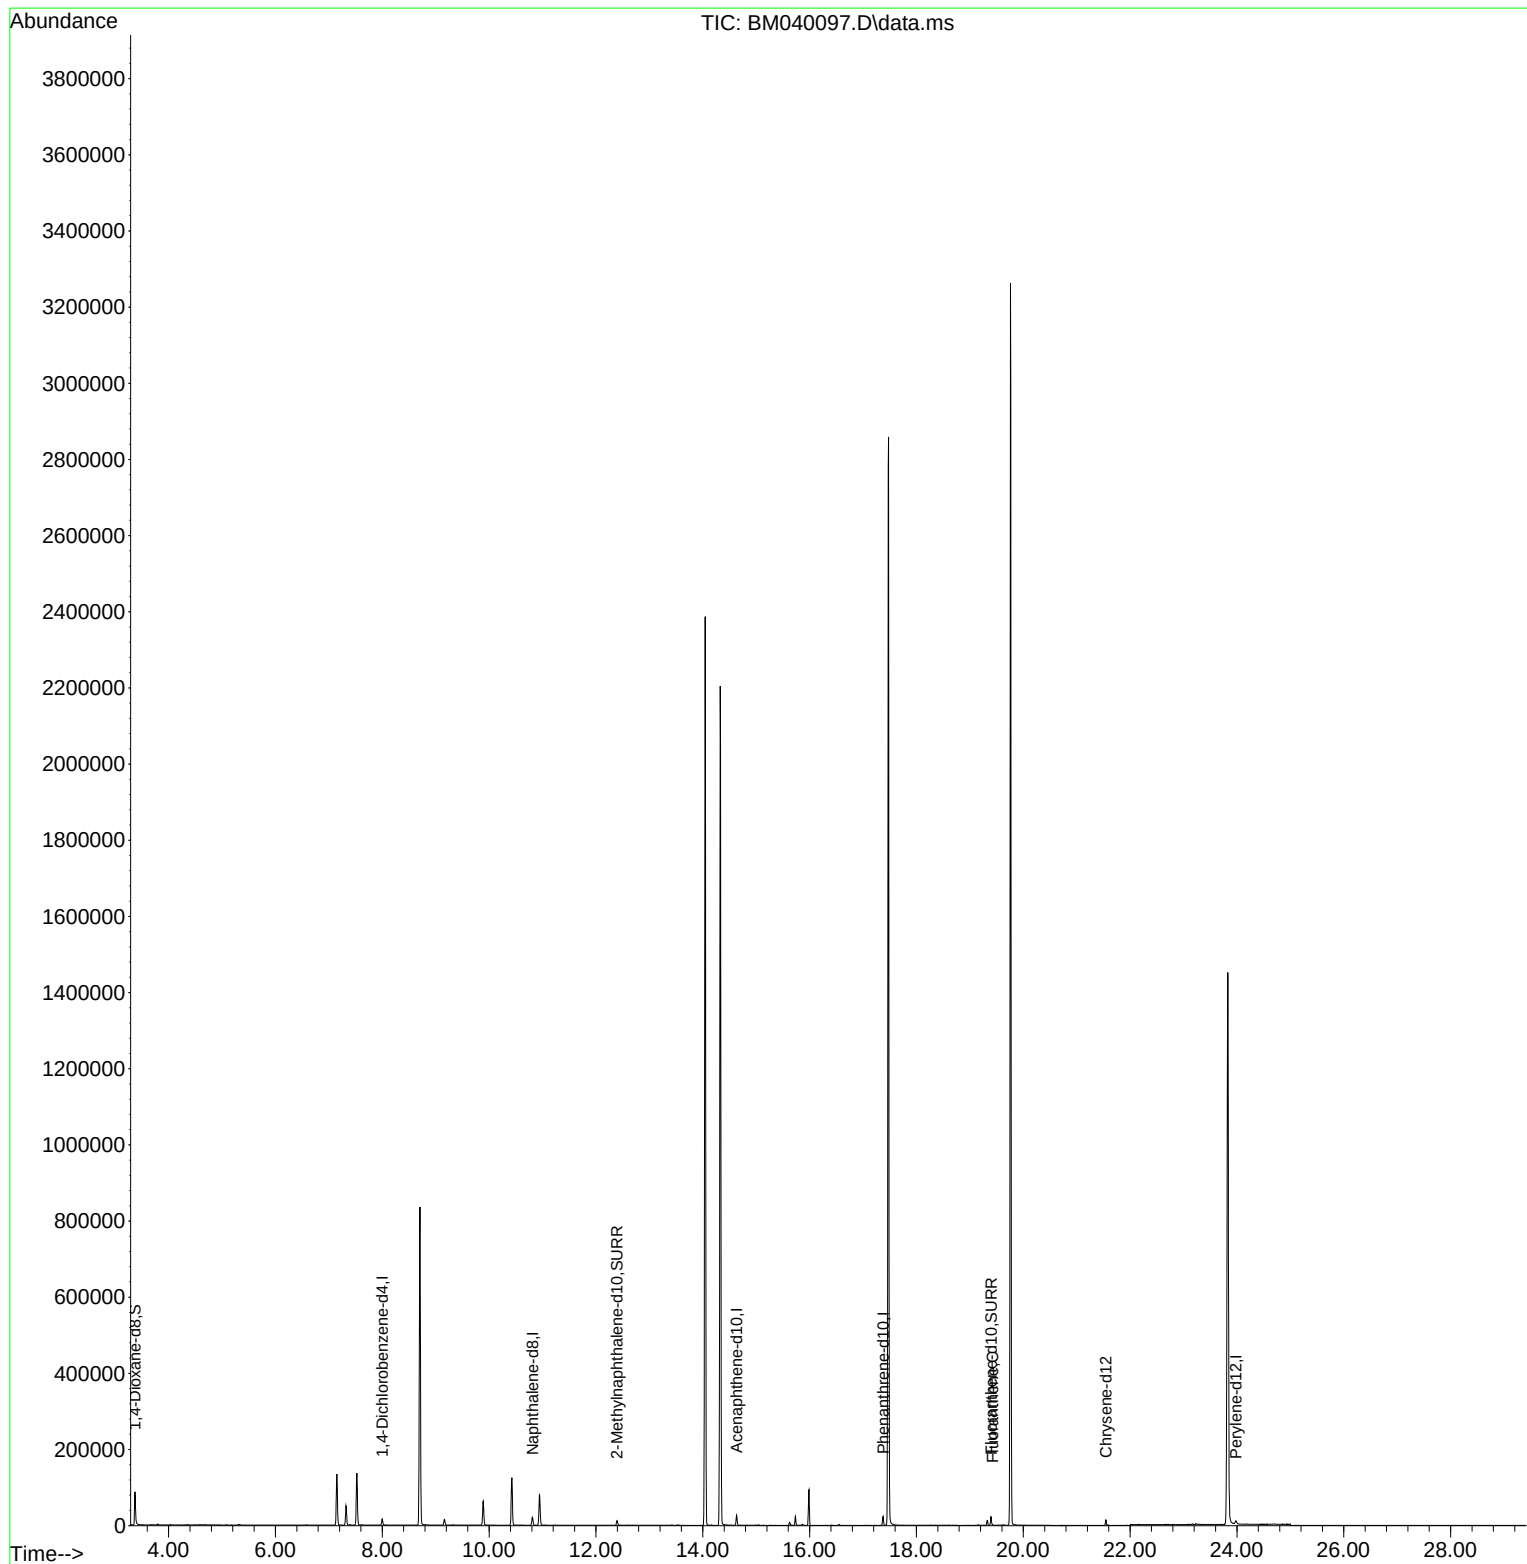

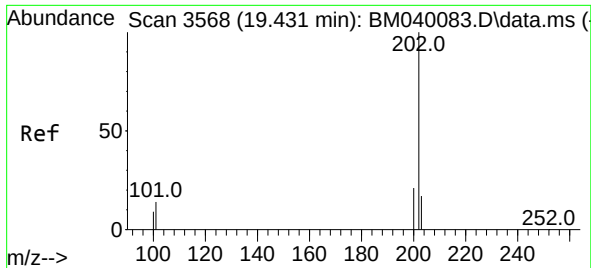

#19
 Fluoranthene
 Concen: 0.023 ng/ul
 RT: 19.426 min Scan# 31
 Delta R.T. -0.005 min
 Lab File: BM040097.D
 Acq: 01 Jun 2023 01:57

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ9RE

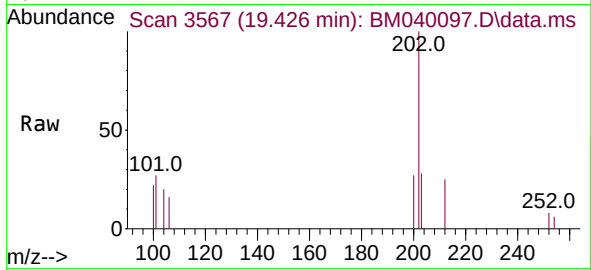

Tgt Ion	Ratio	Lower	Upper
202	100		
101	26.9	11.2	16.8#
100	21.6	8.6	12.8#

