

Data File : BM010356.D
Acq On : 01 Jun 2017 15:36
Operator : SJ/MA
Sample : I3163-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSE6

Quant Time: Jun 02 01:00:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 00:58:56 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	290080	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1049711	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	636991	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1493662	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2017088	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	2111487	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	21638	3.06	ng/uL	0.00
5) Phenol-d5	7.10	99	463154	21.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	280185	22.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	409214	23.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	349084	19.68	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	190968	24.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	212738	23.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	423728	23.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	1151	0.07	ng/ul	0.09
43) Dimethylphthalate-d6	13.97	166	1303366	24.63	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1572370	25.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	99698	12.59	ng/ul	0.00
57) Fluorene-d10	15.54	176	1193287	25.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	177137	16.74	ng/ul	0.00
70) Anthracene-d10	17.40	188	1891473	26.02	ng/ul	0.00
76) Pyrene-d10	19.69	212	2308195	27.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2402603	24.44	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.02	163	195556	3.76 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010356.D

Acq On : 01 Jun 2017 15:36

Operator : SJ/MA

Sample : I3163-02

Misc :

ALS Vial : 11 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHSE6


Quant Time: Jun 02 01:00:16 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 02 00:58:56 2017

Response via : Initial Calibration

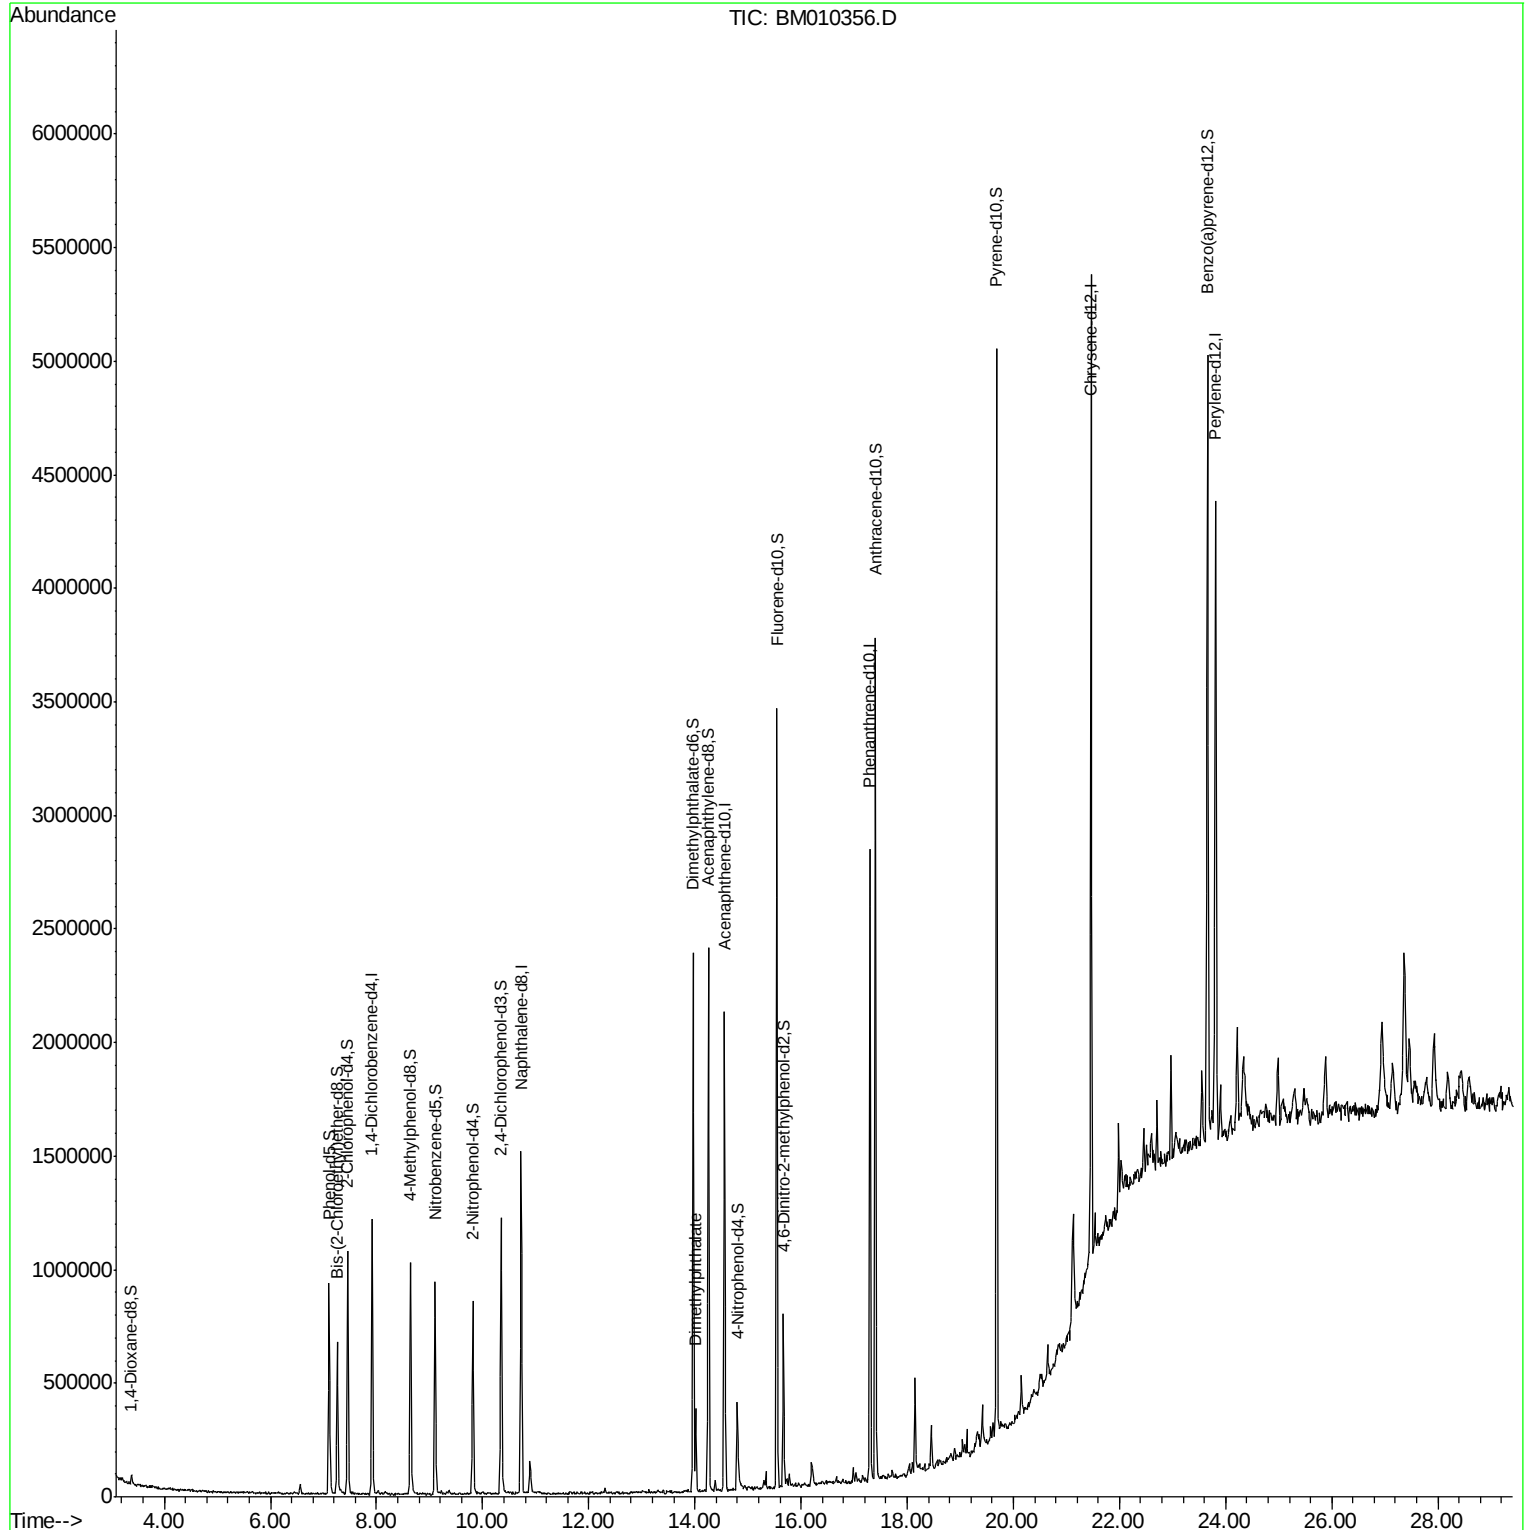

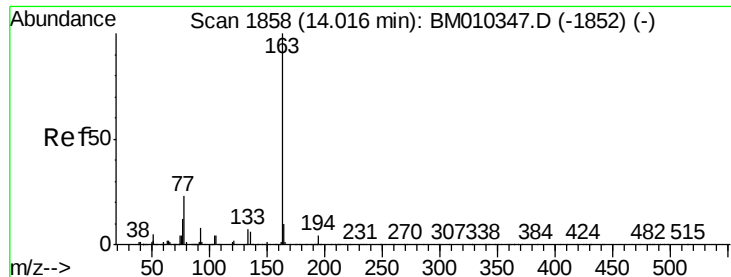

#44

Dimethylphthalate

Concen: 3.76 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. 0.00 min

Lab File: BM010356.D

Acq: 01 Jun 2017 15:36

Instrument :

BNA_M

ClientSampleId :

JHSE6


Tgt Ion:163 Resp: 195556

Ion Ratio Lower Upper

163 100

194 5.3 3.5 5.3

164 9.4 8.2 12.4

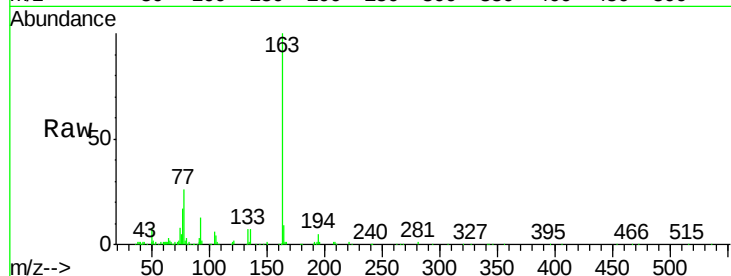

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

