

Data File : BM010368.D
Acq On : 01 Jun 2017 22:47
Operator : SJ/MA
Sample : I3163-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG5

Quant Time: Jun 02 01:57:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	363034	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1289446	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	786325	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1853629	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2734394	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2830726	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	19659	2.22	ng/uL	0.00
5) Phenol-d5	7.10	99	402930	14.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	234020	15.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	361055	16.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	325391	14.66	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	166388	17.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	194299	17.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	368331	16.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	17136	0.79	ng/ul	0.01
43) Dimethylphthalate-d6	13.97	166	1171423	17.93	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1323838	17.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	117483	12.02	ng/ul	0.00
57) Fluorene-d10	15.54	176	1009050	17.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	185815	14.15	ng/ul	0.00
70) Anthracene-d10	17.40	188	1520530	16.86	ng/ul	0.00
76) Pyrene-d10	19.69	212	2239522	19.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2556987	19.40	ng/ul	0.00

Target Compounds						Qvalue
44) Dimethylphthalate	14.02	163	338923	5.27	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010368.D

Acq On : 01 Jun 2017 22:47

Operator : SJ/MA

Sample : I3163-16

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHSG5


Quant Time: Jun 02 01:57:37 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 02 01:55:54 2017

Response via : Initial Calibration

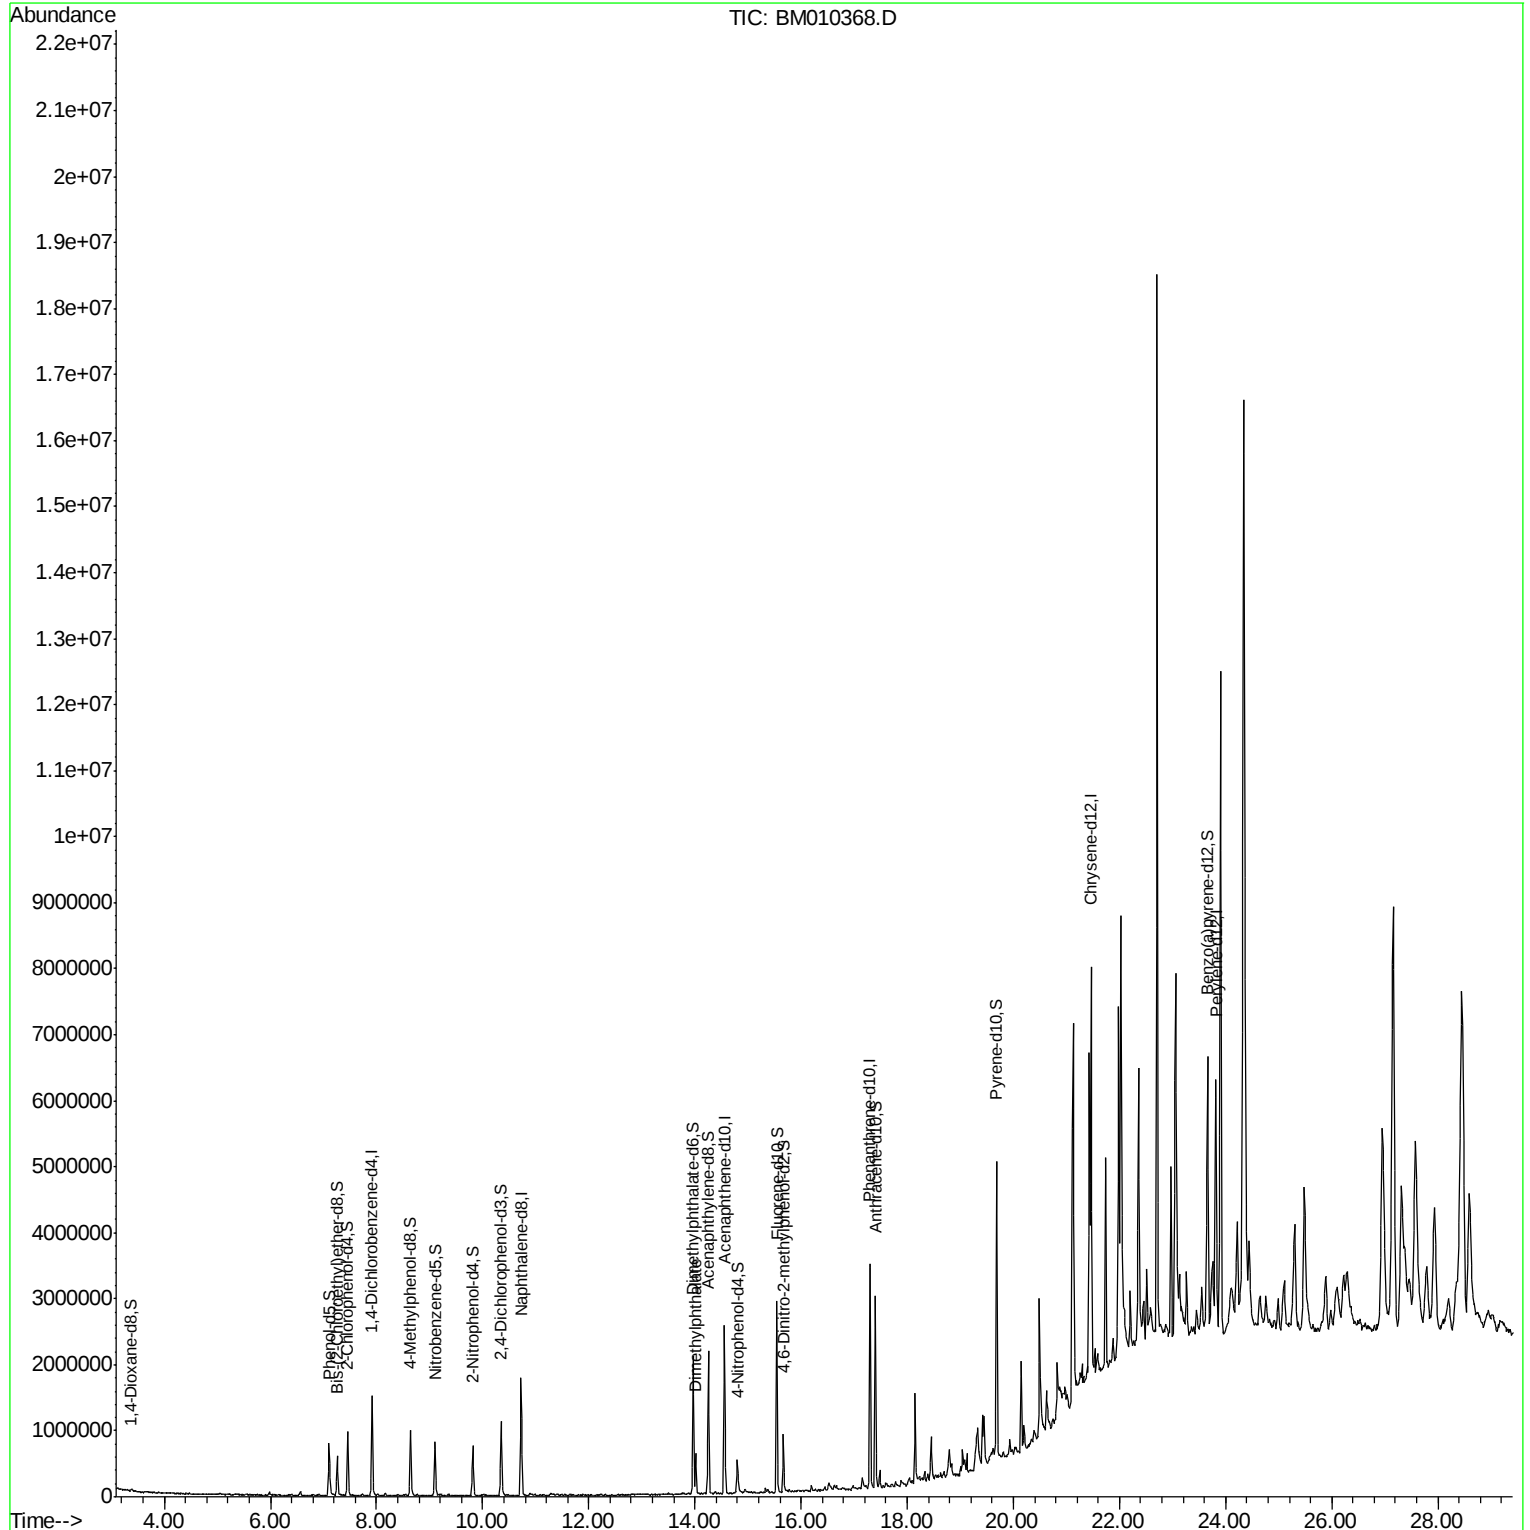

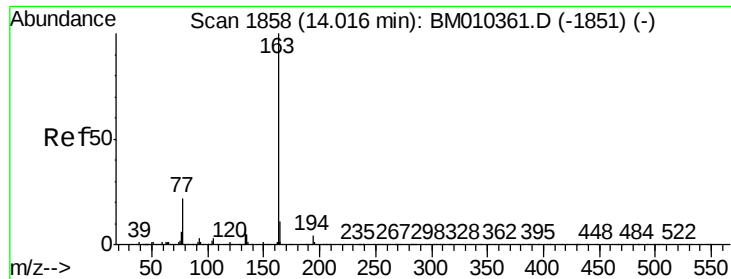

#44

Dimethylphthalate

Concen: 5.27 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.00 min

Lab File: BM010368.D

Acq: 01 Jun 2017 22:47

Instrument :

BNA_M

ClientSampleId :

JHSG5


Tgt Ion:163 Resp: 338923

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 8.7 8.2 12.4

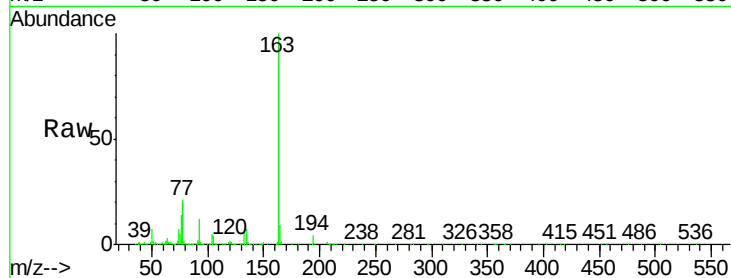

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

