

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010352.D
 Acq On : 01 Jun 2017 13:12
 Operator : SJ/MA
 Sample : I3163-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSF7

Quant Time: Jun 02 00:59:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 00:58:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	314327	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	1159285	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	706846	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1579198	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2106971	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2159629	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	25782	3.37	ng/uL	0.00
5) Phenol-d5	7.10	99	458469	19.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	278441	20.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	395568	20.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	301440	15.69	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	184811	21.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	223199	22.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	426227	21.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	235714	12.09	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1359310	23.15	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1576439	23.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	111424	12.68	ng/ul	0.00
57) Fluorene-d10	15.54	176	1175260	22.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	185334	16.57	ng/ul	0.00
70) Anthracene-d10	17.40	188	1835562	23.89	ng/ul	0.00
76) Pyrene-d10	19.69	212	2219702	25.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2311454	22.99	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.02	163	251747	4.359	ng/ul# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010352.D
Acq On : 01 Jun 2017 13:12
Operator : SJ/MA
Sample : I3163-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF7

Quant Time: Jun 02 00:59:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 00:58:56 2017
Response via : Initial Calibration

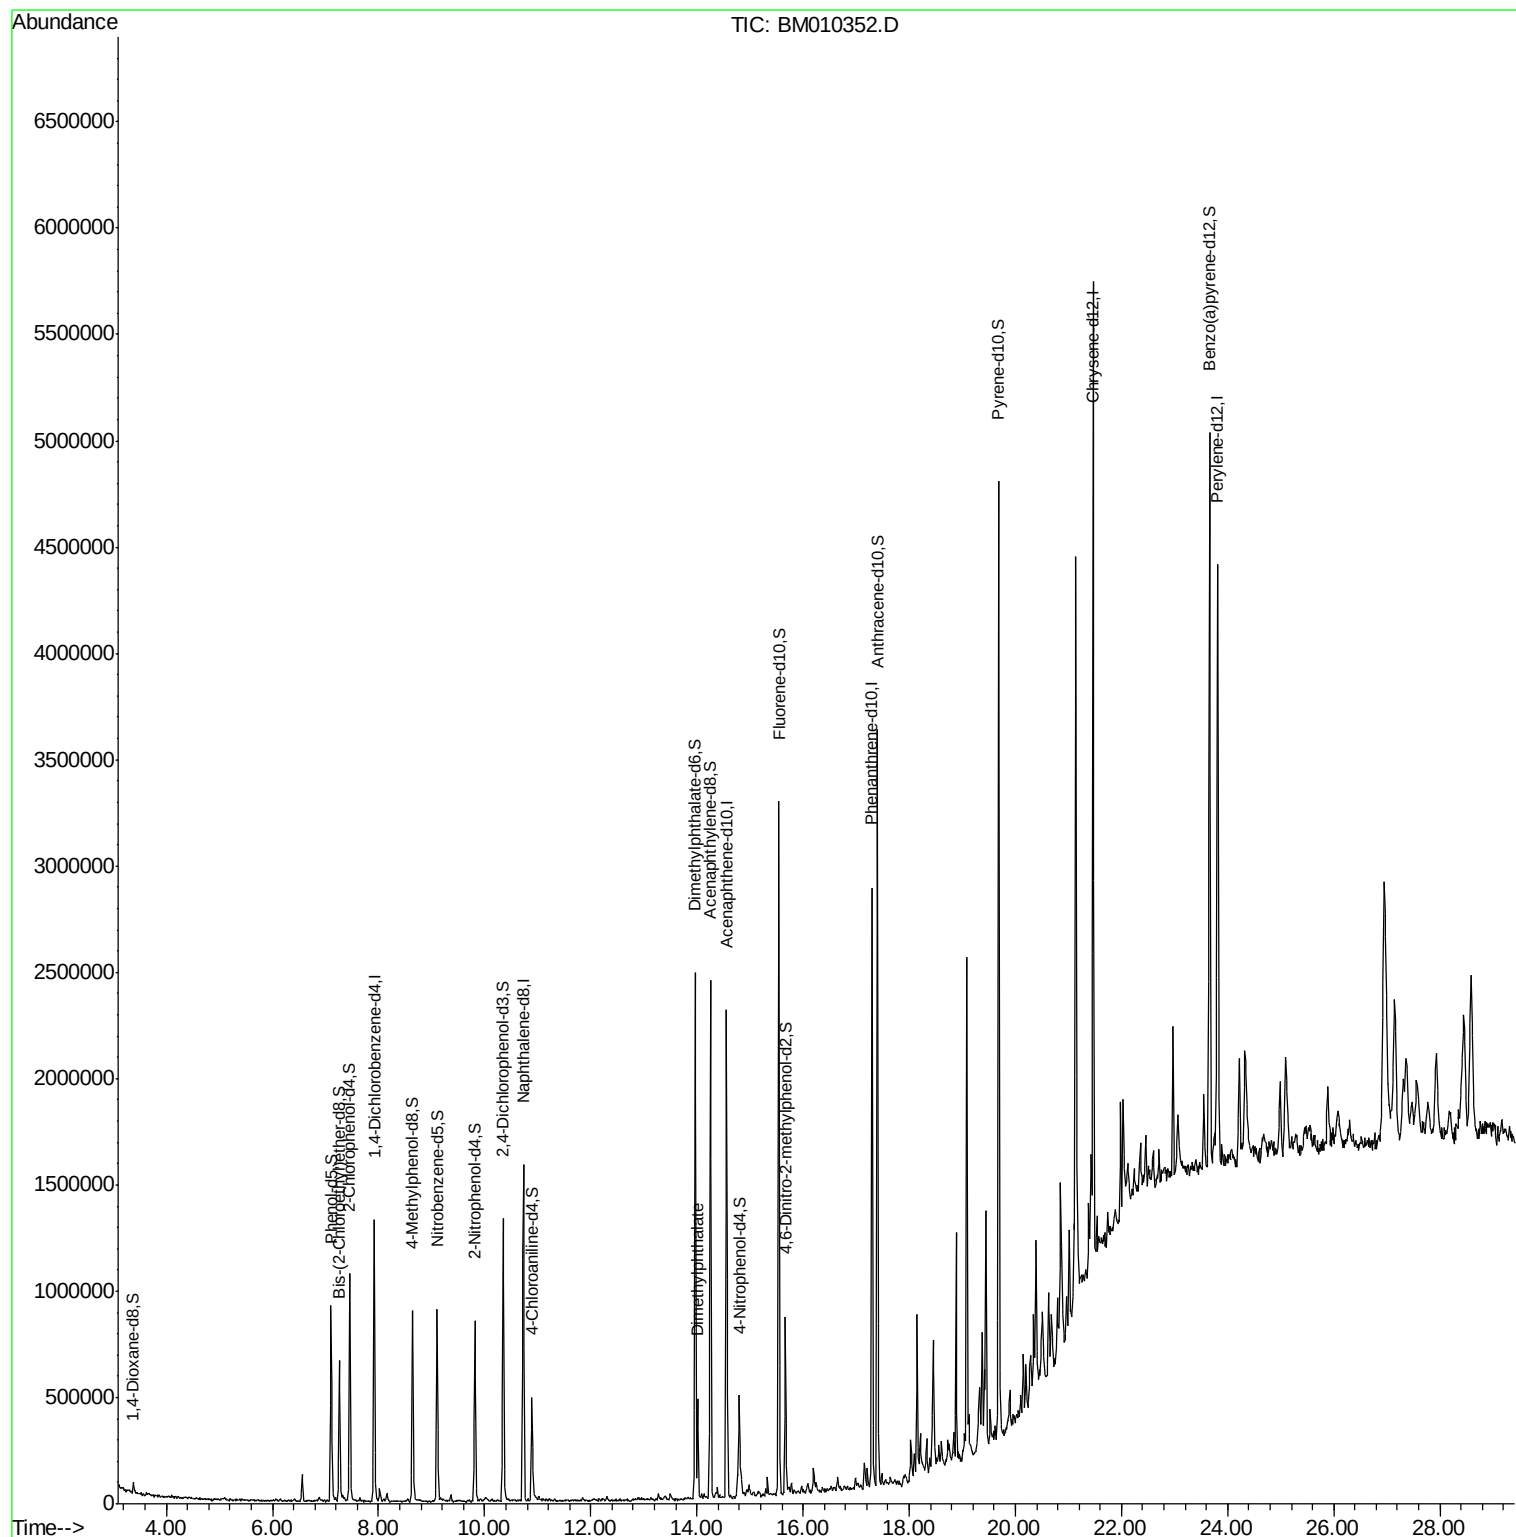

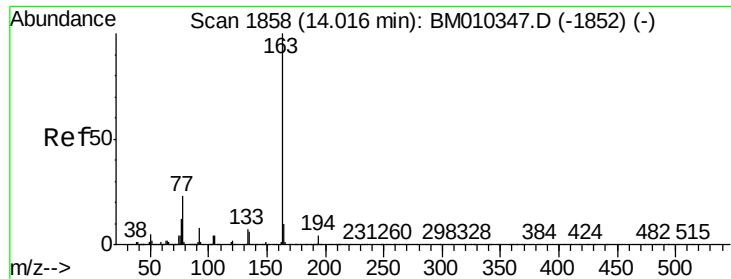

#44

Dimethylphthalate

Concen: 4.359 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.00 min

Lab File: BM010352.D

Acq: 01 Jun 2017 13:12

Instrument :

BNA_M

ClientSampleId :

JHSF7

Tgt Ion:163 Resp: 251747

Ion Ratio Lower Upper

163 100

194 3.2 3.5 5.3#

164 9.5 8.2 12.4

