

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010357.D
 Acq On : 01 Jun 2017 16:12
 Operator : SJ/MA
 Sample : I3163-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSE5

Quant Time: Jun 02 01:00:23 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 00:58:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	272337	20.00	ng/ul	0.00
18) Naphthalene-d8	10.73	136	974125	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	601358	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1378790	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	1878645	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	1968363	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.38	96	23554	3.55	ng/uL	0.00
5) Phenol-d5	7.10	99	412520	19.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	251782	21.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	367025	22.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	309848	18.61	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	169975	23.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	186471	22.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	374173	22.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	118103	7.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1227009	24.56	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1412244	24.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.79	143	109267	14.62	ng/ul	0.00
57) Fluorene-d10	15.54	176	1080253	24.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	170951	17.50	ng/ul	0.00
70) Anthracene-d10	17.40	188	1713517	25.54	ng/ul	0.00
76) Pyrene-d10	19.69	212	2107072	27.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2230194	24.34	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.02	163	198285	4.035	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010357.D
Acq On : 01 Jun 2017 16:12
Operator : SJ/MA
Sample : I3163-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSE5

Quant Time: Jun 02 01:00:23 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 00:58:56 2017
Response via : Initial Calibration

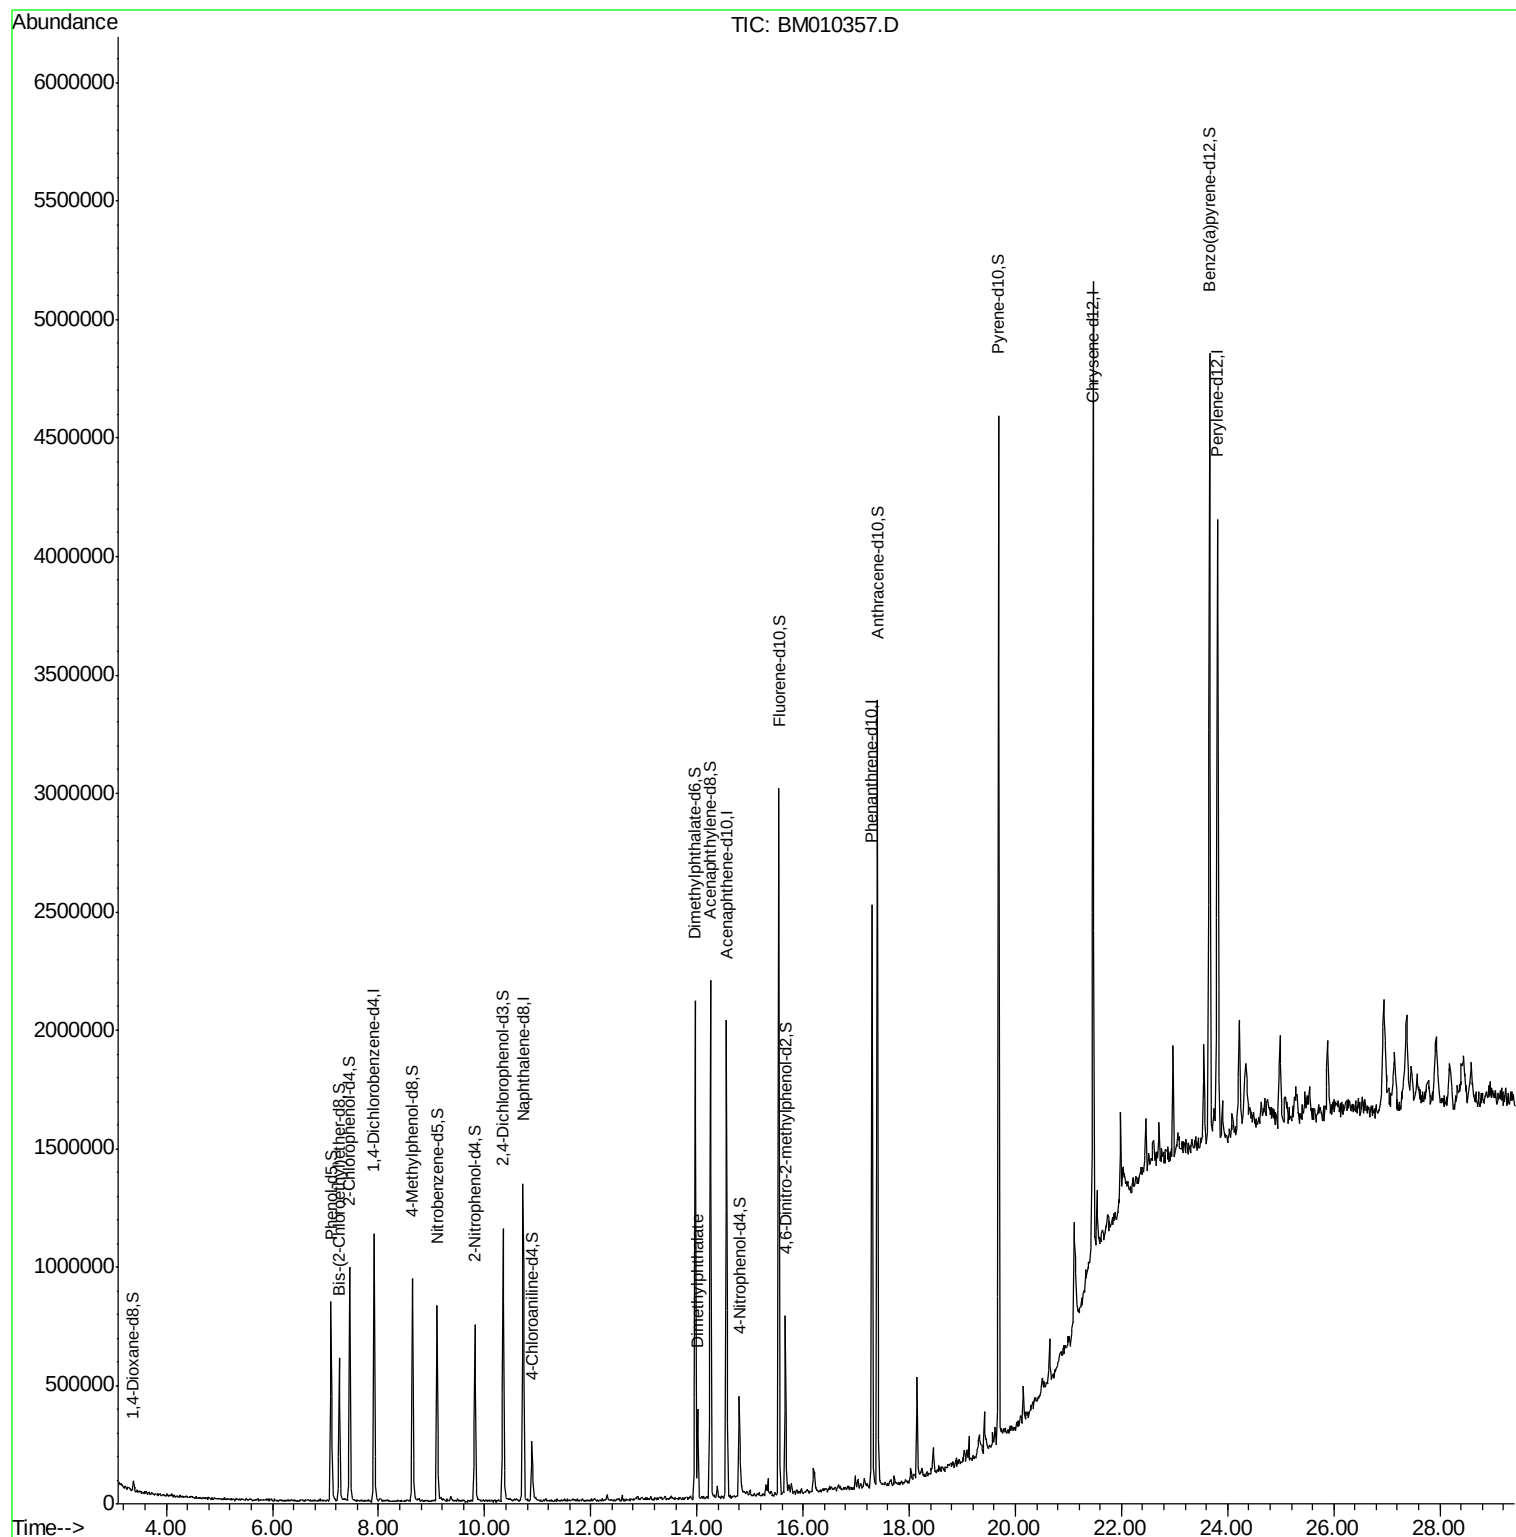

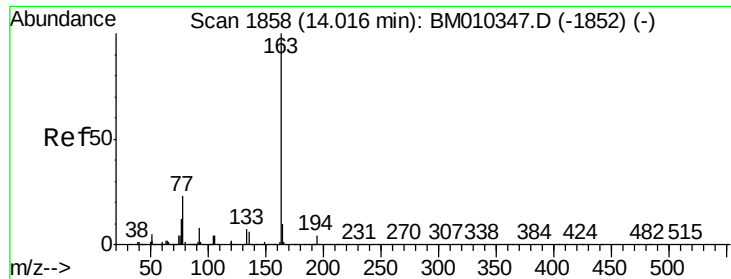

#44

Dimethylphthalate

Concen: 4.035 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.00 min

Lab File: BM010357.D

Acq: 01 Jun 2017 16:12

Instrument :

BNA_M

ClientSampleId :

JHSE5


Tgt Ion:163 Resp: 198285

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 9.5 8.2 12.4

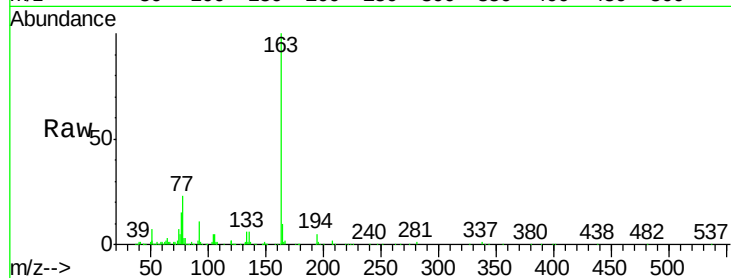

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

