

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010362.D
 Acq On : 01 Jun 2017 19:12
 Operator : SJ/MA
 Sample : I3163-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSF5

Quant Time: Jun 02 01:56:36 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	357157	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1308451	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	803953	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1815857	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2528177	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2594377	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	29188	3.35	ng/uL	0.00
5) Phenol-d5	7.10	99	480322	17.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	299585	19.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	432636	20.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	309699	14.18	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	202078	21.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	229418	20.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	436421	19.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	200670	9.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1394768	20.88	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1657657	21.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.79	143	104536	10.46	ng/ul	0.00
57) Fluorene-d10	15.54	176	1240218	21.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	186166	14.47	ng/ul	0.00
70) Anthracene-d10	17.40	188	1929900	21.84	ng/ul	0.00
76) Pyrene-d10	19.69	212	2395907	22.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2500756	20.70	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.02	163	248068	3.776 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010362.D
Acq On : 01 Jun 2017 19:12
Operator : SJ/MA
Sample : I3163-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF5

Quant Time: Jun 02 01:56:36 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration

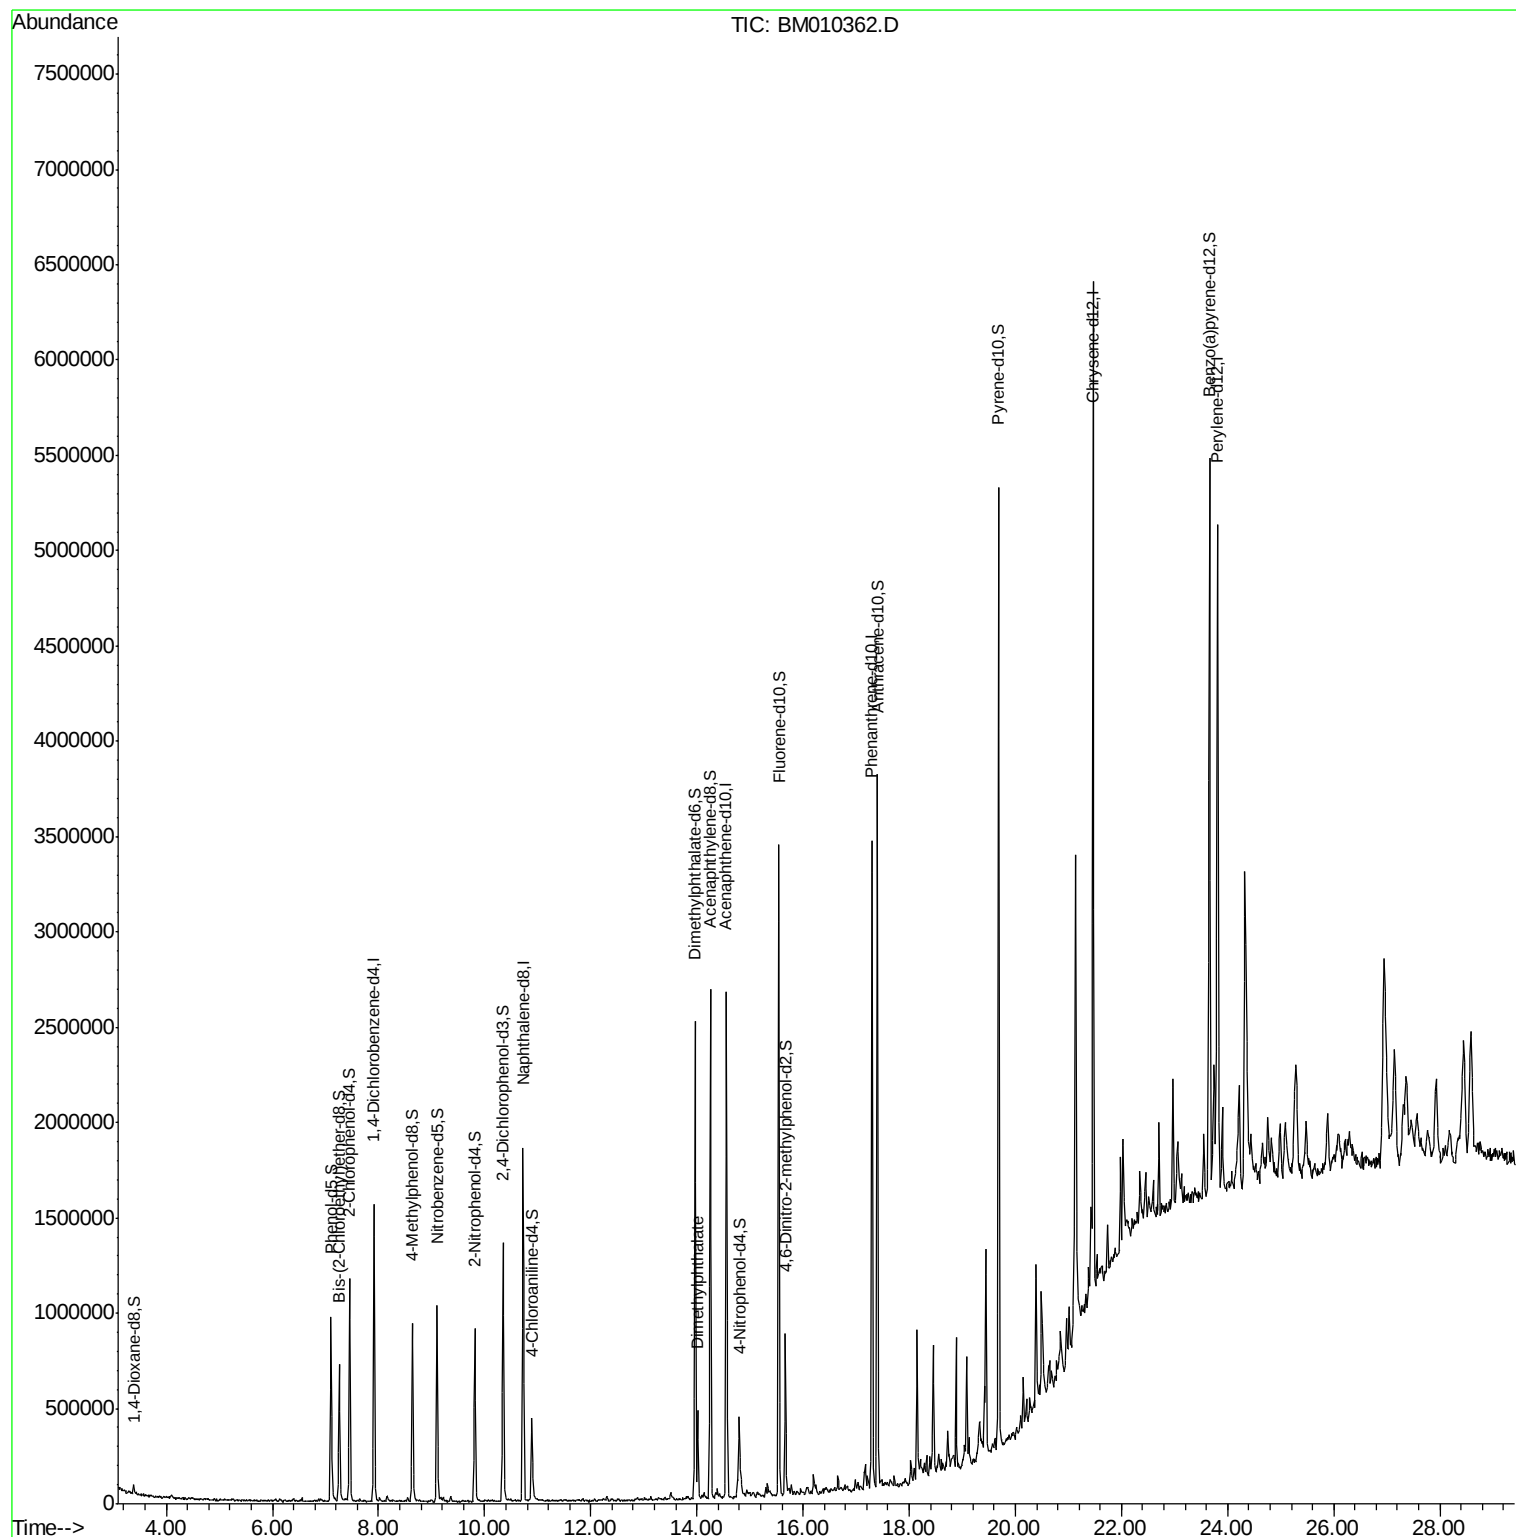

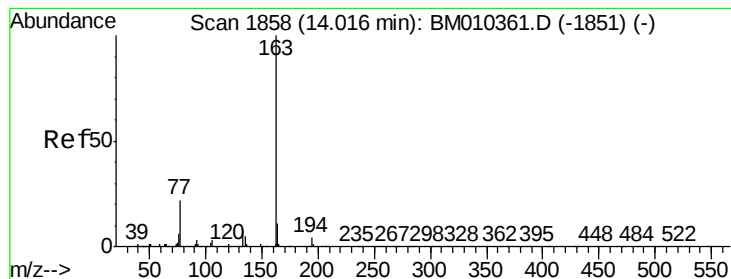

#44

Dimethylphthalate

Concen: 3.776 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.00 min

Lab File: BM010362.D

Acq: 01 Jun 2017 19:12

Instrument :

BNA_M

ClientSampleId :

JHSF5

Tgt Ion:163 Resp: 248068

Ion Ratio Lower Upper

163 100

194 5.2 3.5 5.3

164 10.6 8.2 12.4

