

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010365.D
 Acq On : 01 Jun 2017 20:59
 Operator : SJ/MA
 Sample : I3163-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSG1

Quant Time: Jun 02 03:13:46 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	373266	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1339129	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	802922	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1899126	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2733554	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2817566	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.38	96	15485	1.70	ng/uL	0.00
5) Phenol-d5	7.10	99	370885	13.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	223733	14.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	331536	14.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	246962	10.82	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	154570	15.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	183335	16.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	359355	15.39	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1172997	17.58	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1304877	16.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	89232	8.94	ng/ul	0.00
57) Fluorene-d10	15.54	176	1001015	17.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	173762	12.92	ng/ul	0.00
70) Anthracene-d10	17.40	188	1501509	16.25	ng/ul	0.00
76) Pyrene-d10	19.69	212	2016115	17.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2129262	16.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.01	163	235328	3.587	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010365.D
Acq On : 01 Jun 2017 20:59
Operator : SJ/MA
Sample : I3163-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG1

Quant Time: Jun 02 03:13:46 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration

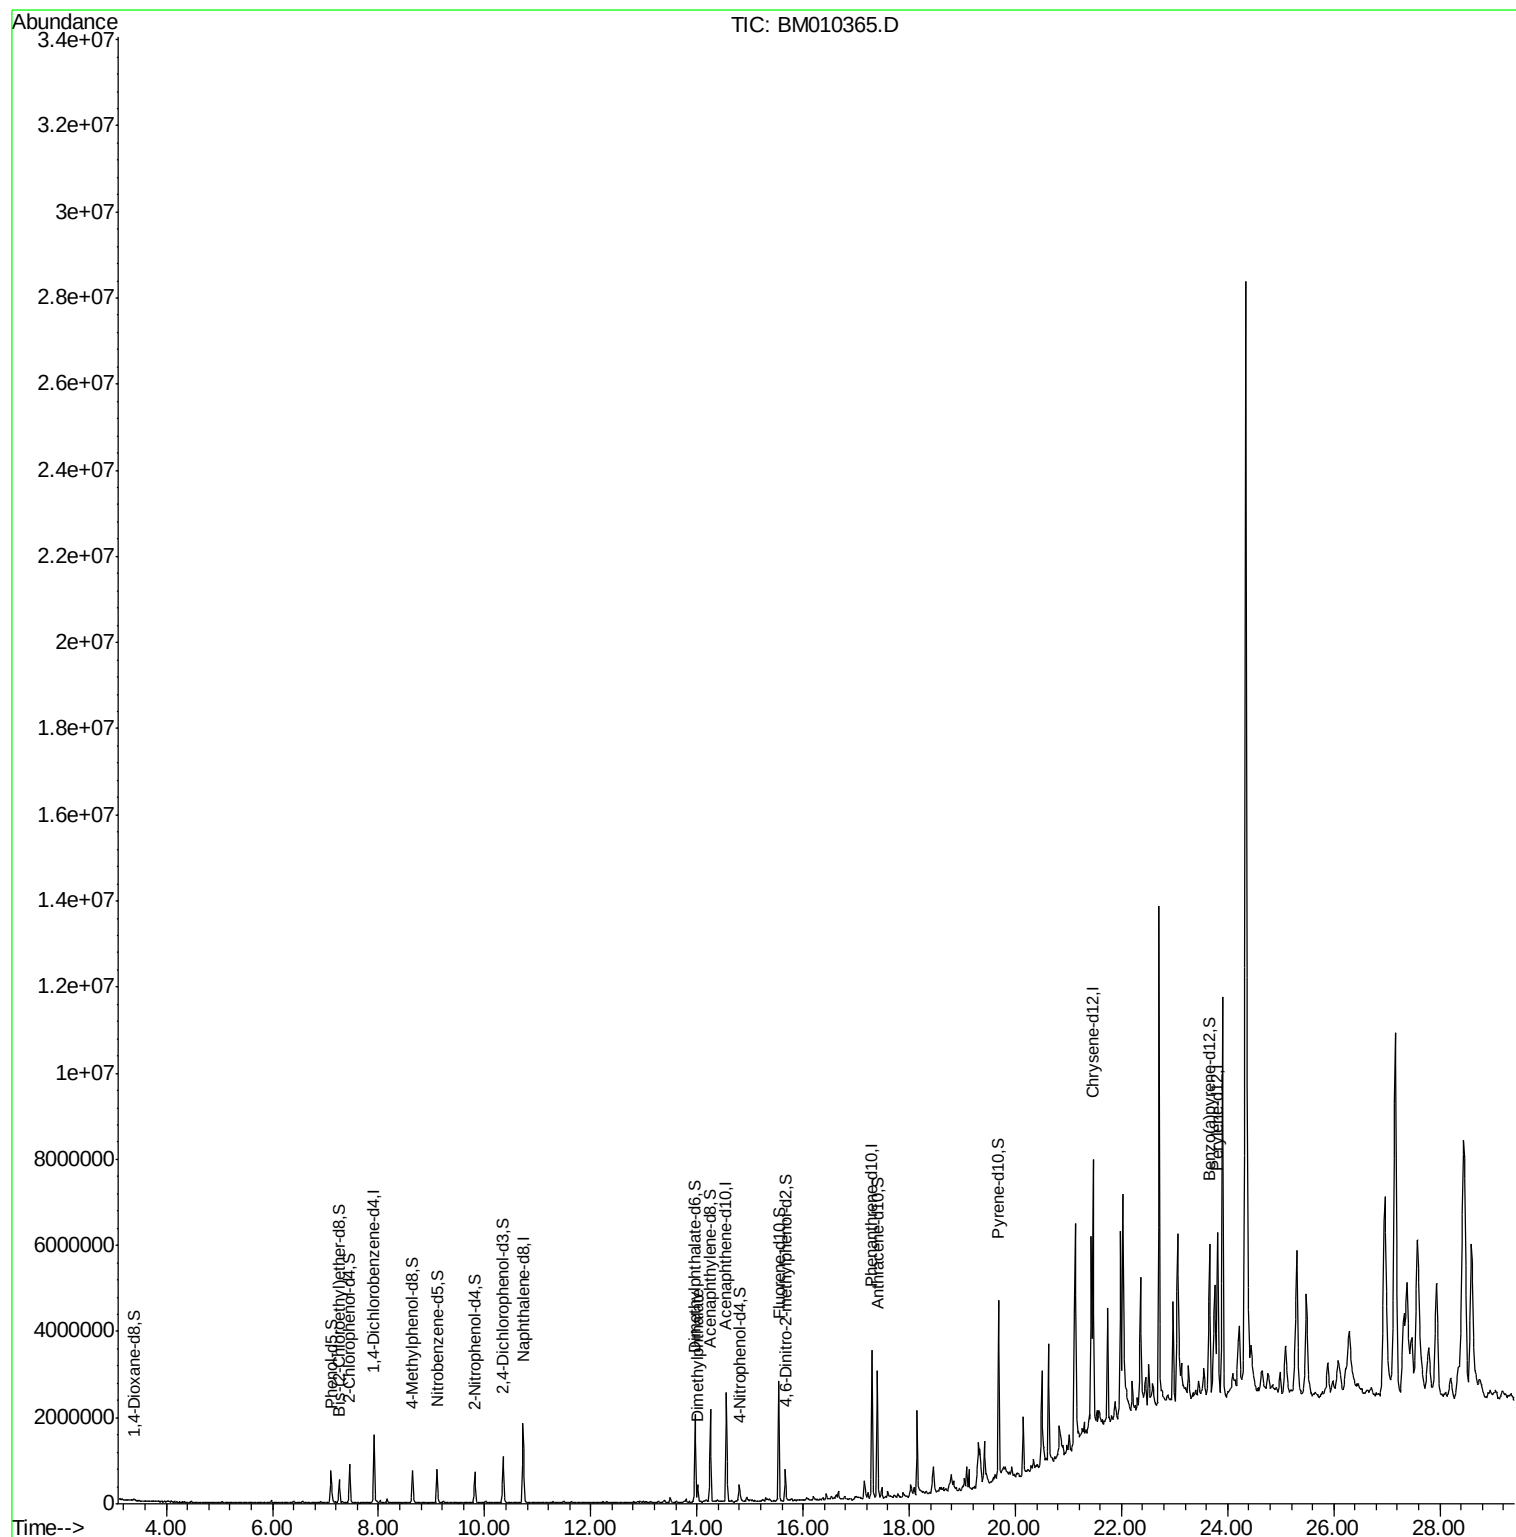

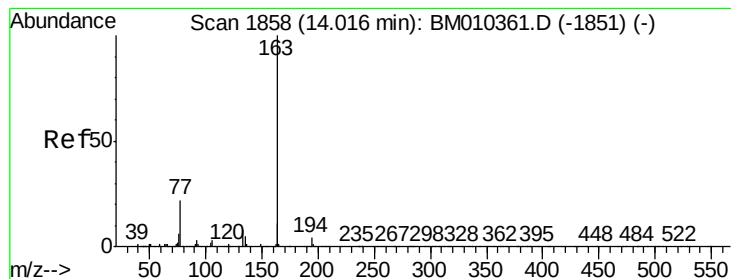

#44

Dimethylphthalate

Concen: 3.587 ng/ul

RT: 14.01 min Scan# 1857

Delta R.T. -0.01 min

Lab File: BM010365.D

Acq: 01 Jun 2017 20:59

Instrument :

BNA_M

ClientSampleId :

JHSG1

Tgt Ion:163 Resp: 235328

Ion Ratio Lower Upper

163 100

194 3.5 3.5 5.3#

164 11.0 8.2 12.4

